

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092519\
 Data File : BM022779.D
 Acq On : 25 Sep 2019 19:43
 Operator : JU
 Sample : K4997-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 WC-12-091919

Manual Integrations
 APPROVED

mohammad
 9/26/2019 3:55:07 PM

Quant Time: Sep 26 06:45:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM092019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 20 16:34:01 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	245956	20.00	ng	0.00
21) Naphthalene-d8	10.61	136	866279	20.00	ng	-0.01
39) Acenaphthene-d10	14.45	164	465507	20.00	ng	-0.01
64) Phenanthrene-d10	17.19	188	837391	20.00	ng	0.00
76) Chrysene-d12	21.37	240	835142	20.00	ng	-0.01
87) Perylene-d12	23.64	264	1038118	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.40	112	2075090	133.81	ng	0.00
7) Phenol-d6	6.99	99	2709416	136.02	ng	0.00
23) Nitrobenzene-d5	8.97	82	1553036	99.52	ng	0.00
42) 2,4,6-Tribromophenol	15.94	330	888652	152.92	ng	0.00
45) 2-Fluorobiphenyl	13.08	172	3607283	106.71	ng	0.00
79) Terphenyl-d14	19.82	244	4309091	99.91	ng	0.00
Target Compounds						
49) Acenaphthylene	14.17	152	112449	2.644	ng	Qvalue 100
50) Dimethylphthalate	13.91	163	227445	6.761	ng	99
71) Phenanthrene	17.23	178	399914	8.464	ng	100
72) Anthracene	17.32	178	101825	2.224	ng	98
75) Fluoranthene	19.24	202	545216	10.226	ng	99
78) Pyrene	19.61	202	635165	11.605	ng	100
81) Benzo(a)anthracene	21.35	228	299298	5.530	ng	95
83) Chrysene	21.40	228	345659	6.587	ng	97
86) Indeno(1,2,3-cd)pyrene	25.94	276	204835	3.270	ng	# 100
88) Benzo(b)fluoranthene	22.96	252	372442m	5.925	ng	
89) Benzo(k)fluoranthene	23.00	252	137872m	2.211	ng	
90) Benzo(a)pyrene	23.54	252	301695	5.209	ng	98
92) Benzo(a,h,i)perylene	26.65	276	217649	3.782	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092519\
Data File : BM022779.D
Acq On : 25 Sep 2019 19:43
Operator : JU
Sample : K4997-09
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
WC-12-091919

Manual Integrations
APPROVED

mohammad
9/26/2019 3:55:07 PM

Quant Time: Sep 26 06:45:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM092019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 20 16:34:01 2019
Response via : Initial Calibration

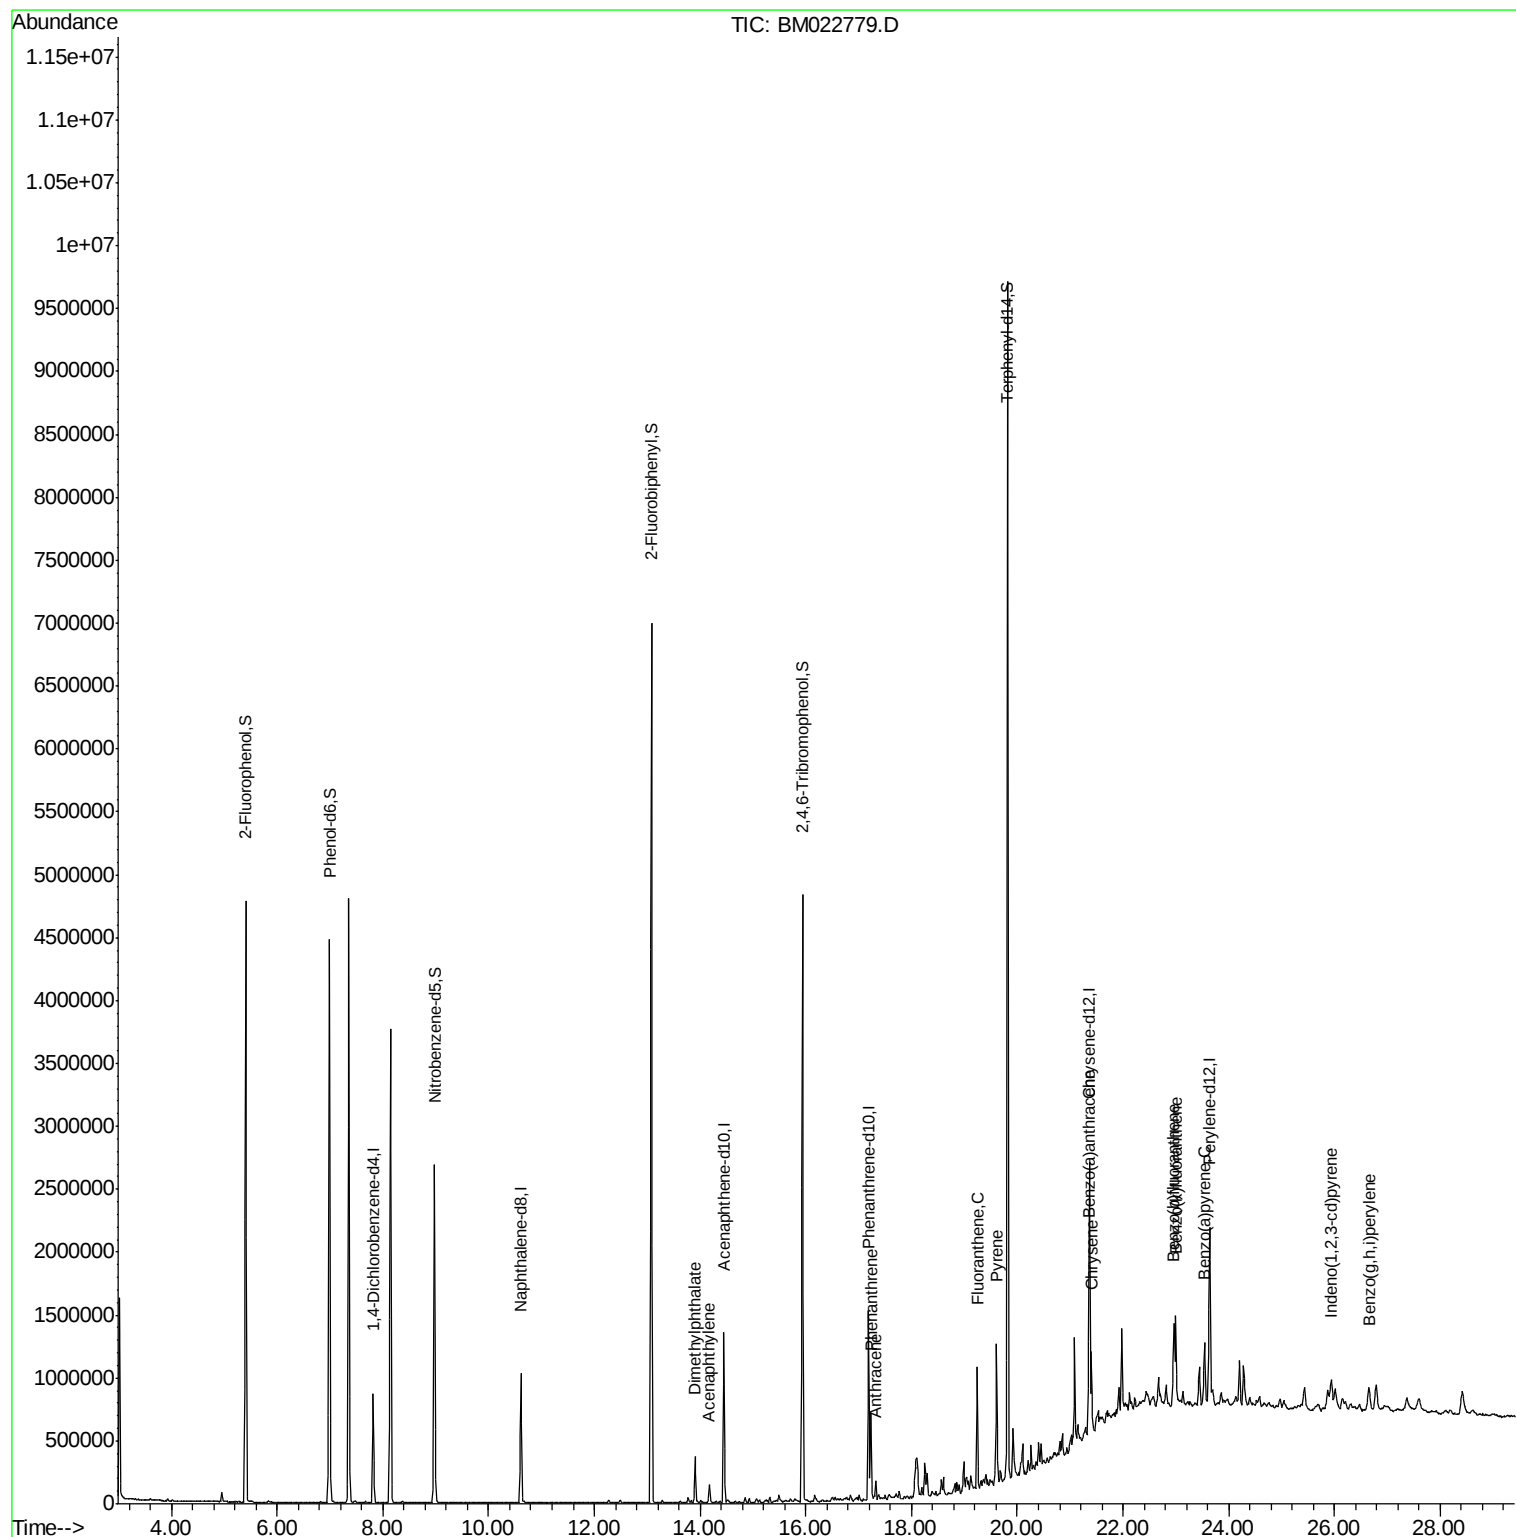

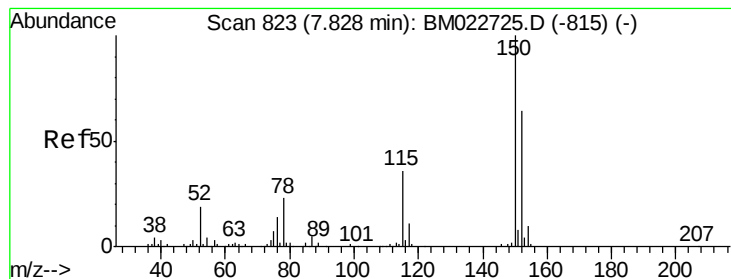





#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.82 min Scan# 822
 Delta R.T. -0.01 min
 Lab File: BM022779.D
 Acq: 25 Sep 2019 19:43

Instrument :
 BNA_M
 ClientSampleId :
 WC-12-091919

Tot Ion	Ratio	Lower	Upper
152	100		
150	157.2	124.5	186.7
115	56.4	45.0	67.4




Manual Integrations
 APPROVED


mohammad
 9/26/2019 3:55:07 PM

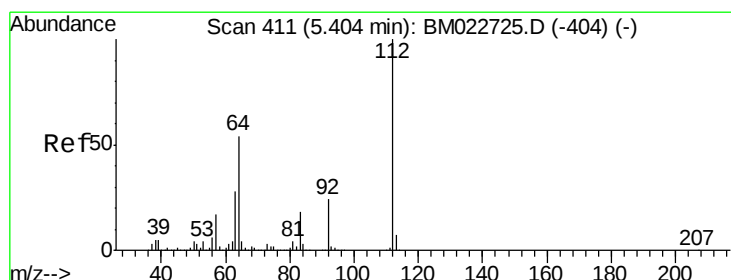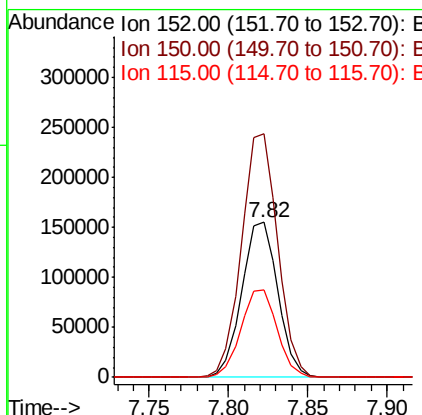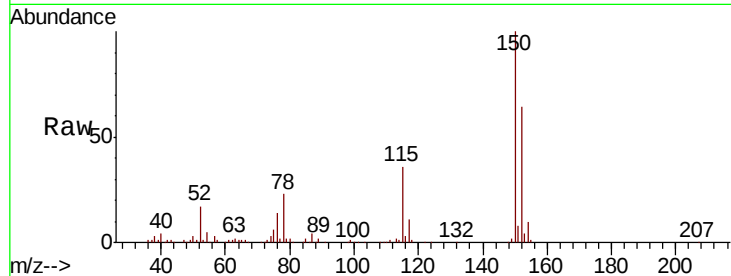

#5
 2-Fluorophenol
 Concen: 133.805 ng
 RT: 5.40 min Scan# 411
 Delta R.T. 0.00 min
 Lab File: BM022779.D
 Acq: 25 Sep 2019 19:43

Tgt Ion	Ratio	Lower	Upper
112	100		
64	53.3	43.4	65.2
63	27.4	22.1	33.1

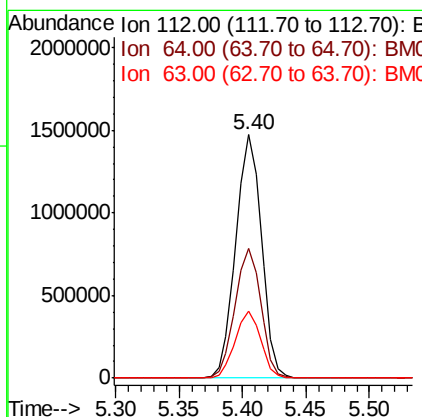

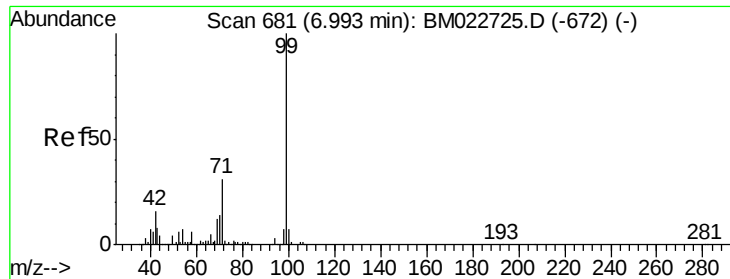

#7

Phenol-d6

Concen: 136.024 ng

RT: 6.99 min Scan# 681

Delta R.T. 0.00 min

Lab File: BM022779.D

Acq: 25 Sep 2019 19:43

Instrument :

BNA_M

ClientSampleId :

WC-12-091919

Tot Ion: 99 Resp: 2709416

Ion Ratio Lower Upper

99 100

42 15.5 13.0 19.4


71 31.0 24.7 37.1

Manual Integrations

APPROVED

mohammad




9/26/2019 3:55:07 PM

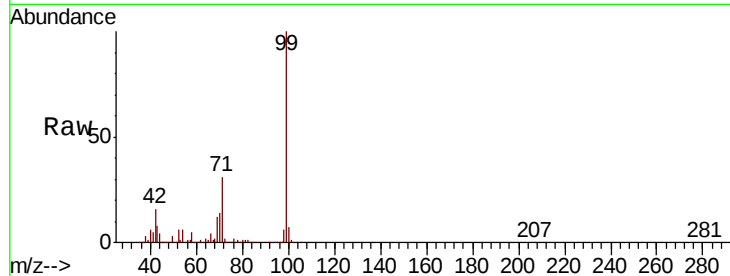

Abundance Ion 99.00 (98.70 to 99.70): BM022779.D (-664) (-)

Ion 42.00 (41.70 to 42.70): BM022779.D (-664) (-)

Ion 71.00 (70.70 to 71.70): BM022779.D (-664) (-)

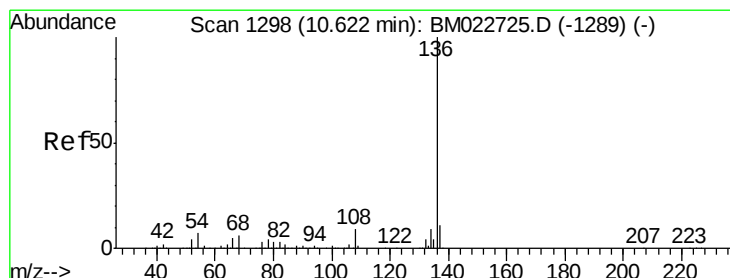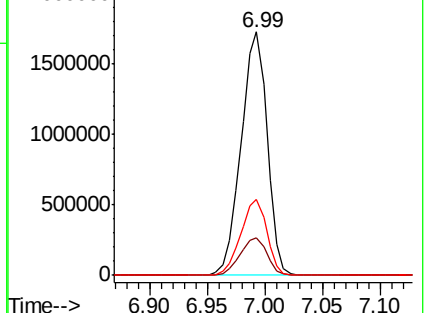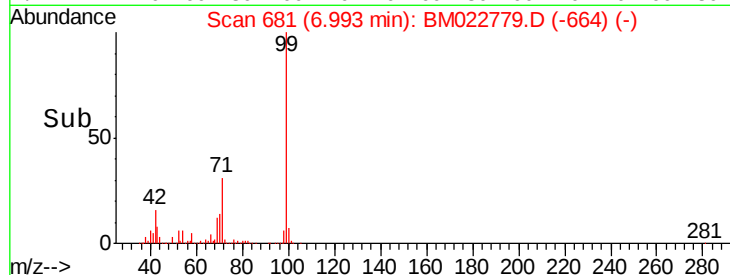

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.61 min Scan# 1296

Delta R.T. -0.01 min

Lab File: BM022779.D

Acq: 25 Sep 2019 19:43

Tgt Ion: 136 Resp: 866279


Ion Ratio Lower Upper

136 100

137 10.9 8.6 13.0

54 7.2 6.0 9.0

68 5.8 4.9 7.3


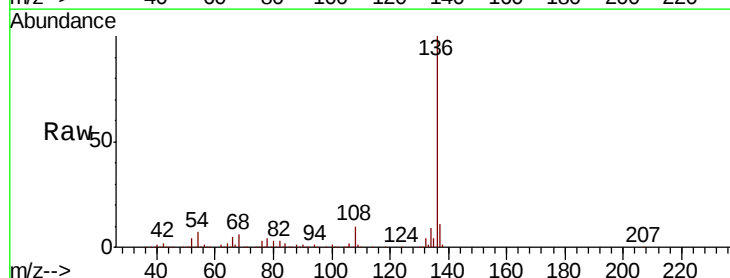



Abundance Ion 136.00 (135.70 to 136.70): BM022779.D (-1281) (-)

Ion 137.00 (136.70 to 137.70): BM022779.D (-1281) (-)

Ion 54.00 (53.70 to 54.70): BM022779.D (-1281) (-)

Ion 68.00 (67.70 to 68.70): BM022779.D (-1281) (-)

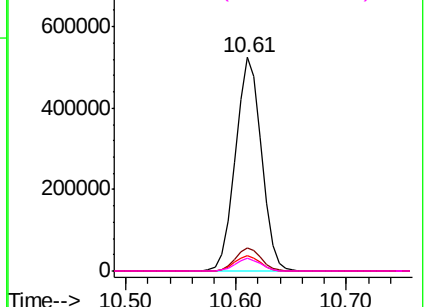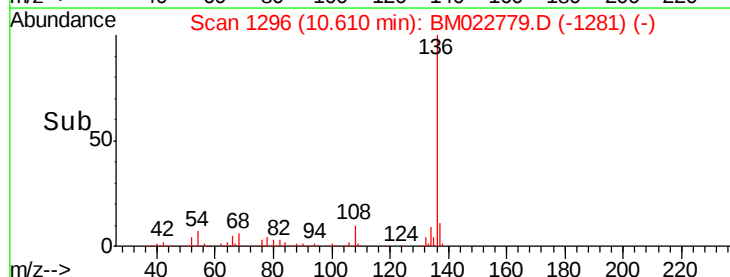

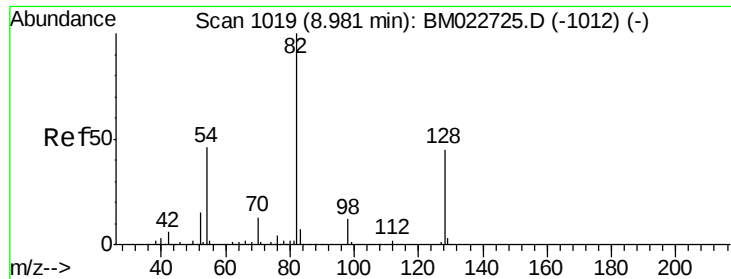





#23
 Nitrobenzene-d5
 Concen: 99.517 ng
 RT: 8.97 min Scan# 1018
 Delta R.T. -0.01 min
 Lab File: BM022779.D
 Acq: 25 Sep 2019 19:43

Instrument :
 BNA_M
 ClientSampleId :
 WC-12-091919

Tot Ion	82	Resp	1553036
Ion Ratio	100	Lower	Upper
128	46.7	36.0	54.0
54	45.8	37.1	55.7




Manual Integrations
 APPROVED


mohammad
 9/26/2019 3:55:07 PM

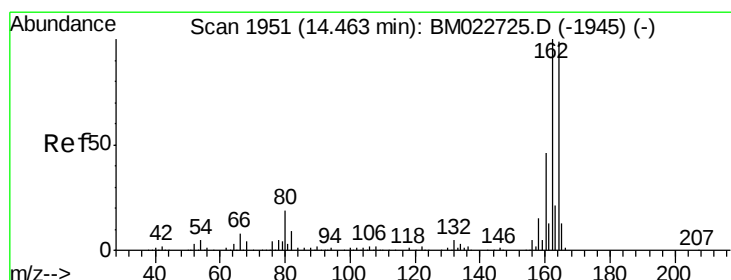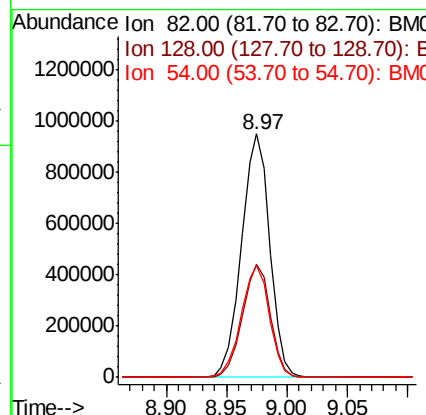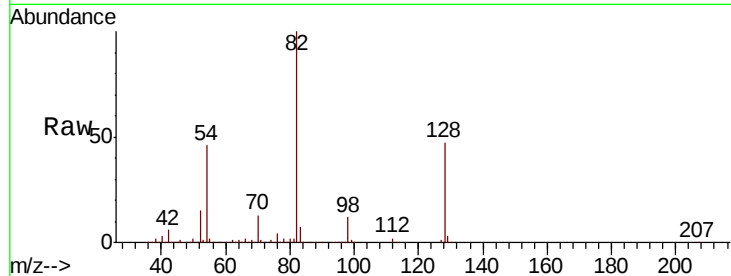

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.45 min Scan# 1949
 Delta R.T. -0.01 min
 Lab File: BM022779.D
 Acq: 25 Sep 2019 19:43

Tgt Ion	164	Resp	465507
Ion Ratio	100	Lower	Upper
162	101.1	81.1	121.7
160	45.0	36.9	55.3

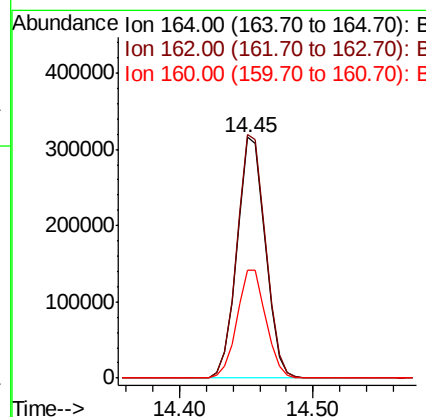

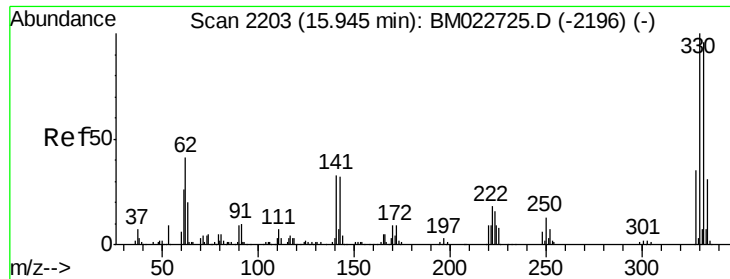


#42
 2,4,6-Tribromophenol
 Concen: 152.923 ng
 RT: 15.94 min Scan# 2202
 Delta R.T. -0.01 min
 Lab File: BM022779.D
 Acq: 25 Sep 2019 19:43

Instrument :
 BNA_M
 ClientSampleId :
 WC-12-091919

Tot Ion	Ratio	Resp	Lower	Upper
330	100	888652		
332	96.0		76.9	115.3
141	33.2		28.6	42.8

Manual Integrations
 APPROVED

mohammad
 9/26/2019 3:55:07 PM



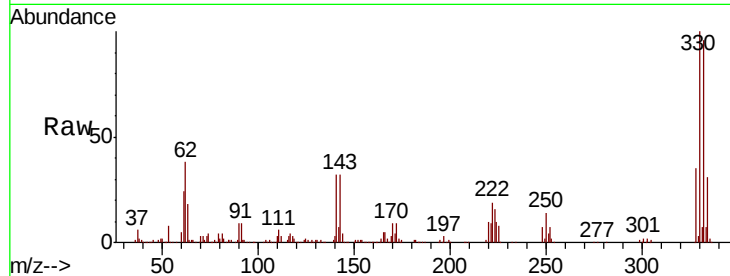


Abundance

Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

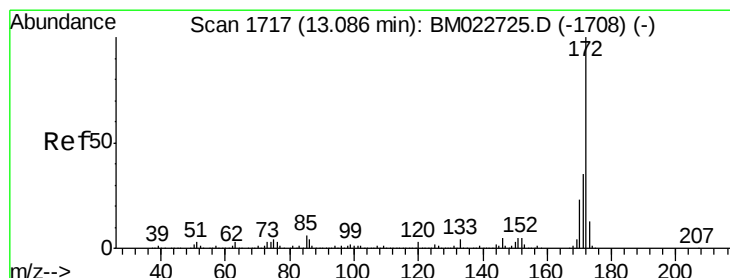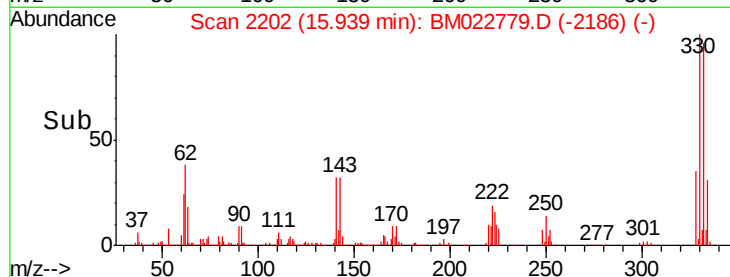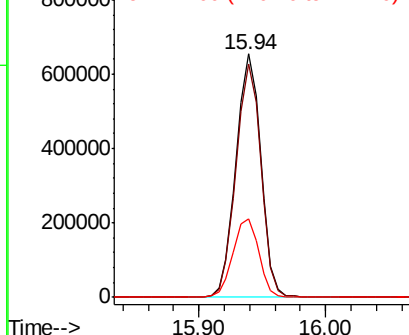

#45
 2-Fluorobiphenyl
 Concen: 106.709 ng
 RT: 13.08 min Scan# 1716
 Delta R.T. -0.01 min
 Lab File: BM022779.D
 Acq: 25 Sep 2019 19:43




Tgt Ion	Ratio	Resp	Lower	Upper
172	100	3607283		
171	35.3		27.8	41.8
170	23.6		18.7	28.1


Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

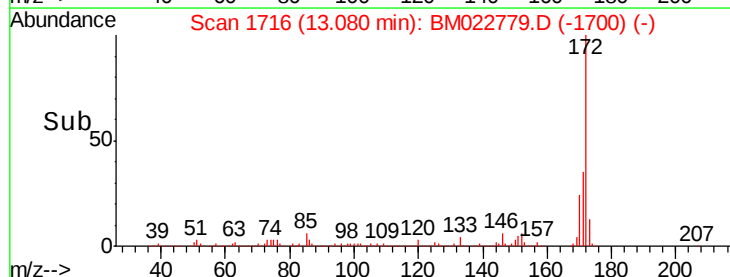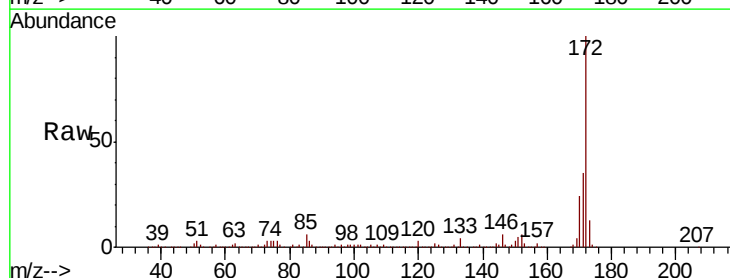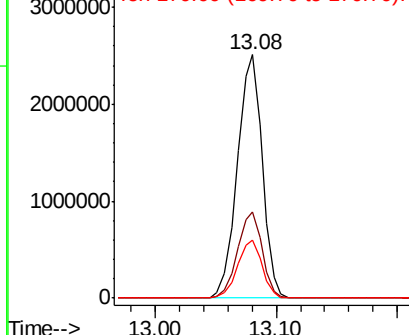

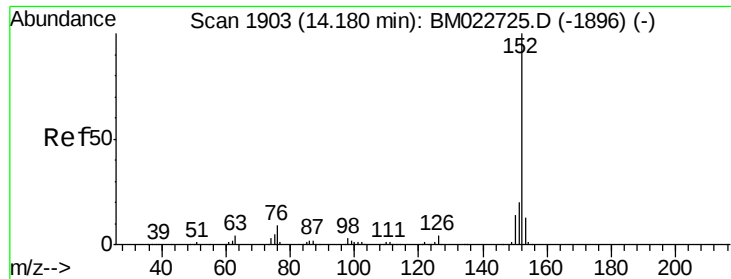

#49

Acenaphthylene

Concen: 2.644 ng

RT: 14.17 min Scan# 1902

Delta R.T. -0.01 min

Lab File: BM022779.D

Acq: 25 Sep 2019 19:43

Instrument :

BNA_M





ClientSampleId :

WC-12-091919

Tot Ion:	152	Resp:	112449
Ion Ratio	Lower	Upper	
152	100		
151	20.0	15.9	23.9
153	13.4	10.5	15.7

Manual Integrations
APPROVED

mohammad
9/26/2019 3:55:07 PM

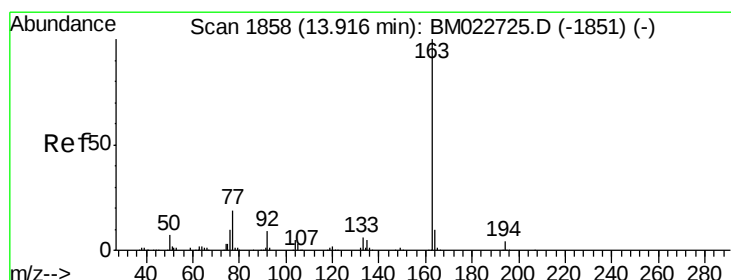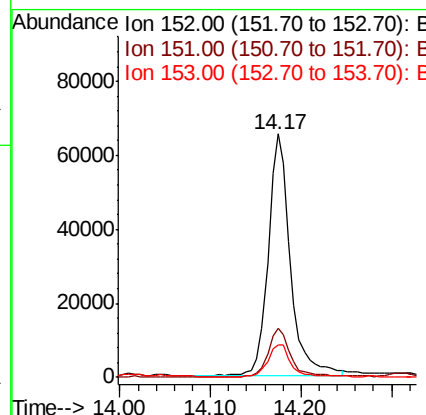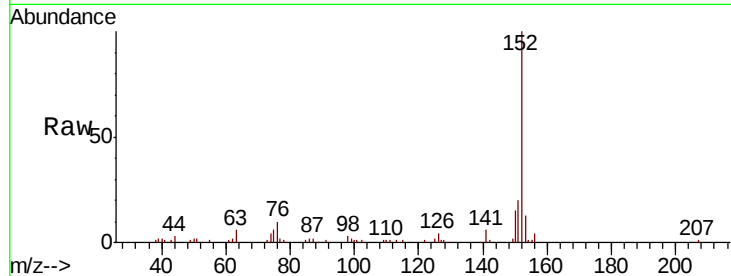

#50

Dimethylphthalate

Concen: 6.761 ng




RT: 13.91 min Scan# 1857


Delta R.T. -0.01 min

Lab File: BM022779.D

Acq: 25 Sep 2019 19:43

Tgt Ion:	163	Resp:	227445
Ion Ratio	Lower	Upper	
163	100		
194	4.2	3.3	4.9
164	9.9	8.2	12.2

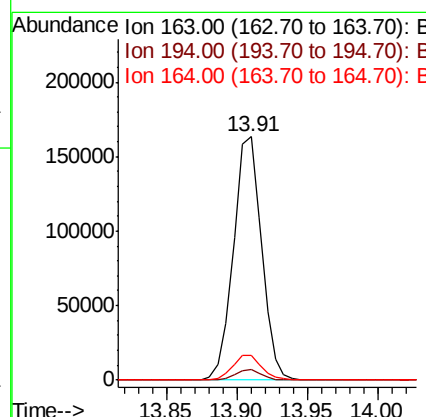

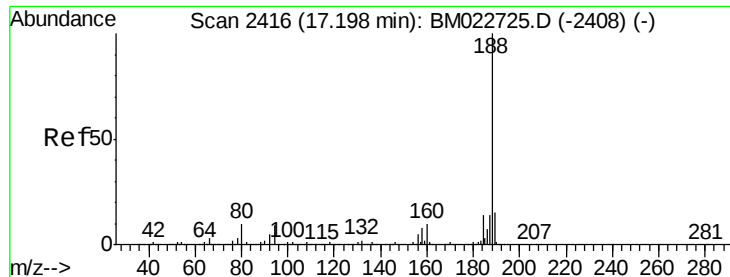





#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.19 min Scan# 2415
Delta R.T. -0.01 min
Lab File: BM022779.D
Acq: 25 Sep 2019 19:43

Instrument :
BNA_M
ClientSampleId :
WC-12-091919

Tot Ion	Ratio	Resp	Lower	Upper
188	100	837391		
94	9.0		7.3	10.9
80	9.9		7.8	11.8




Manual Integrations
APPROVED


mohammad
9/26/2019 3:55:07 PM

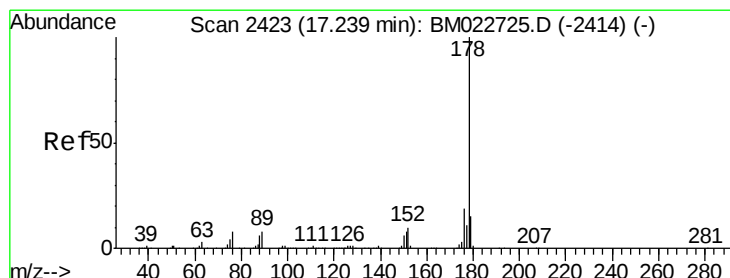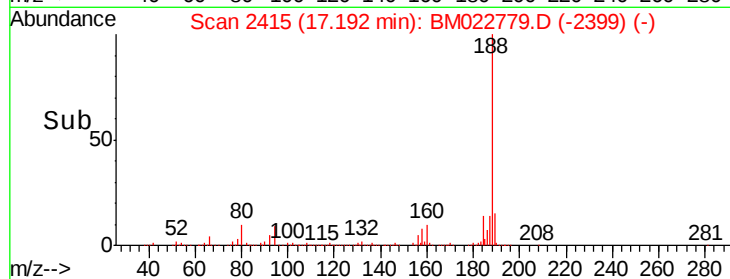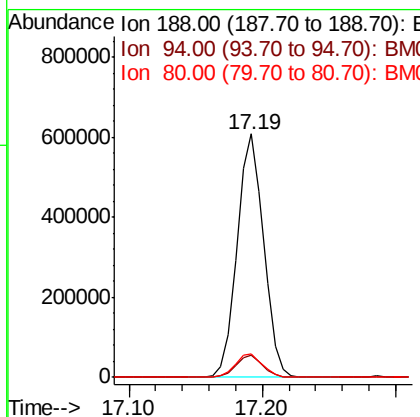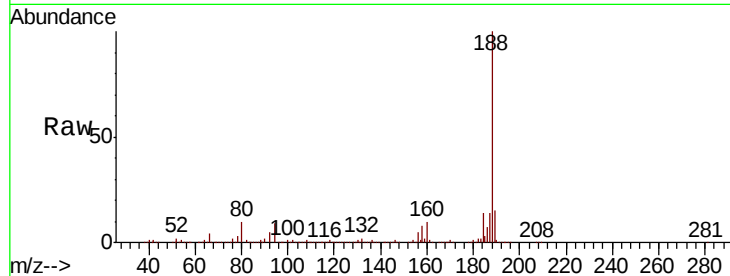

#71
Phenanthrene
Concen: 8.464 ng
RT: 17.23 min Scan# 2422
Delta R.T. -0.01 min
Lab File: BM022779.D
Acq: 25 Sep 2019 19:43

Tgt Ion	Ratio	Resp	Lower	Upper
178	100	399914		
176	19.1		15.4	23.2
179	15.4		12.3	18.5

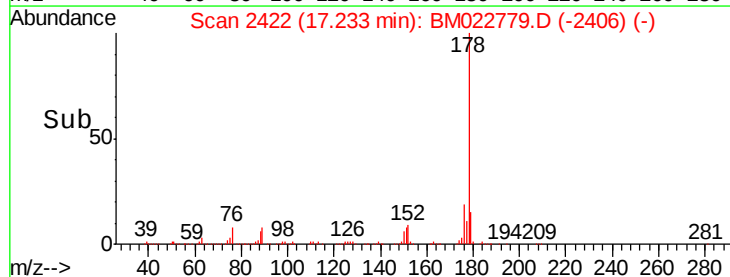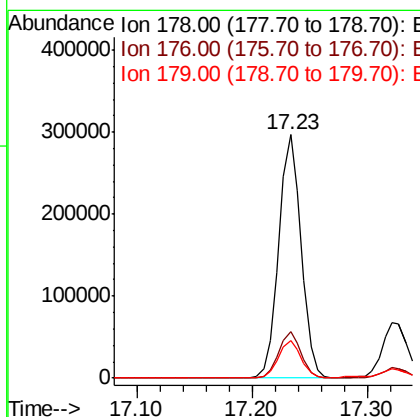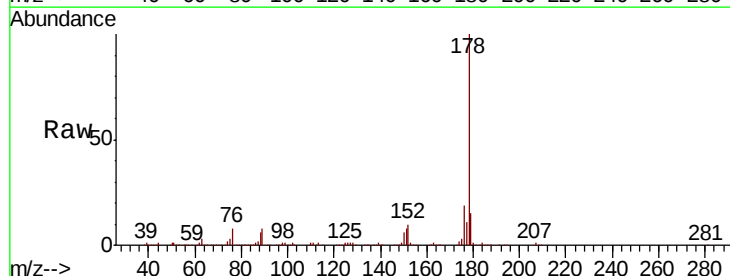

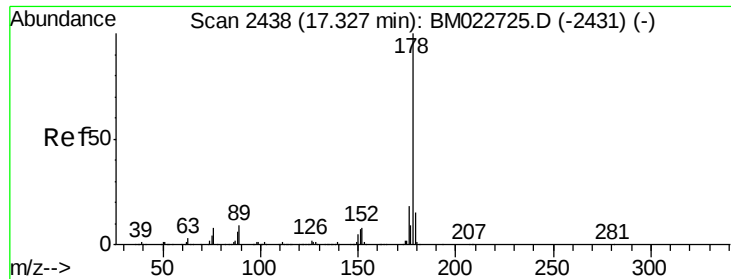

#72

Anthracene

Concen: 2.224 ng

RT: 17.32 min Scan# 2437

Delta R.T. -0.01 min

Lab File: BM022779.D

Acq: 25 Sep 2019 19:43

Instrument :

BNA_M


ClientSampleId :

WC-12-091919




Tot Ion:	178	Resp:	101825
Ion Ratio	Lower	Upper	
178	100		
176	19.2	14.7	22.1
179	15.9	12.2	18.4

Manual Integrations
APPROVED

mohammad
9/26/2019 3:55:07 PM

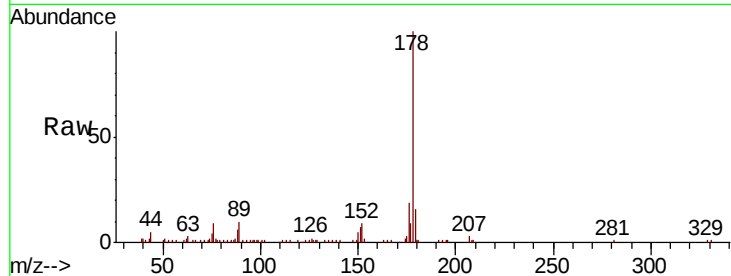

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

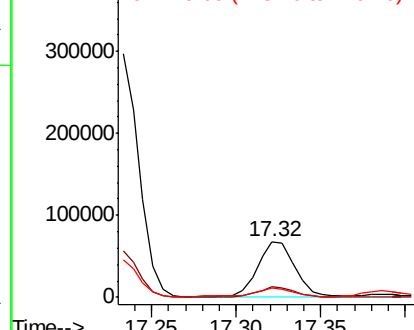

#75

Fluoranthene

Concen: 10.226 ng


RT: 19.24 min Scan# 2764

Delta R.T. -0.01 min



Lab File: BM022779.D


Acq: 25 Sep 2019 19:43

Tgt Ion:	202	Resp:	545216
Ion Ratio	Lower	Upper	
202	100		
101	11.5	0.0	32.1
203	17.8	0.0	37.7



Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 203.00 (202.70 to 203.70): E

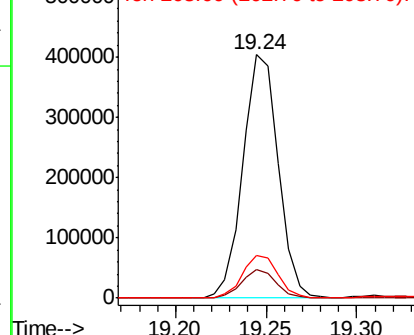

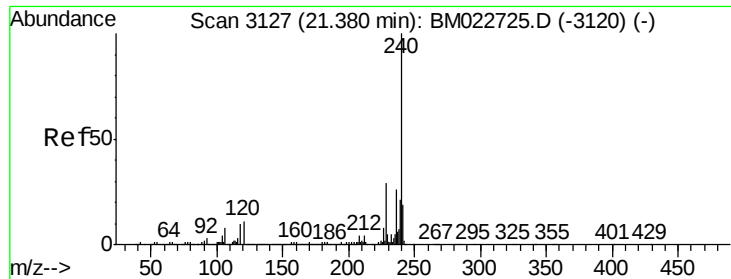





#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.37 min Scan# 3125
Delta R.T. -0.01 min
Lab File: BM022779.D
Acq: 25 Sep 2019 19:43

Instrument :
BNA_M
ClientSampleId :
WC-12-091919

Tot Ion	Ratio	Resp	Lower	Upper
240	100	835142		
120	10.9		8.8	13.2
236	25.8		20.8	31.2




Manual Integrations
APPROVED


mohammad
9/26/2019 3:55:07 PM

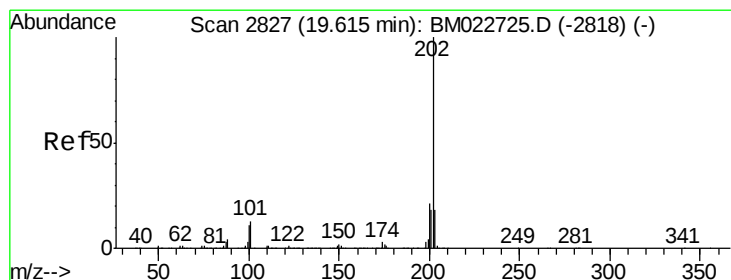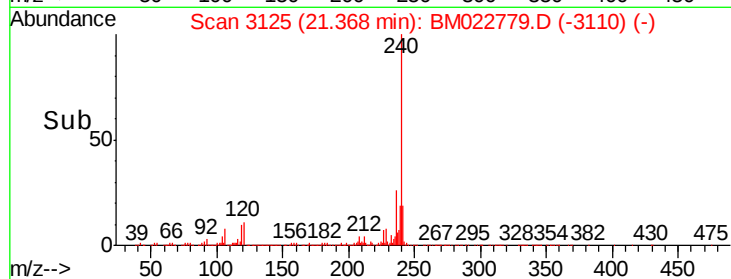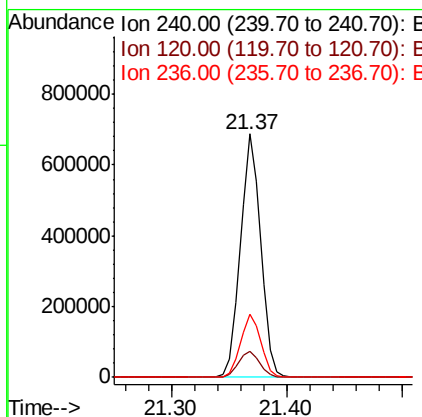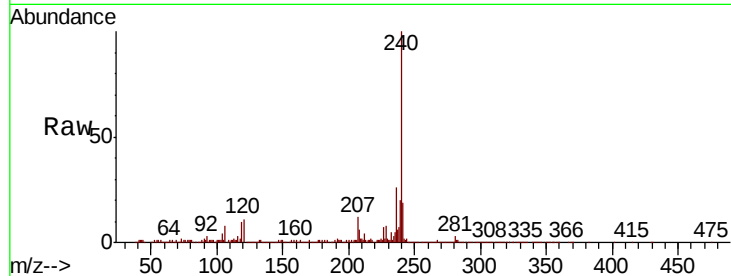

#78
Pyrene
Concen: 11.605 ng
RT: 19.61 min Scan# 2826
Delta R.T. -0.01 min
Lab File: BM022779.D
Acq: 25 Sep 2019 19:43

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	635165		
200	20.9		16.7	25.1
203	17.8		14.1	21.1

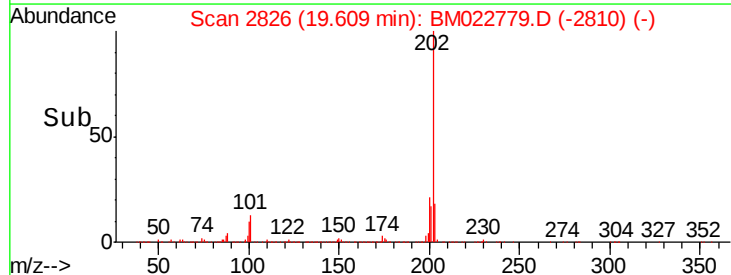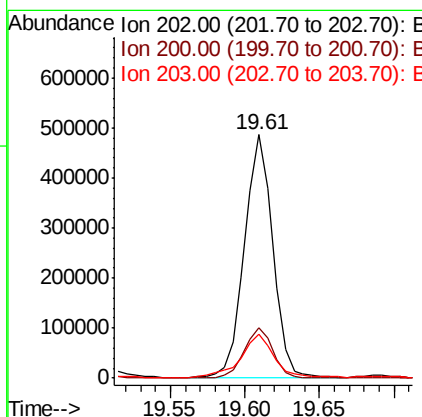

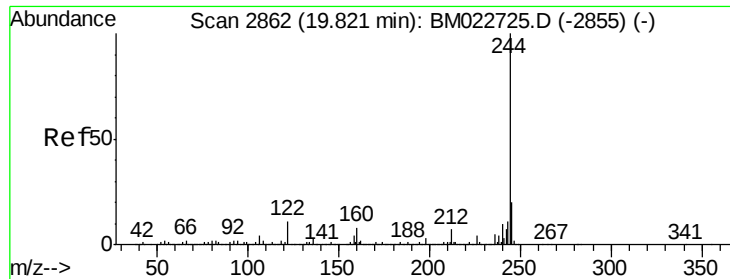





#79
 Terphenyl-d14
 Concen: 99.911 ng
 RT: 19.82 min Scan# 2861
 Delta R.T. -0.01 min
 Lab File: BM022779.D
 Acq: 25 Sep 2019 19:43

Instrument :
 BNA_M
 ClientSampleId :
 WC-12-091919

Tot Ion	Ratio	Lower	Upper
244	100		
212	7.5	5.9	8.9
122	11.0	9.0	13.4




Manual Integrations
 APPROVED


mohammad
 9/26/2019 3:55:07 PM

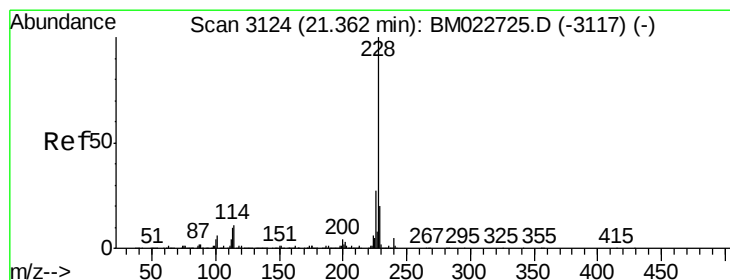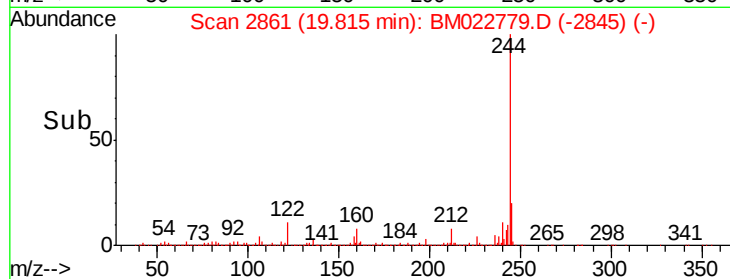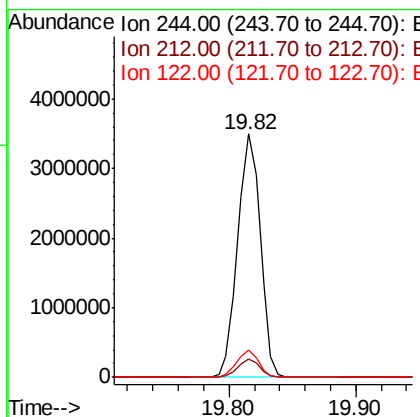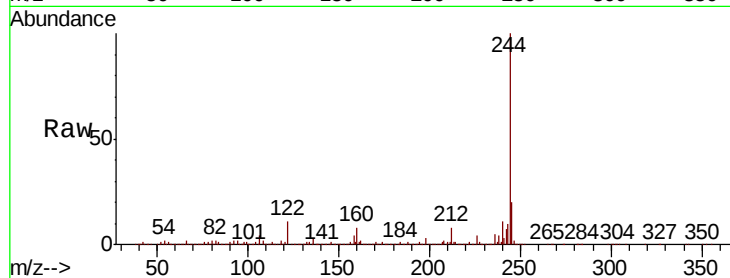

#81
 Benzo(a)anthracene
 Concen: 5.530 ng
 RT: 21.35 min Scan# 3122
 Delta R.T. -0.01 min
 Lab File: BM022779.D
 Acq: 25 Sep 2019 19:43

Tgt Ion	Ratio	Lower	Upper
228	100		
226	30.4	22.0	33.0
229	21.9	15.9	23.9

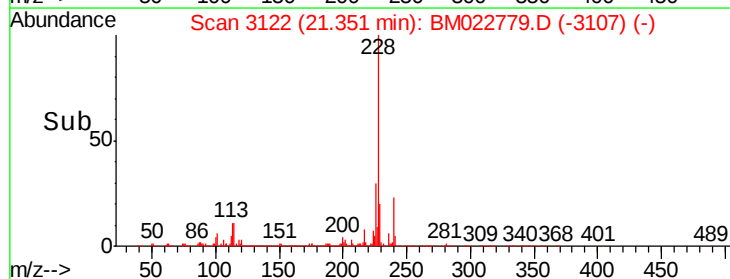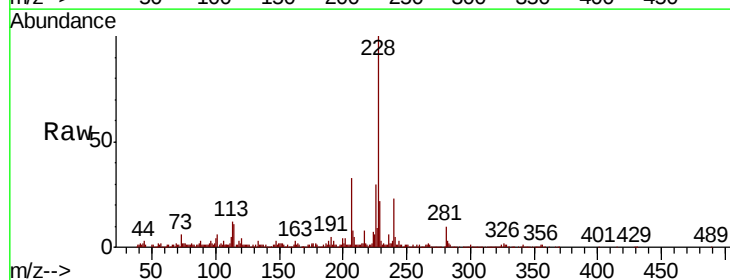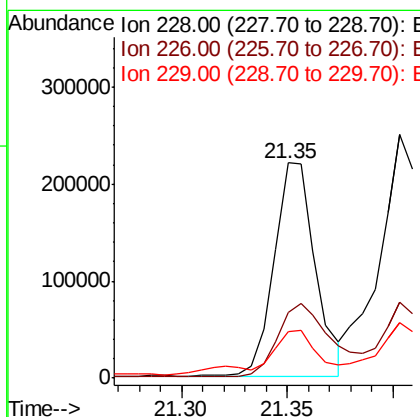







#83
Chrysene
Concen: 6.587 ng
RT: 21.40 min Scan# 3131
Delta R.T. -0.01 min
Lab File: BM022779.D
Acq: 25 Sep 2019 19:43

Instrument :
BNA_M
ClientSampleId :
WC-12-091919

Tot Ion	Ratio	Resp	Lower	Upper
228	100	345659		
226	31.1	24.5	36.7	
229	22.6	15.9	23.9	




Manual Integrations
APPROVED


mohammad
9/26/2019 3:55:07 PM

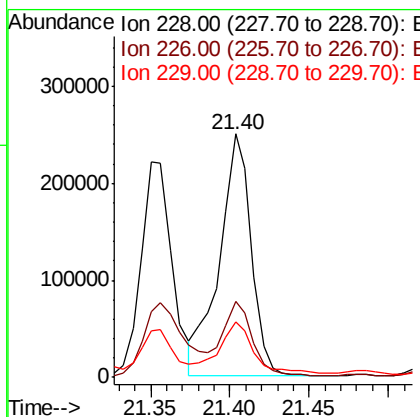

#86
Indeno(1,2,3-cd)pyrene
Concen: 3.270 ng
RT: 25.94 min Scan# 3903
Delta R.T. -0.02 min
Lab File: BM022779.D
Acq: 25 Sep 2019 19:43

Tgt Ion	Ratio	Resp	Lower	Upper
276	100	204835		
138	20.7	0.0	0.0#	
277	24.9	0.0	0.0#	

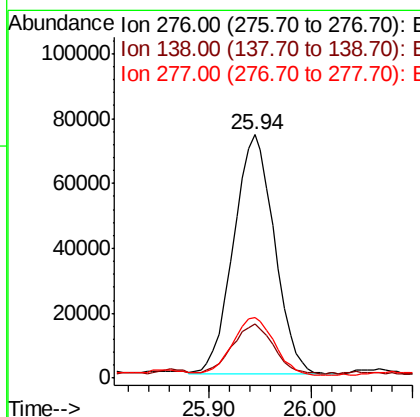

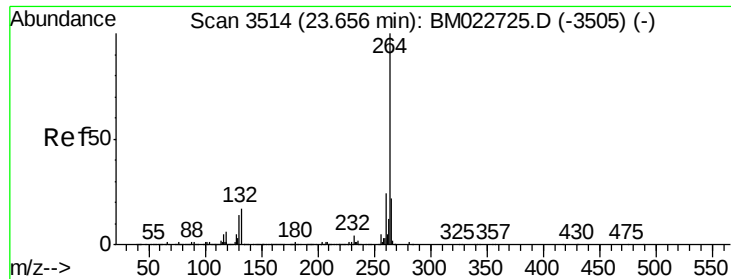





#87
Pervlene-d12
Concen: 20.000 ng
RT: 23.64 min Scan# 3512
Delta R.T. -0.01 min
Lab File: BM022779.D
Acq: 25 Sep 2019 19:43

Instrument :
BNA_M
ClientSampleId :
WC-12-091919

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.6	19.1	28.7
265	22.3	17.9	26.9




Manual Integrations
APPROVED


mohammad
9/26/2019 3:55:07 PM

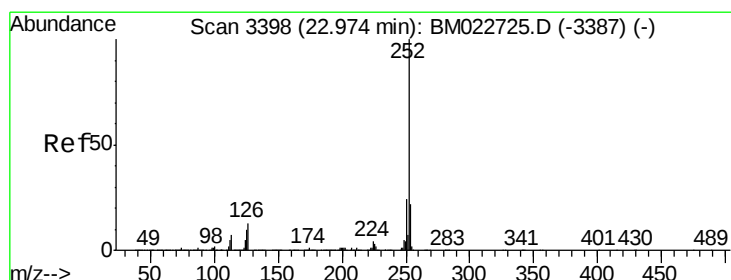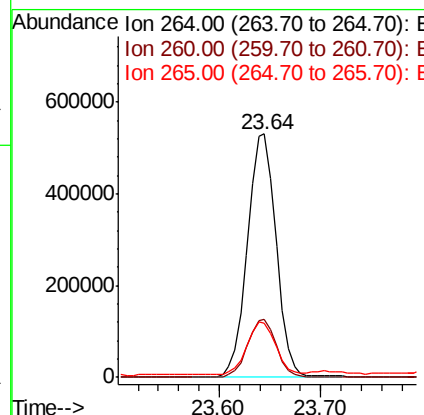

#88
Benzo(b)fluoranthene
Concen: 5.925 ng m
RT: 22.96 min Scan# 3396
Delta R.T. -0.01 min
Lab File: BM022779.D
Acq: 25 Sep 2019 19:43

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.6	17.7	26.5
125	12.2	8.2	12.4

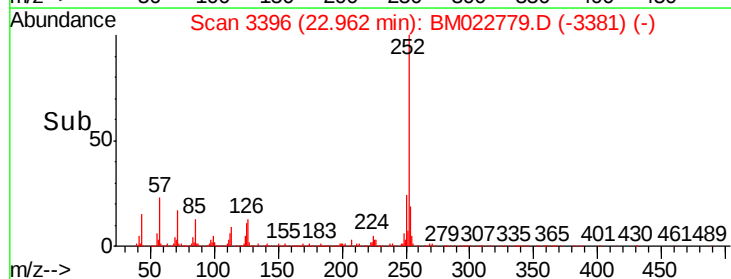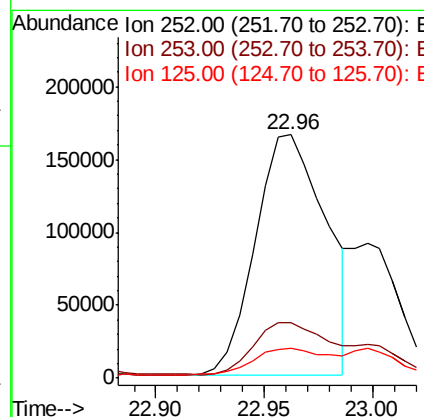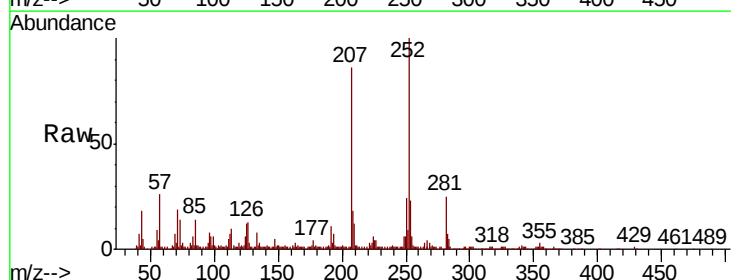

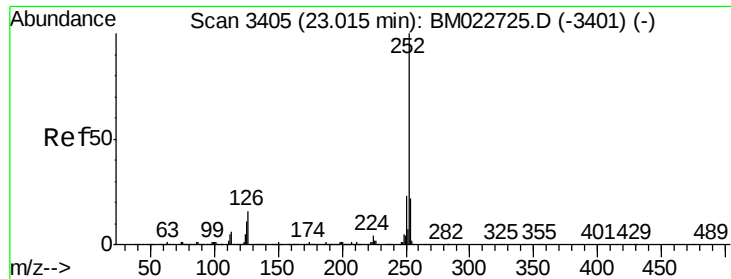





#89
Benzo(k)fluoranthene
Concen: 2.211 ng m
RT: 23.00 min Scan# 3402
Delta R.T. -0.02 min
Lab File: BM022779.D
Acq: 25 Sep 2019 19:43

Instrument :
BNA_M
ClientSampleId :
WC-12-091919

Tot Ion	Ratio	Lower	Upper
252	100		
253	25.2	17.7	26.5
125	21.8	8.5	12.7




Manual Integrations
APPROVED


mohammad
9/26/2019 3:55:07 PM

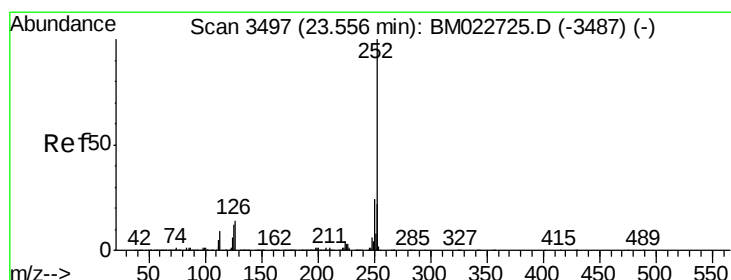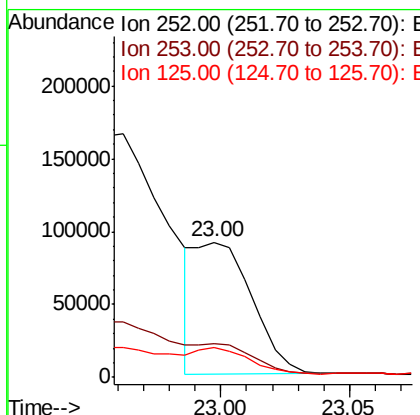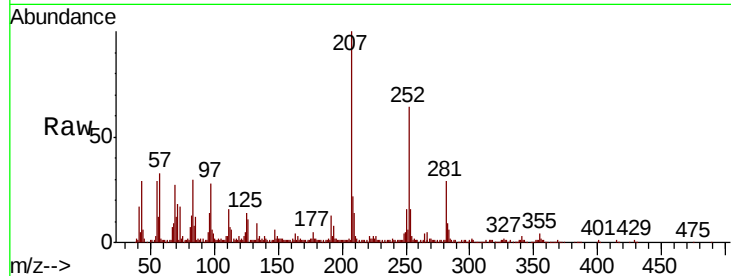

#90
Benzo(a)pyrene
Concen: 5.209 ng
RT: 23.54 min Scan# 3495
Delta R.T. -0.01 min
Lab File: BM022779.D
Acq: 25 Sep 2019 19:43

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.1	17.3	25.9
125	11.5	9.3	13.9

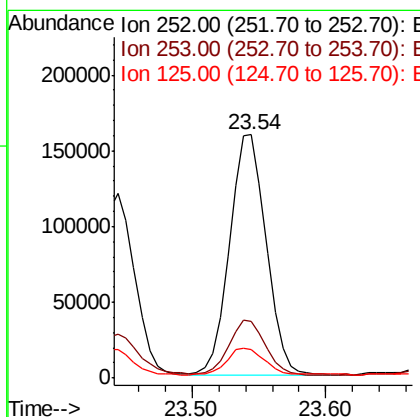



#92
 Benzo(a,h,i)perylene
 Concen: 3.782 ng
 RT: 26.65 min Scan# 4023
 Delta R.T. -0.02 min
 Lab File: BM022779.D
 Acq: 25 Sep 2019 19:43

Instrument :
 BNA_M
 ClientSampleId :
 WC-12-091919

Tot Ion:	276	Resp:	217649
Ion Ratio	Lower	Upper	
276	100		
277	24.8	19.1	28.7
138	23.3	18.5	27.7

Manual Integrations
 APPROVED

mohammad
 9/26/2019 3:55:07 PM

