


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092519\
 Data File : BM022768.D
 Acq On : 25 Sep 2019 13:00
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM092019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 20 16:34:01 2019

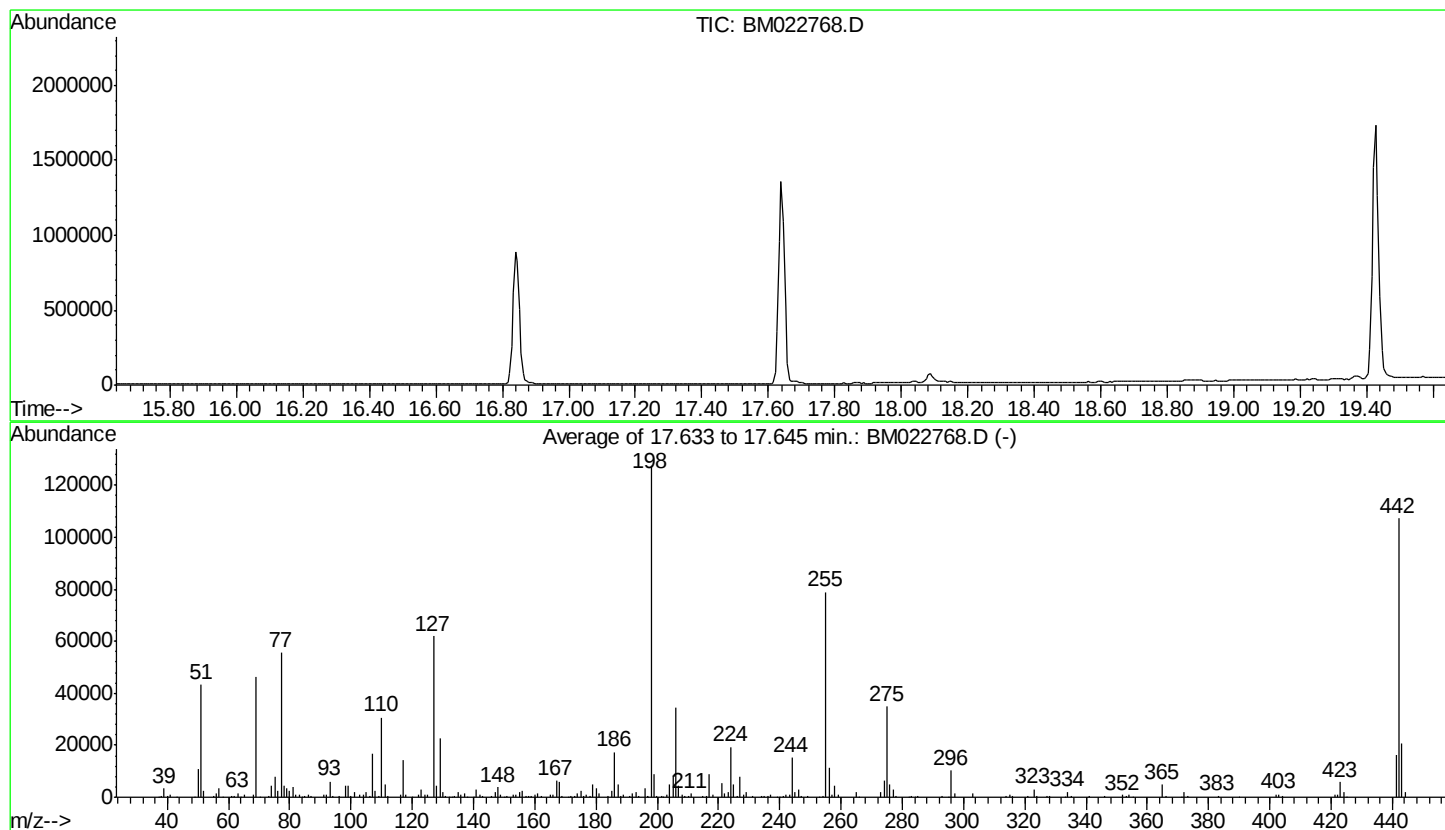

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	43138	PASS
68	69	0.00	2	1.9	882	PASS
69	198	0.00	100	36.1	46088	PASS
70	69	0.00	2	0.5	226	PASS
127	198	10	80	48.5	61914	PASS
197	198	0.00	2	0.4	479	PASS
198	198	100	100	100.0	127560	PASS
199	198	5	9	6.9	8803	PASS
275	198	10	60	27.3	34805	PASS
365	198	1	100	3.8	4802	PASS
441	198	0.01	100	12.6	16118	PASS
442	198	50	100	84.1	107288	PASS
443	442	15	24	19.3	20700	PASS