

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092523\
 Data File : BM042037.D
 Acq On : 25 Sep 2023 17:59
 Operator : MA/JU
 Sample : PB155688BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK688

Quant Time: Sep 26 02:19:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 13:50:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.950	152	6113	0.400	ng/ul	0.00
4) Naphthalene-d8	10.763	136	15904	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.592	164	8116	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.346	188	15802	0.400	ng/ul	0.00
17) Chrysene-d12	21.521	240	5352	0.400	ng/ul	0.00
23) Perylene-d12	23.927	264	4938	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.368	96	44003	5.282	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.346	152	5678	0.285	ng/ul	0.00
18) Fluoranthene-d10	19.366	212	7990	0.363	ng/ul	0.00
Target Compounds						Qvalue
12) Fluorene	15.587	166	2937	0.063	ng/ul#	14
20) Pyrene	19.738	202	2421	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.769	252	3108	0.099	ng/ul#	41


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092523\
Data File : BM042037.D
Acq On : 25 Sep 2023 17:59
Operator : MA/JU
Sample : PB155688BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK688

Quant Time: Sep 26 02:19:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 13:50:58 2023
Response via : Initial Calibration




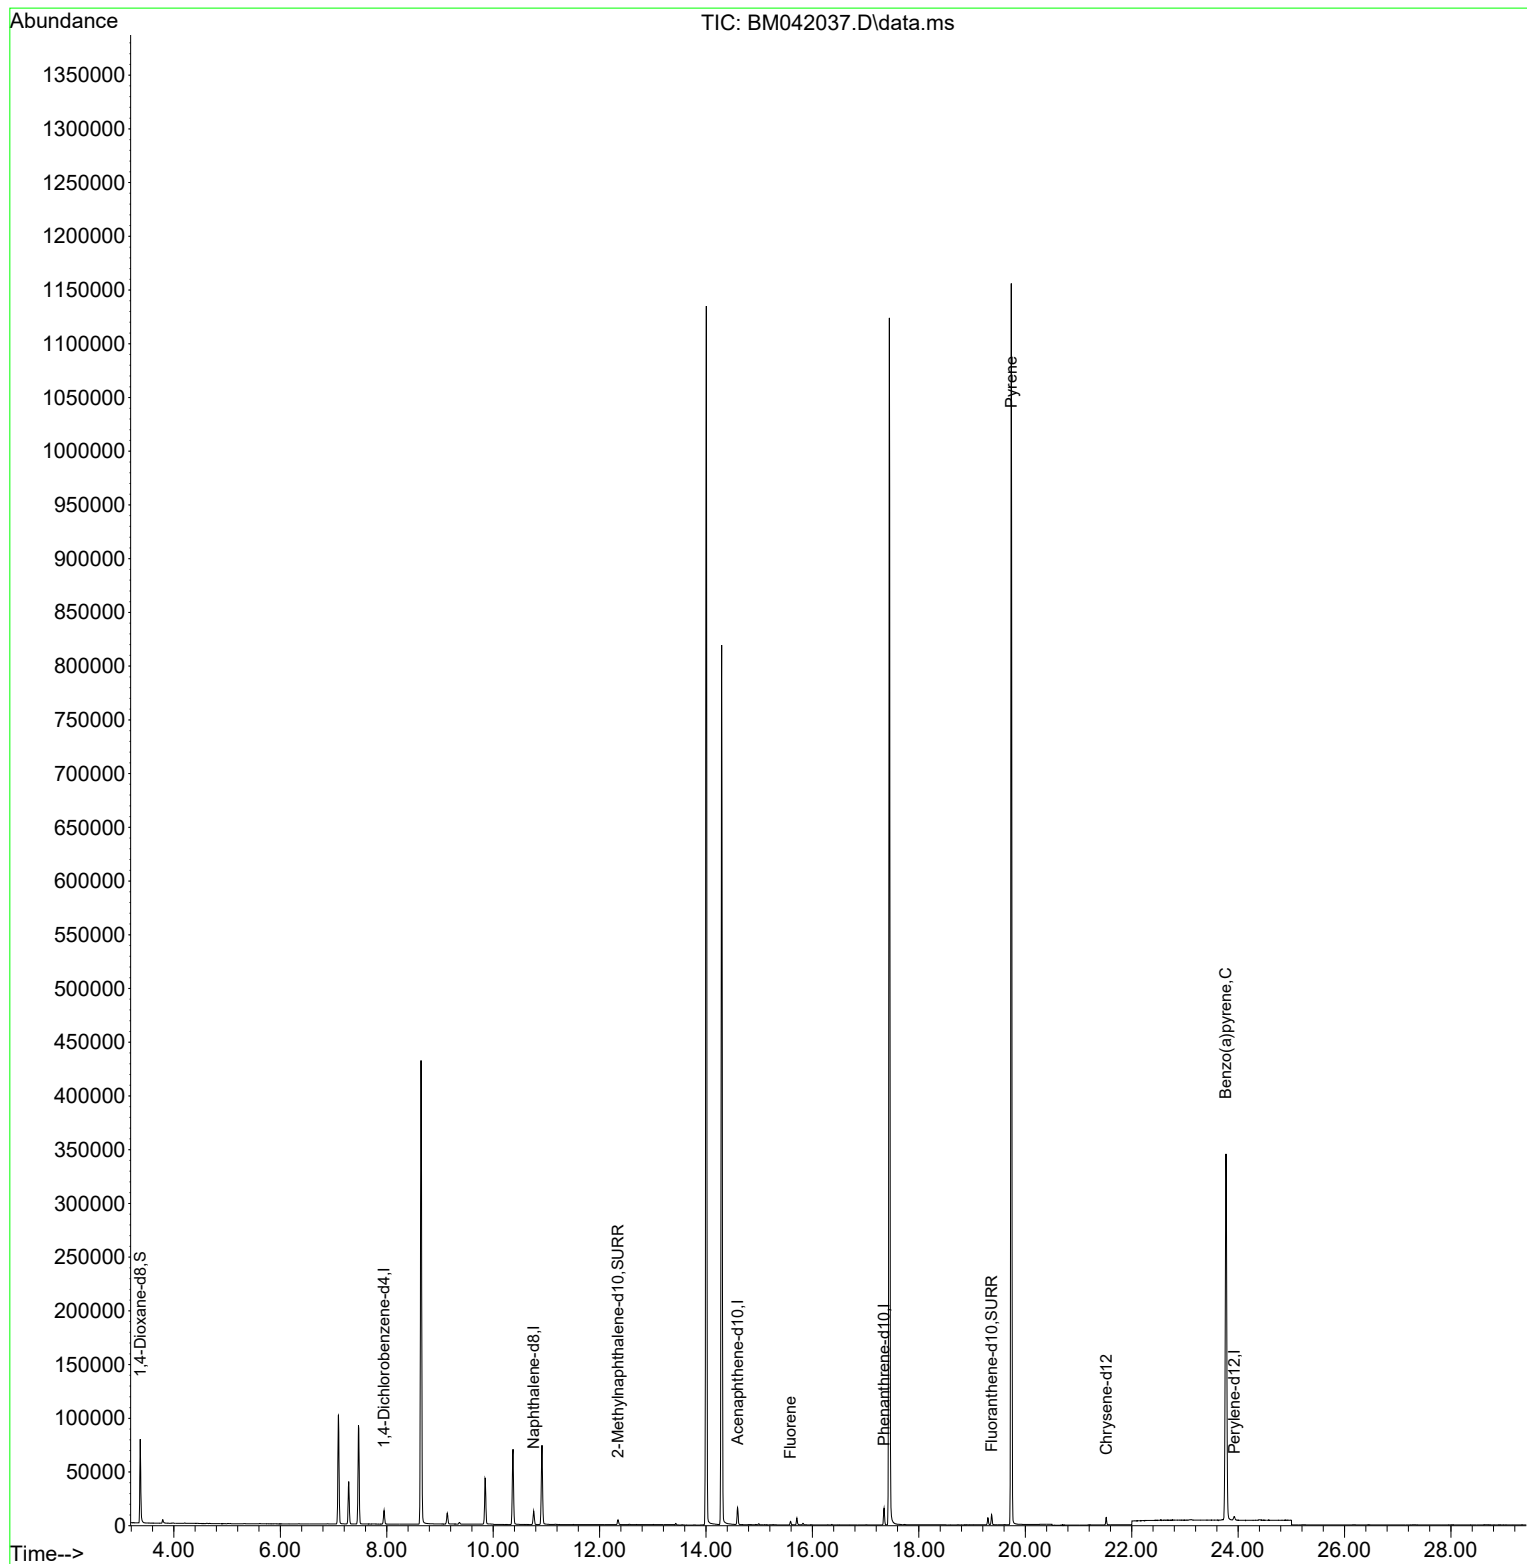


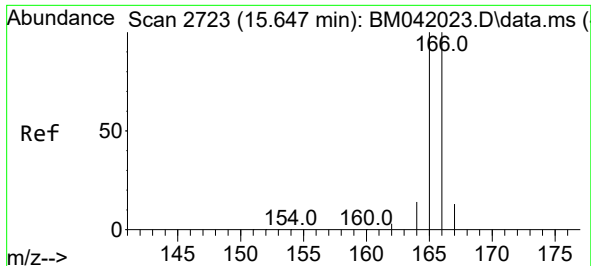

#12
Fluorene
Concen: 0.063 ng/ul
RT: 15.587 min Scan# 21
Delta R.T. -0.065 min
Lab File: BM042037.D
Acq: 25 Sep 2023 17:59




Instrument :
BNA_M
ClientSampleId :
SBLK688


Tgt Ion:166 Resp: 2937
Ion Ratio Lower Upper
166 100
165 8.7 79.8 119.8#
167 32.3 11.1 16.7#

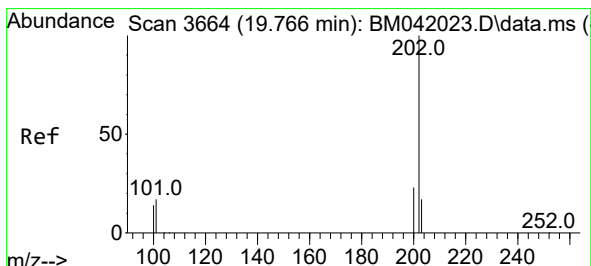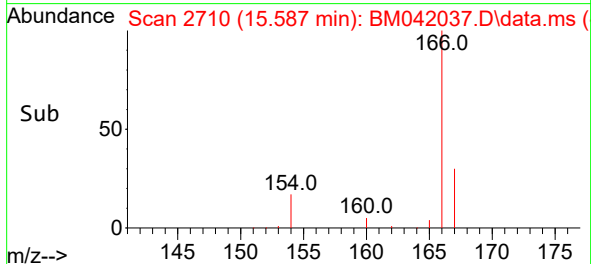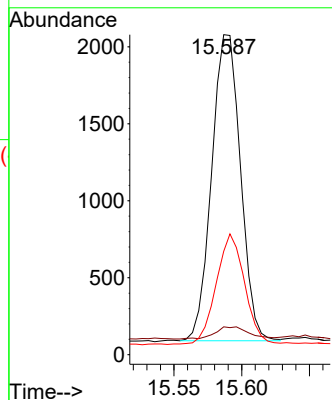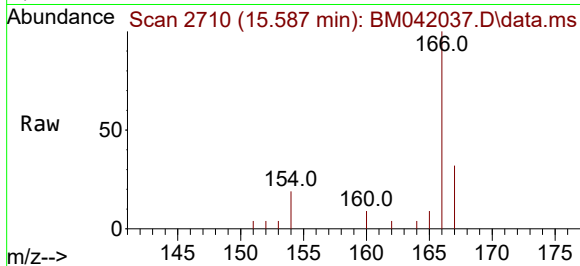

#20
Pyrene
Concen: 0.041 ng/ul
RT: 19.738 min Scan# 3658
Delta R.T. -0.032 min
Lab File: BM042037.D
Acq: 25 Sep 2023 17:59

Tgt Ion:202 Resp: 2421
Ion Ratio Lower Upper
202 100
101 179.4 14.1 21.1#
100 1298.6 11.4 17.0#

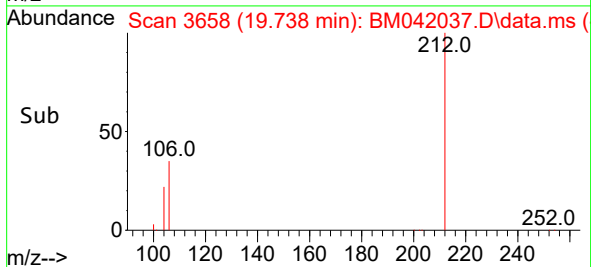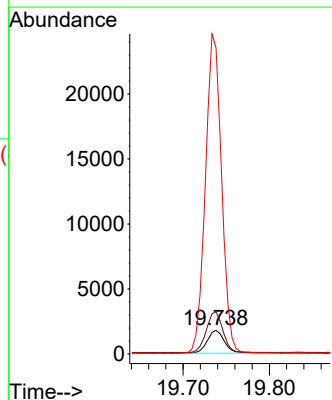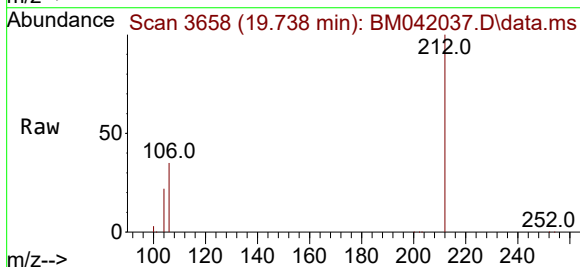

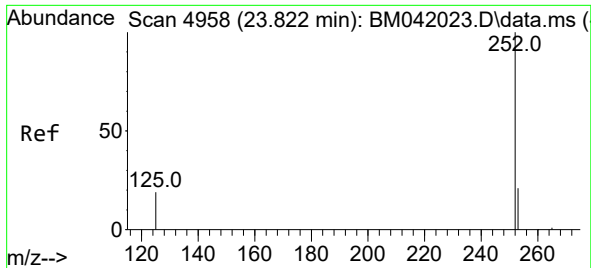

#26

Benzo(a)pyrene

Concen: 0.099 ng/ul

RT: 23.769 min Scan# 49

Delta R.T. -0.058 min

Lab File: BM042037.D


Acq: 25 Sep 2023 17:59

Instrument :

BNA_M

ClientSampleId :

SBLK688

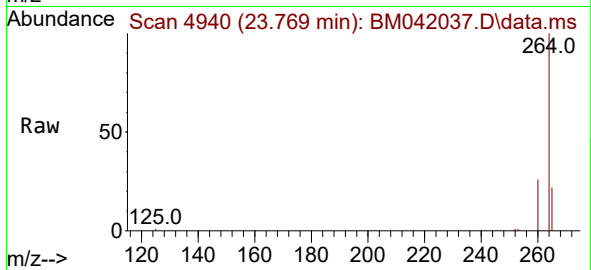

Tgt Ion:252 Resp: 3108

Ion Ratio Lower Upper

252 100

253 57.8 23.2 34.8#

125 61.6 22.5 33.7#

