

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092523\
 Data File : BM042038.D
 Acq On : 25 Sep 2023 18:35
 Operator : MA/JU
 Sample : PB155693BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK693

Quant Time: Sep 26 02:19:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 13:50:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.950	152	5373	0.400	ng/ul	0.00
4) Naphthalene-d8	10.762	136	13908	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.592	164	6877	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.345	188	13085	0.400	ng/ul	0.00
17) Chrysene-d12	21.521	240	4203	0.400	ng/ul	0.00
23) Perylene-d12	23.927	264	4027	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.368	96	46116	6.298	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.346	152	5756	0.330	ng/ul	0.00
18) Fluoranthene-d10	19.371	212	7662	0.443	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.591	166	3036	0.076	ng/ul#	13
20) Pyrene	19.738	202	2344	0.050	ng/ul#	1
26) Benzo(a)pyrene	23.772	252	3149	0.124	ng/ul#	43


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092523\
Data File : BM042038.D
Acq On : 25 Sep 2023 18:35
Operator : MA/JU
Sample : PB155693BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK693

Quant Time: Sep 26 02:19:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 13:50:58 2023
Response via : Initial Calibration




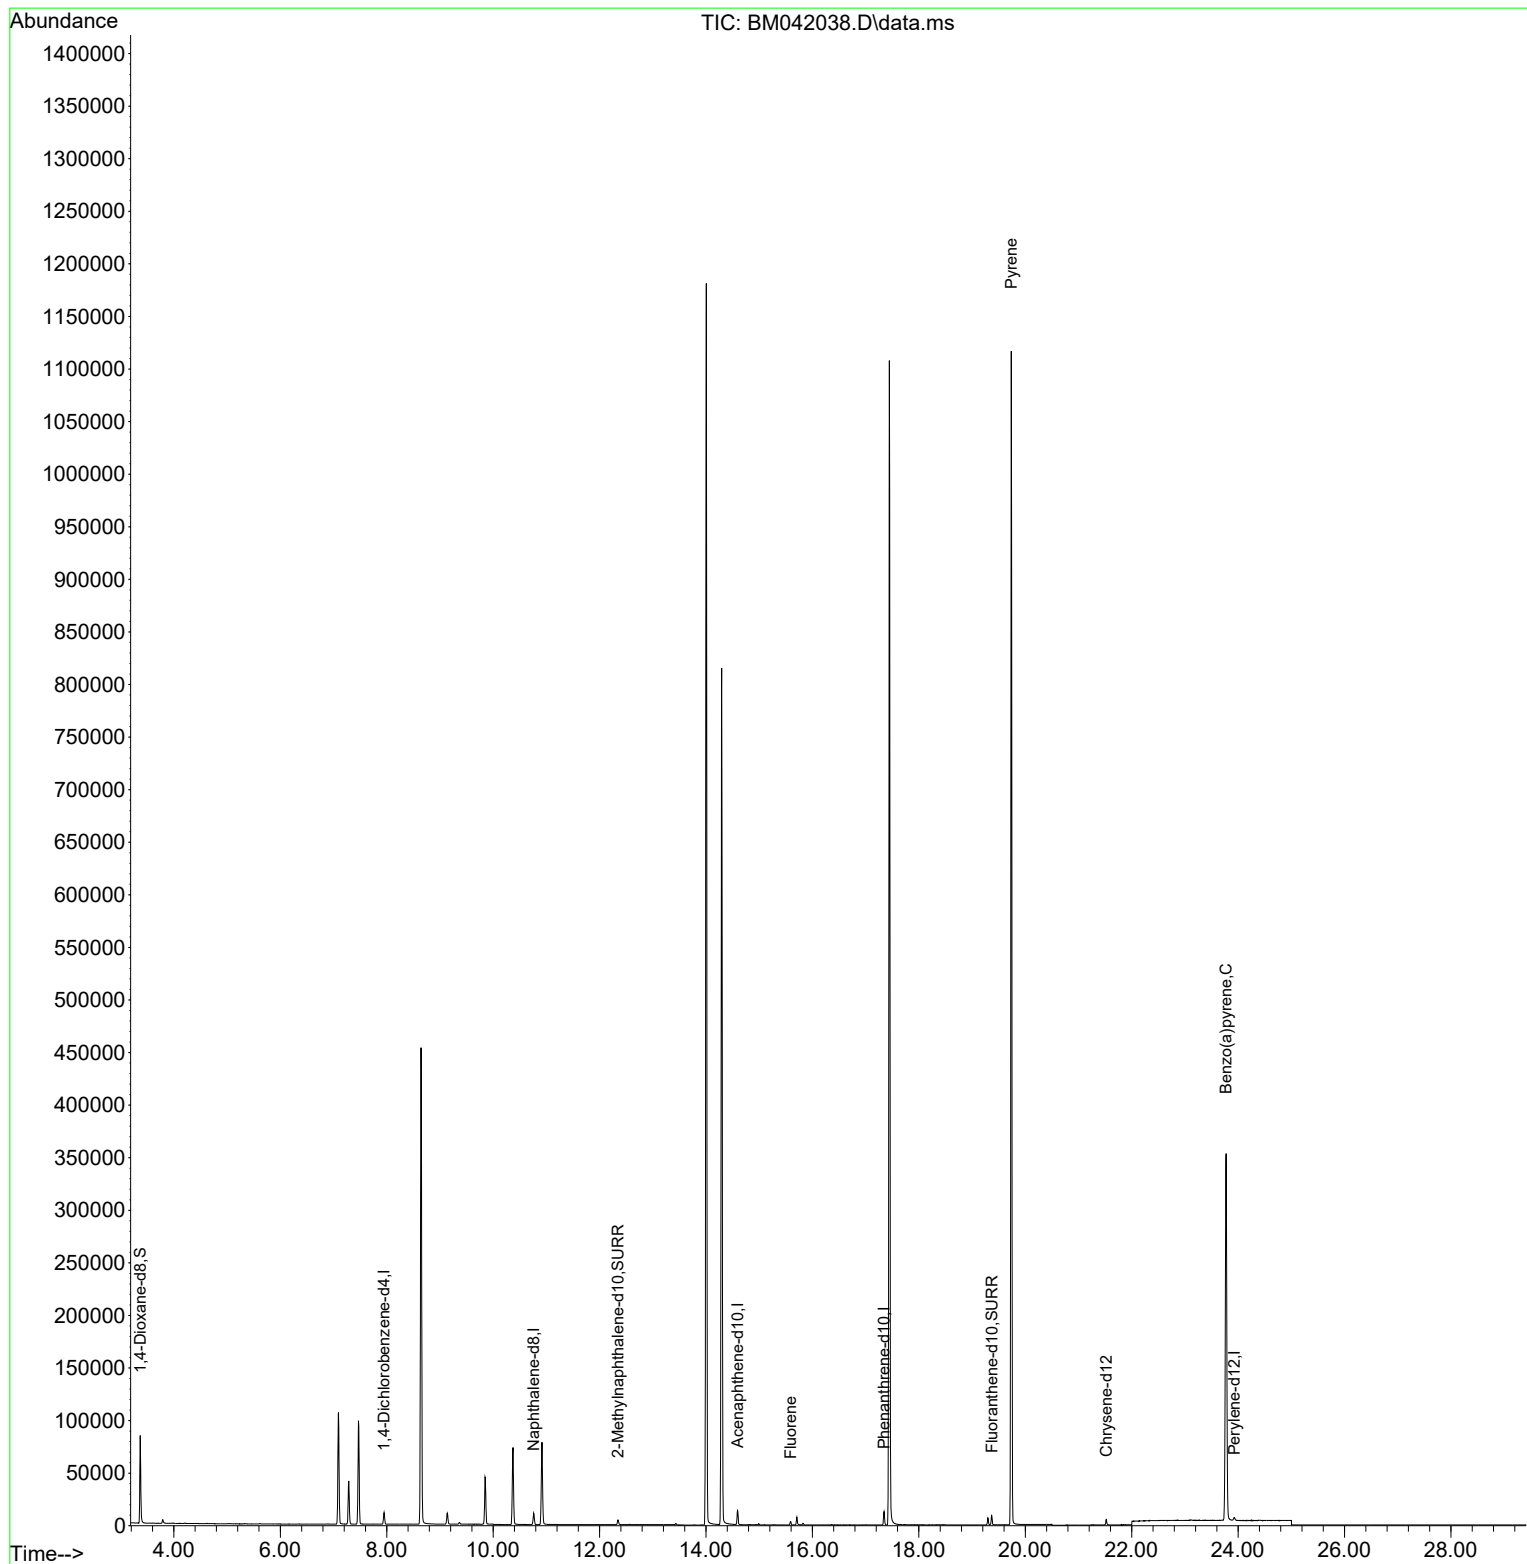


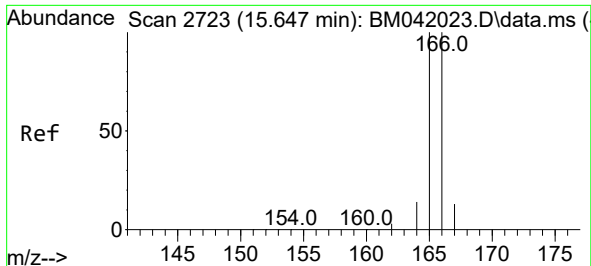

#12
Fluorene
Concen: 0.076 ng/ul
RT: 15.591 min Scan# 21
Delta R.T. -0.060 min
Lab File: BM042038.D
Acq: 25 Sep 2023 18:35




Instrument :
BNA_M
ClientSampleId :
SBLK693


Tgt Ion:166 Resp: 3036
Ion Ratio Lower Upper
166 100
165 8.3 79.8 119.8#
167 35.6 11.1 16.7#

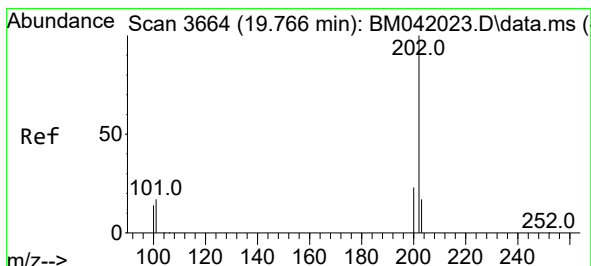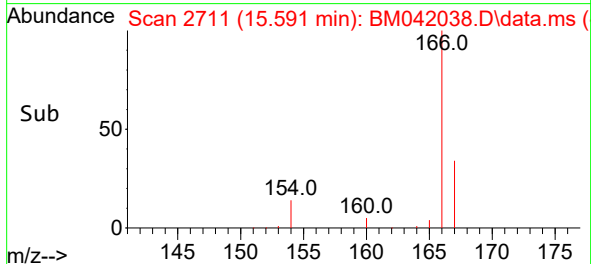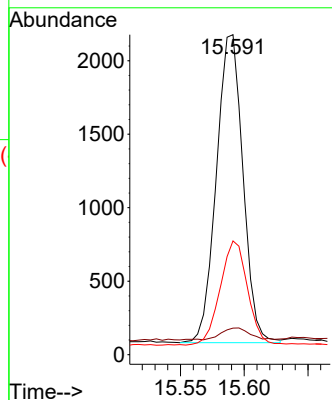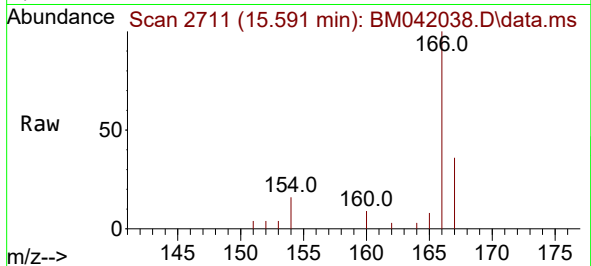

#20
Pyrene
Concen: 0.050 ng/ul
RT: 19.738 min Scan# 3658
Delta R.T. -0.033 min
Lab File: BM042038.D
Acq: 25 Sep 2023 18:35


Tgt Ion:202 Resp: 2344
Ion Ratio Lower Upper
202 100
101 175.9 14.1 21.1#
100 1298.2 11.4 17.0#

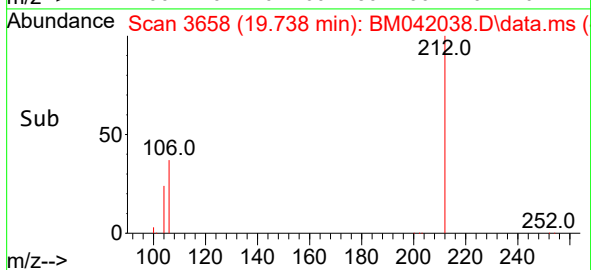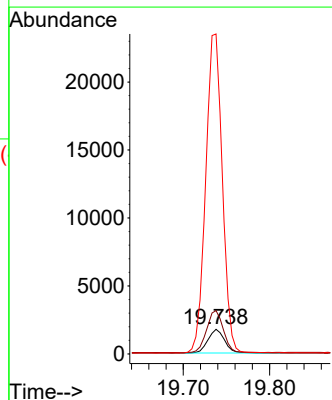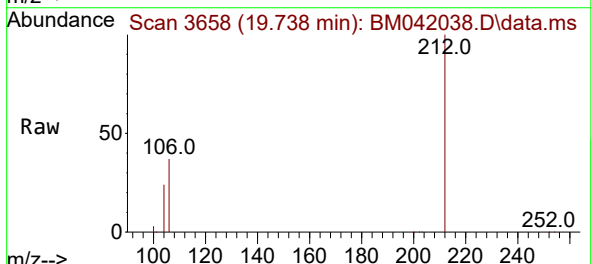

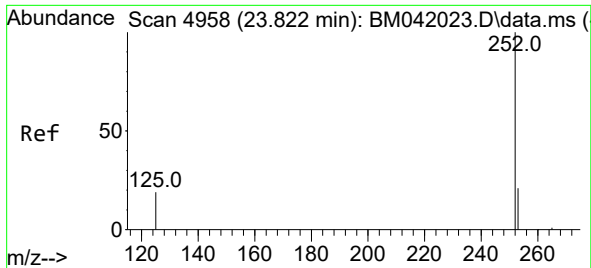

#26
Benzo(a)pyrene
Concen: 0.124 ng/ul
RT: 23.772 min Scan# 4941
Delta R.T. -0.056 min
Lab File: BM042038.D
Acq: 25 Sep 2023 18:35

Instrument :
BNA_M
ClientSampleId :
SBLK693

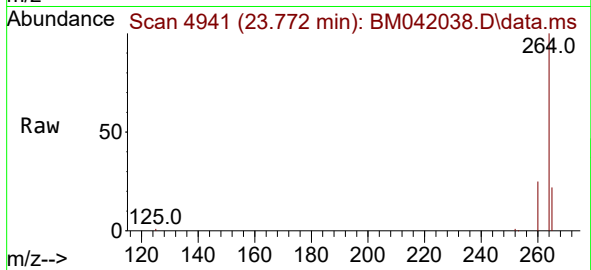

Tgt Ion:252 Resp: 3149
Ion Ratio Lower Upper
252 100
253 57.2 23.2 34.8#
125 60.3 22.5 33.7#

