

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092523\
 Data File : BM042048.D
 Acq On : 26 Sep 2023 00:37
 Operator : MA/JU
 Sample : 04429-17
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJC6

Quant Time: Sep 26 02:21:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 13:50:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.950	152	5458	0.400	ng/ul	0.00
4) Naphthalene-d8	10.762	136	13559	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.592	164	6312	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.345	188	13411	0.400	ng/ul	0.00
17) Chrysene-d12	21.518	240	6844	0.400	ng/ul	0.00
23) Perylene-d12	23.927	264	6836	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.368	96	27957	3.759	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.346	152	5673	0.334	ng/ul	0.00
18) Fluoranthene-d10	19.366	212	10415	0.370	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.406	88	10822	1.383	ng/ul#	89
20) Pyrene	19.738	202	2449	0.032	ng/ul#	1
26) Benzo(a)pyrene	23.772	252	3888	0.090	ng/ul#	46


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092523\
Data File : BM042048.D
Acq On : 26 Sep 2023 00:37
Operator : MA/JU
Sample : 04429-17
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJC6

Quant Time: Sep 26 02:21:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 13:50:58 2023
Response via : Initial Calibration




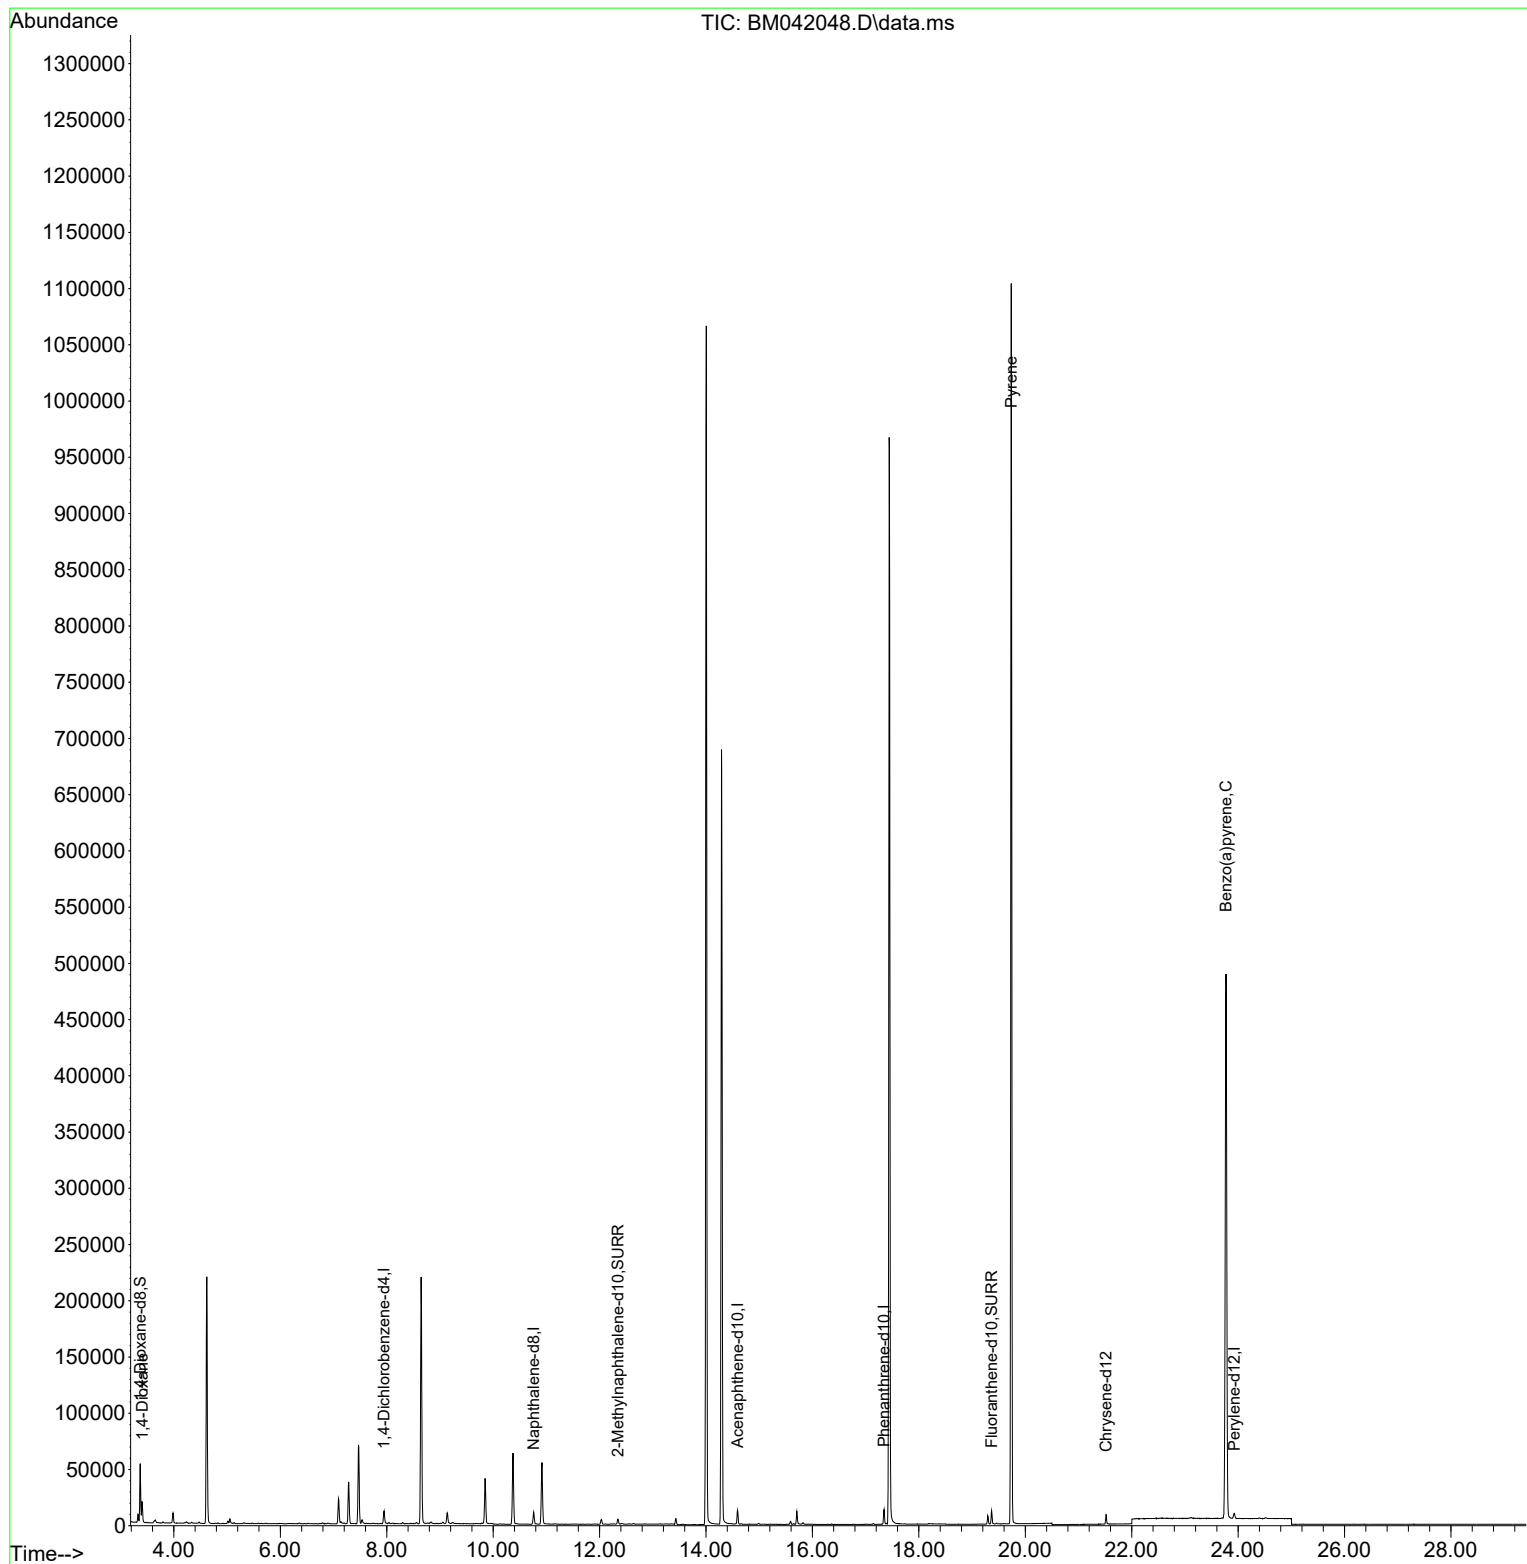


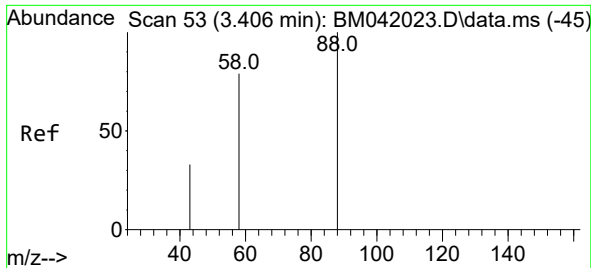

#2
1,4-Dioxane
Concen: 1.383 ng/ul
RT: 3.406 min Scan# 51
Delta R.T. -0.004 min
Lab File: BM042048.D
Acq: 26 Sep 2023 00:37




Instrument :
BNA_M
ClientSampleId :
BBJC6


Tgt Ion: 88 Resp: 10822
Ion Ratio Lower Upper
88 100
43 39.1 42.9 64.3#
58 74.4 56.4 84.6

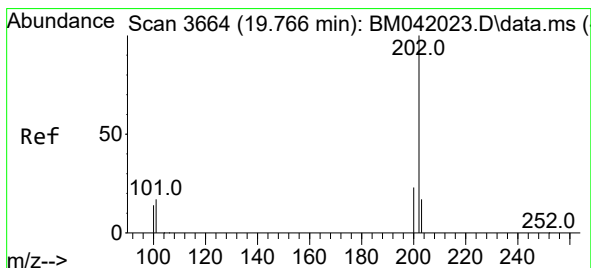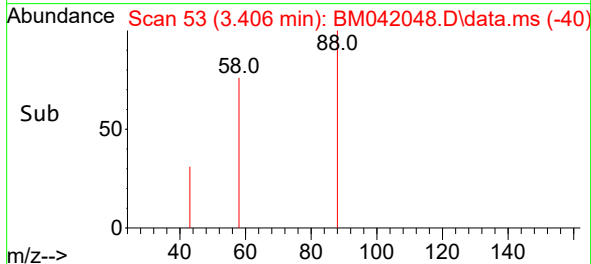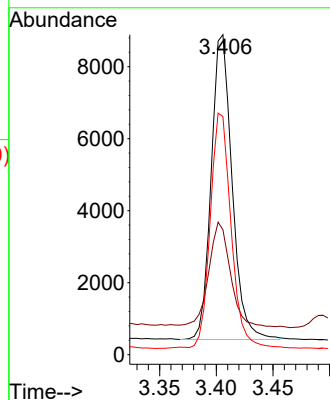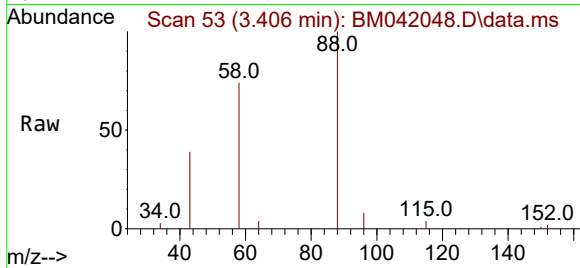

#20
Pyrene
Concen: 0.032 ng/ul
RT: 19.738 min Scan# 3658
Delta R.T. -0.033 min
Lab File: BM042048.D
Acq: 26 Sep 2023 00:37


Tgt Ion: 202 Resp: 2449
Ion Ratio Lower Upper
202 100
101 160.1 14.1 21.1#
100 1152.5 11.4 17.0#

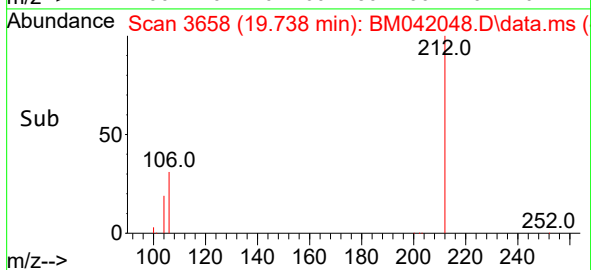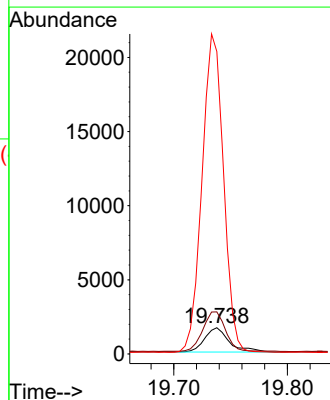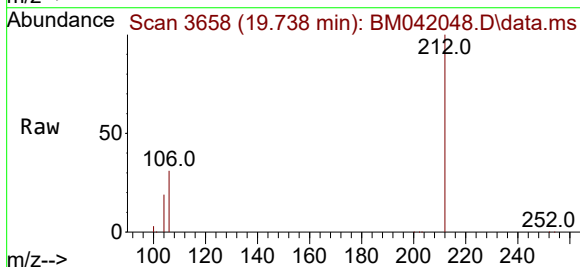

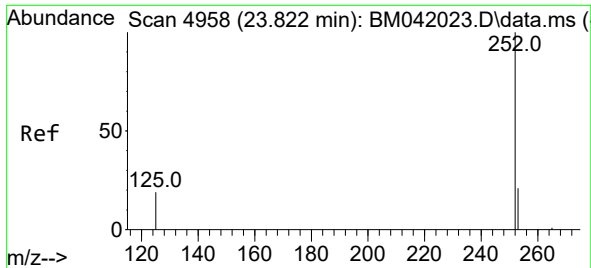

#26
Benzo(a)pyrene
Concen: 0.090 ng/ul
RT: 23.772 min Scan# 4958
Delta R.T. -0.056 min
Lab File: BM042048.D
Acq: 26 Sep 2023 00:37

Instrument :
BNA_M
ClientSampleId :
BBJC6

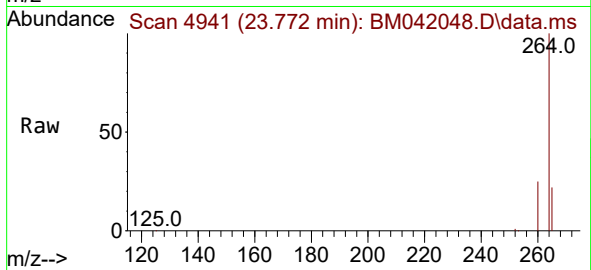

Tgt Ion:252 Resp: 3888
Ion Ratio Lower Upper
252 100
253 60.2 23.2 34.8#
125 54.5 22.5 33.7#

