

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092523\
 Data File : BM042071.D
 Acq On : 26 Sep 2023 15:40
 Operator : MA/JU
 Sample : PB155721BL
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK721

Quant Time: Sep 27 04:26:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 13:50:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	6257	0.400	ng/ul	0.00
4) Naphthalene-d8	10.757	136	16446	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.592	164	7601	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.341	188	15671	0.400	ng/ul	-0.01
17) Chrysene-d12	21.518	240	5586	0.400	ng/ul	0.00
23) Perylene-d12	23.924	264	5567	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	57215	6.710	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.341	152	7539	0.366	ng/ul	-0.01
18) Fluoranthene-d10	19.366	212	9851	0.428	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.587	166	3471	0.079	ng/ul#	13
20) Pyrene	19.733	202	2654	0.043	ng/ul#	1
26) Benzo(a)pyrene	23.766	252	3724	0.106	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092523\
Data File : BM042071.D
Acq On : 26 Sep 2023 15:40
Operator : MA/JU
Sample : PB155721BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK721

Quant Time: Sep 27 04:26:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 13:50:58 2023
Response via : Initial Calibration




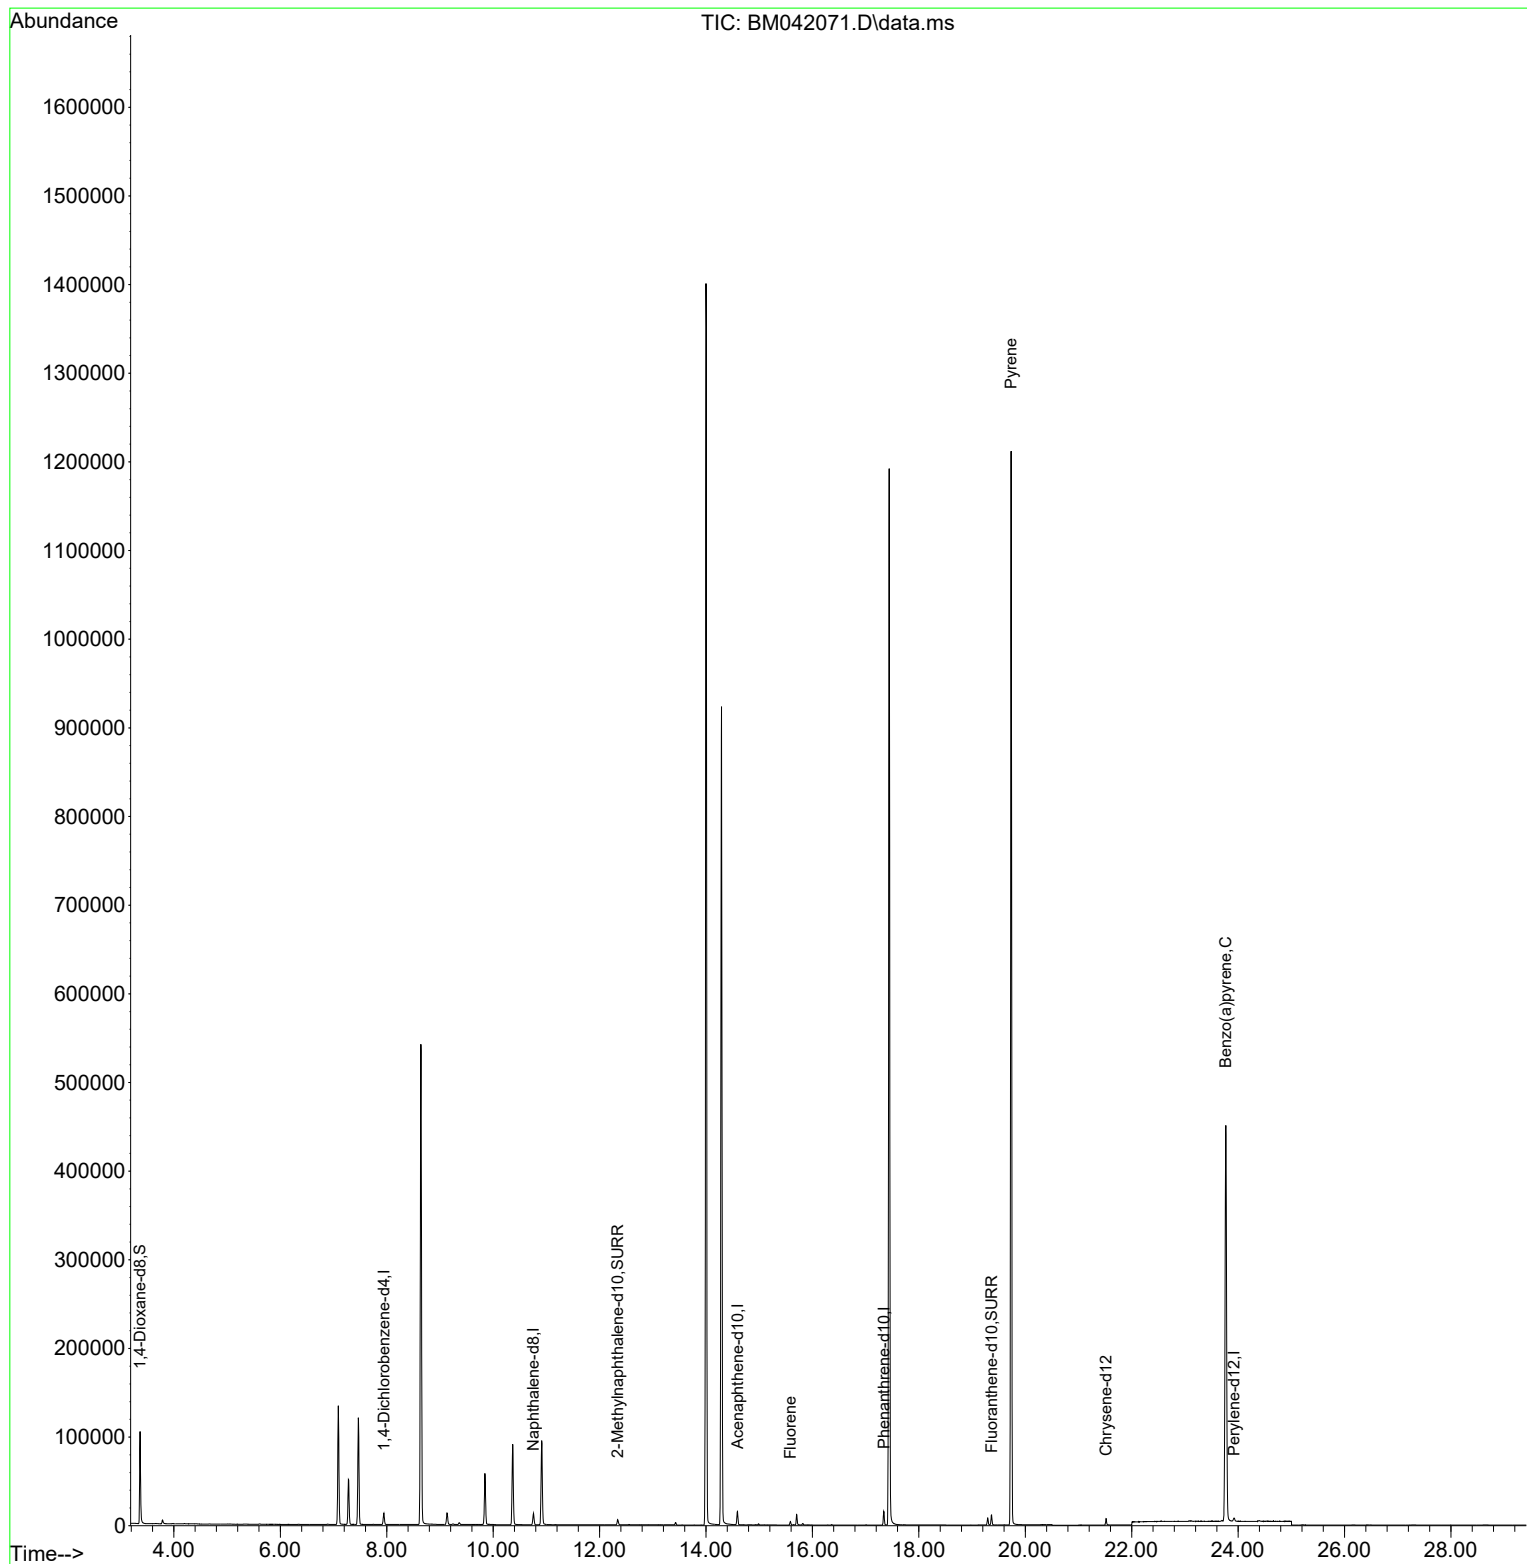


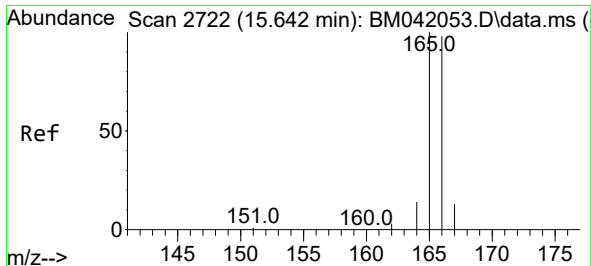

#12
Fluorene
Concen: 0.079 ng/ul
RT: 15.587 min Scan# 21
Delta R.T. -0.065 min
Lab File: BM042071.D
Acq: 26 Sep 2023 15:40




Instrument :
BNA_M
ClientSampleId :
SBLK721


Tgt Ion:166 Resp: 3471
Ion Ratio Lower Upper
166 100
165 7.6 79.8 119.8#
167 34.0 11.1 16.7#

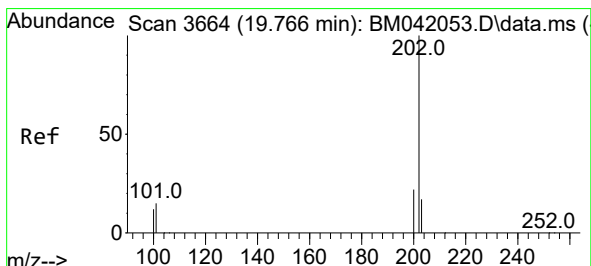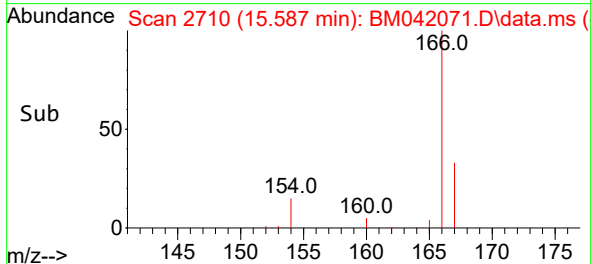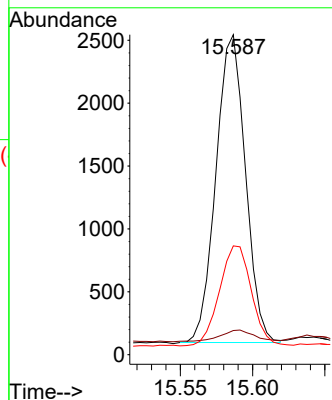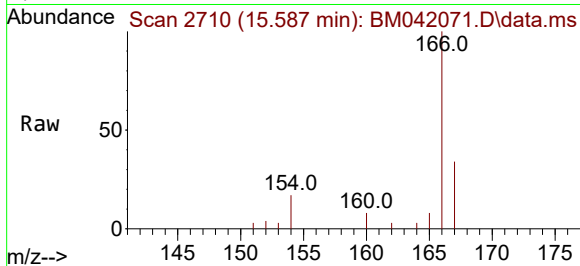

#20
Pyrene
Concen: 0.043 ng/ul
RT: 19.733 min Scan# 3657
Delta R.T. -0.037 min
Lab File: BM042071.D
Acq: 26 Sep 2023 15:40


Tgt Ion:202 Resp: 2654
Ion Ratio Lower Upper
202 100
101 179.8 14.1 21.1#
100 1364.7 11.4 17.0#

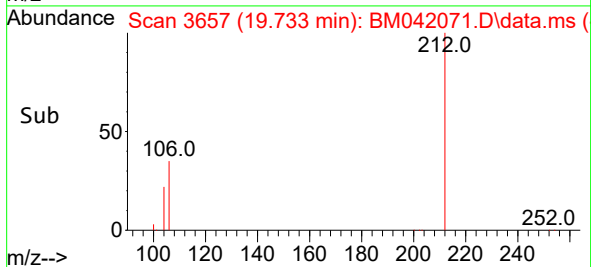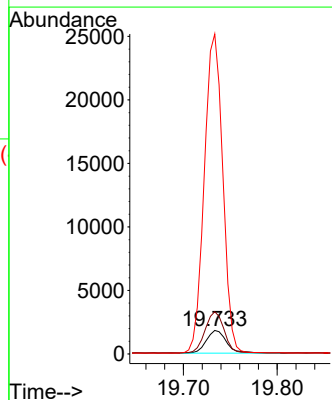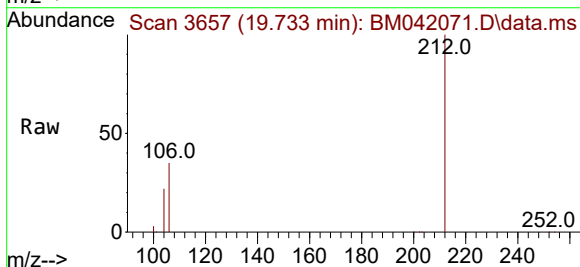

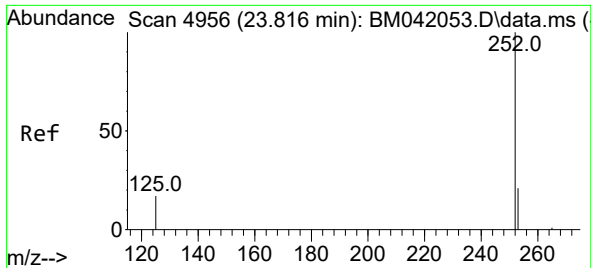

#26
Benzo(a)pyrene
Concen: 0.106 ng/ul
RT: 23.766 min Scan# 4939
Delta R.T. -0.061 min
Lab File: BM042071.D
Acq: 26 Sep 2023 15:40

Instrument :
BNA_M
ClientSampleId :
SBLK721

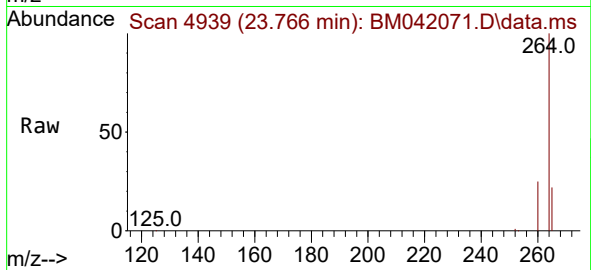

Tgt Ion:252 Resp: 3724
Ion Ratio Lower Upper
252 100
253 52.7 23.2 34.8#
125 50.2 22.5 33.7#

