

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092523\
 Data File : BM042076.D
 Acq On : 26 Sep 2023 18:41
 Operator : MA/JU
 Sample : 04450-03DL 5X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJN8DL

Quant Time: Sep 27 04:26:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 13:50:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	5493	0.400	ng/ul	0.00
4) Naphthalene-d8	10.757	136	14110	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.587	164	6901	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.341	188	13531	0.400	ng/ul	-0.01
17) Chrysene-d12	21.518	240	5349	0.400	ng/ul	0.00
23) Perylene-d12	23.921	264	5221	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.368	96	7073	0.945	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.341	152	1489	0.084	ng/ul	-0.01
18) Fluoranthene-d10	19.366	212	2568	0.117	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.402	88	6138	0.779	ng/ul#	90
26) Benzo(a)pyrene	23.766	252	1071	0.032	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092523\
Data File : BM042076.D
Acq On : 26 Sep 2023 18:41
Operator : MA/JU
Sample : 04450-03DL 5X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJN8DL

Quant Time: Sep 27 04:26:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 13:50:58 2023
Response via : Initial Calibration




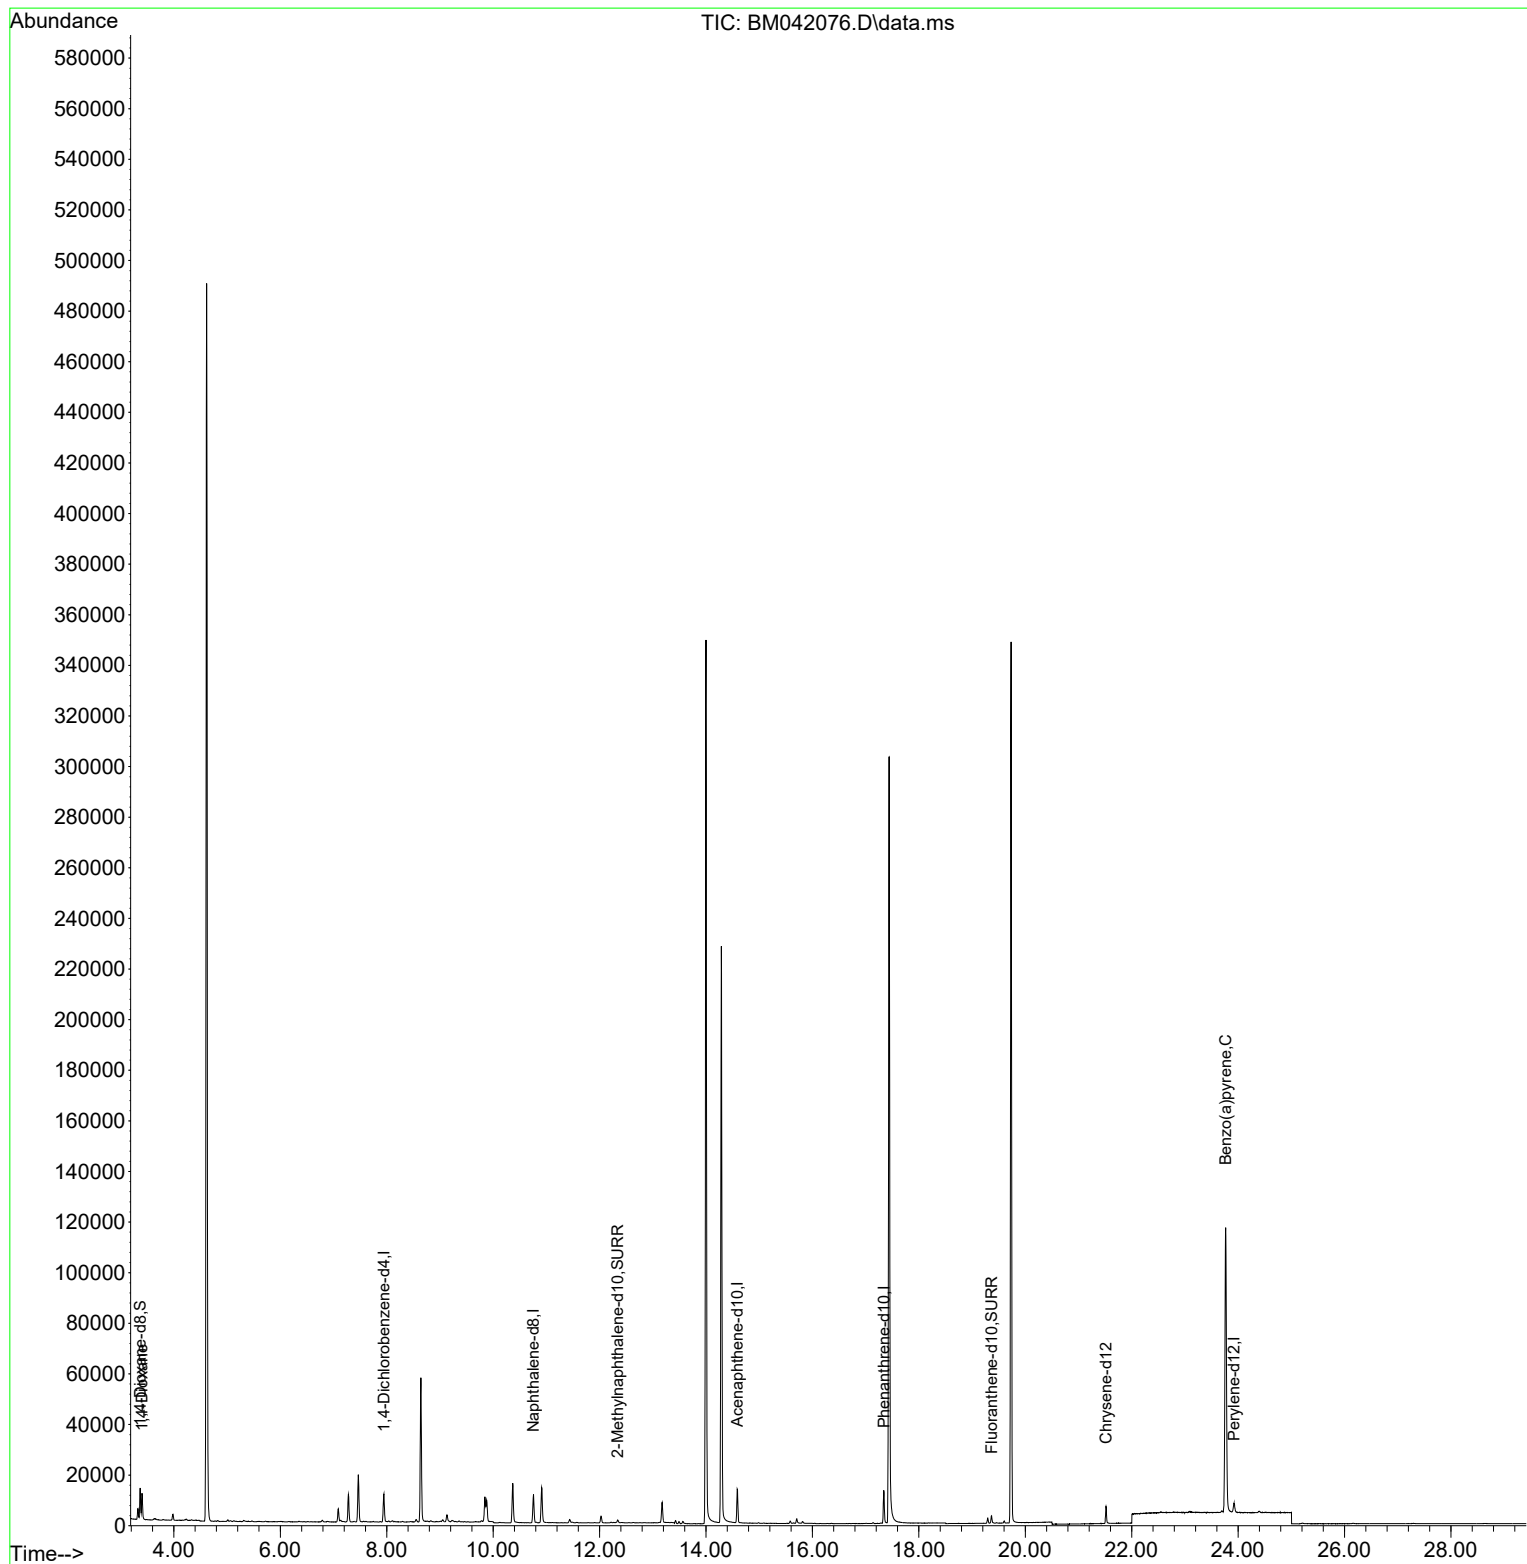


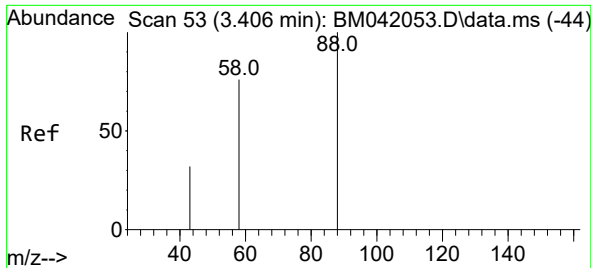

#2
1,4-Dioxane
Concen: 0.779 ng/ul
RT: 3.402 min Scan# 51
Delta R.T. -0.008 min
Lab File: BM042076.D
Acq: 26 Sep 2023 18:41

Instrument :
BNA_M
ClientSampleId :
BBJN8DL

Tgt Ion: 88 Resp: 6138
Ion Ratio Lower Upper
88 100
43 42.3 42.9 64.3#
58 75.3 56.4 84.6

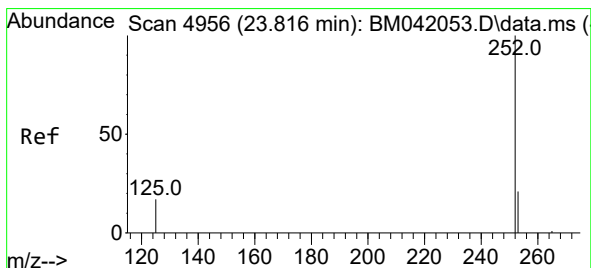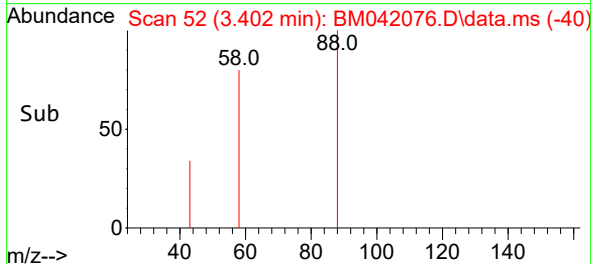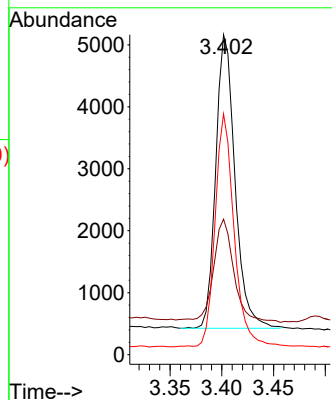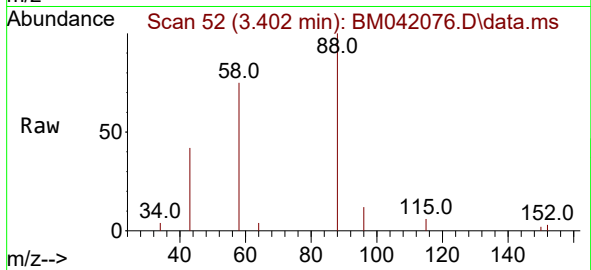

#26
Benzo(a)pyrene
Concen: 0.032 ng/ul
RT: 23.766 min Scan# 4939
Delta R.T. -0.061 min
Lab File: BM042076.D
Acq: 26 Sep 2023 18:41

Tgt Ion: 252 Resp: 1071
Ion Ratio Lower Upper
252 100
253 89.9 23.2 34.8#
125 95.1 22.5 33.7#

