

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092523\
 Data File : BM042026.D
 Acq On : 25 Sep 2023 10:43
 Operator : MA/JU
 Sample : 04385-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EZYP3

Quant Time: Sep 25 12:29:31 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 13:50:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.950	152	4998	0.400	ng/ul	0.00
4) Naphthalene-d8	10.763	136	13344	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.597	164	6333	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.346	188	12090	0.400	ng/ul	0.00
17) Chrysene-d12	21.521	240	4007	0.400	ng/ul	0.00
23) Perylene-d12	23.924	264	3549	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.368	96	32022	4.702	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.346	152	5733	0.343	ng/ul	0.00
18) Fluoranthene-d10	19.371	212	8601	0.521	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.406	88	1668	0.233	ng/ul	90
5) Naphthalene	10.812	128	1737	0.039	ng/ul#	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092523\
Data File : BM042026.D
Acq On : 25 Sep 2023 10:43
Operator : MA/JU
Sample : 04385-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EZYP3

Quant Time: Sep 25 12:29:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 13:50:58 2023
Response via : Initial Calibration




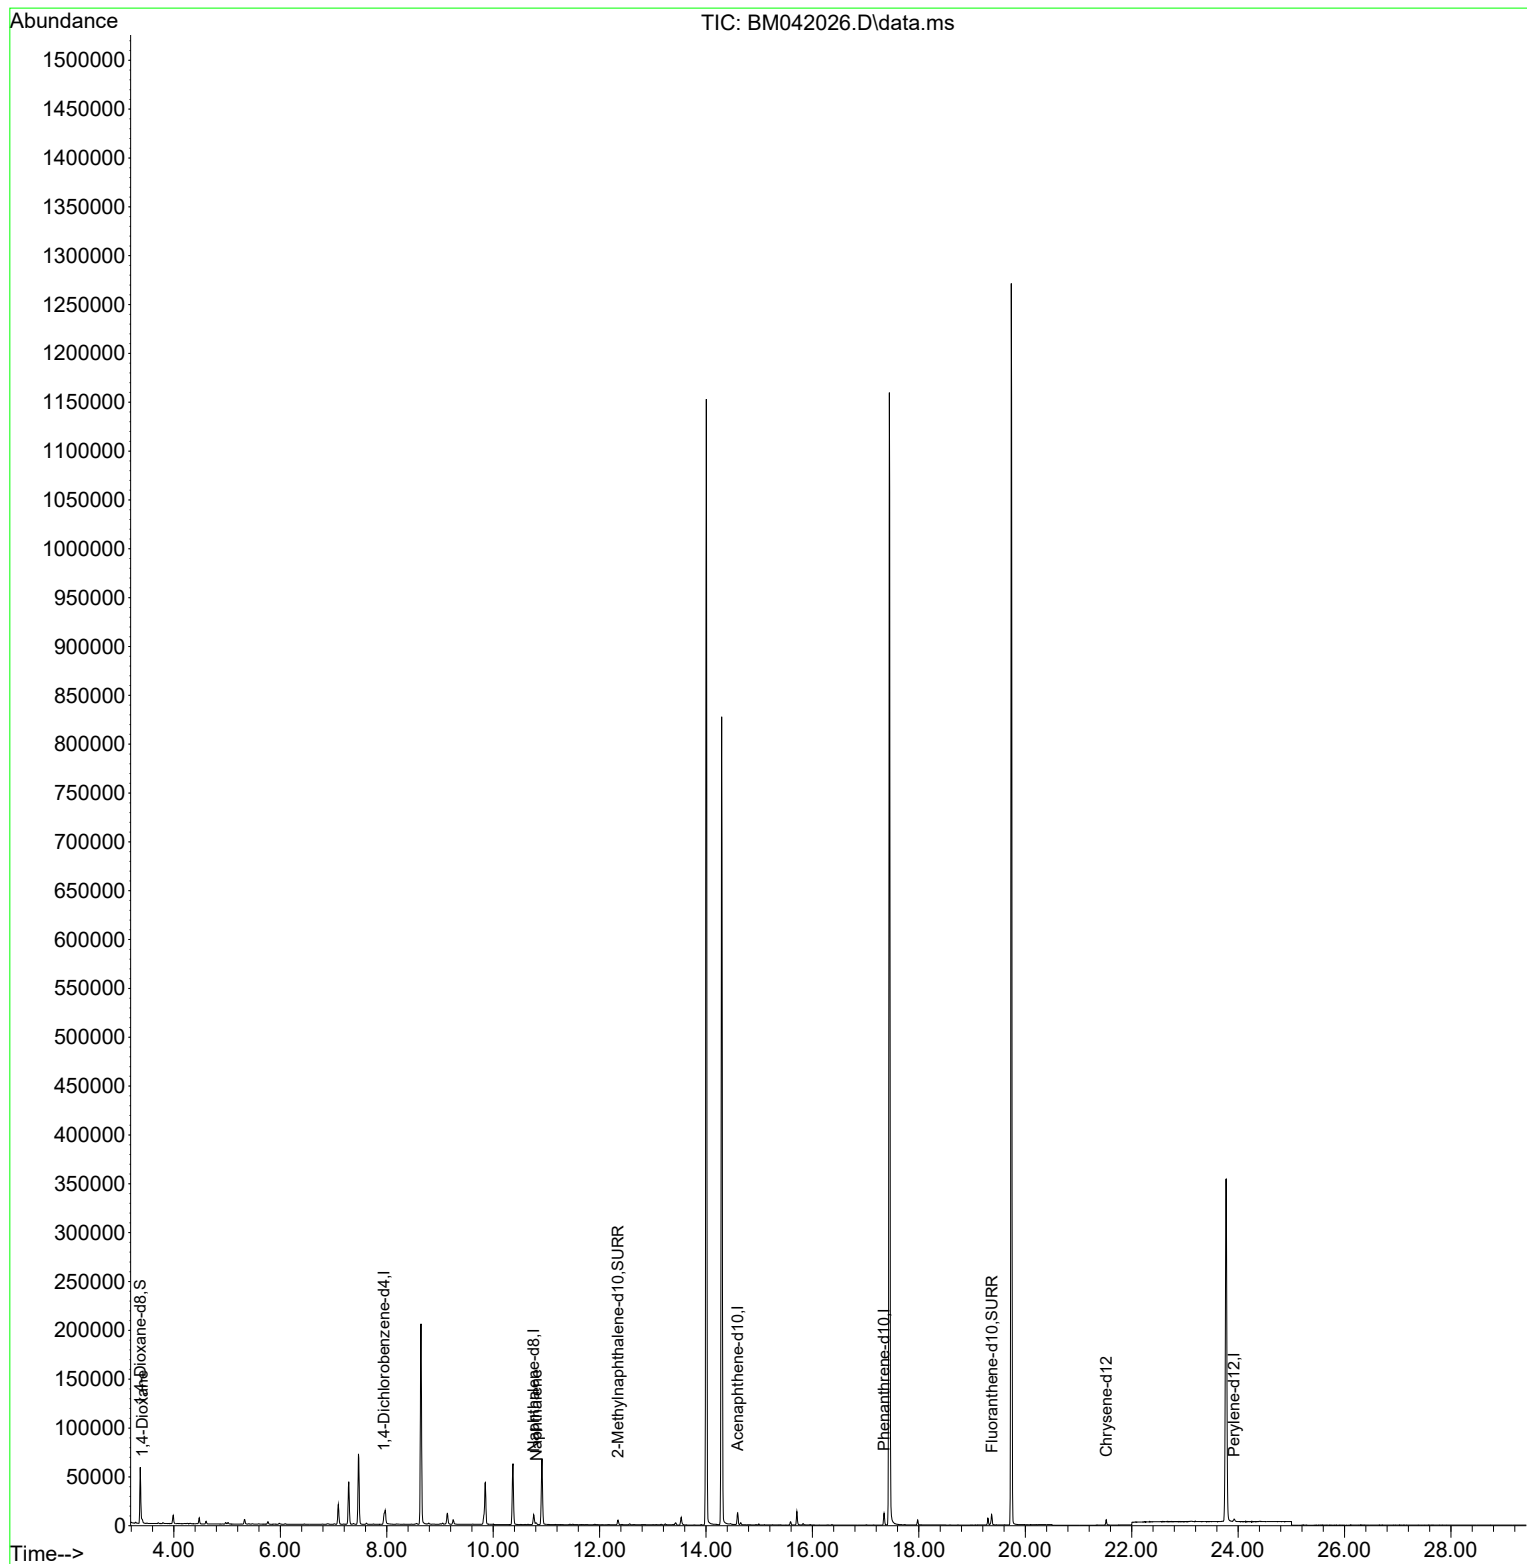


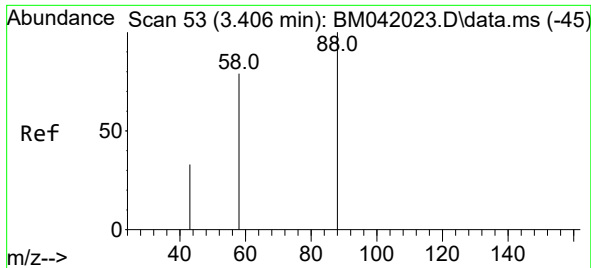

#2
1,4-Dioxane
Concen: 0.233 ng/ul
RT: 3.406 min Scan# 51
Delta R.T. -0.004 min
Lab File: BM042026.D
Acq: 25 Sep 2023 10:43

Instrument :
BNA_M
ClientSampleId :
EZYP3

Tgt Ion: 88 Resp: 1668
Ion Ratio Lower Upper
88 100
43 63.2 42.9 64.3
58 64.6 56.4 84.6

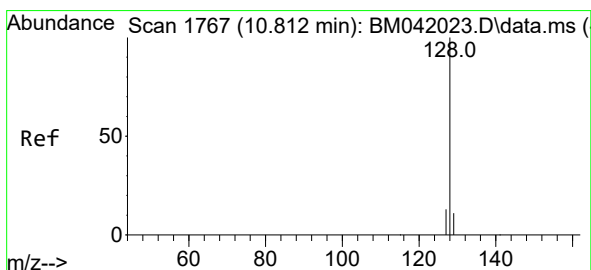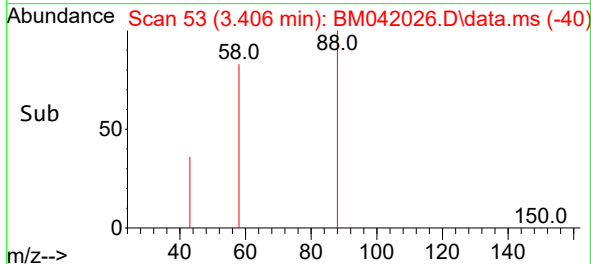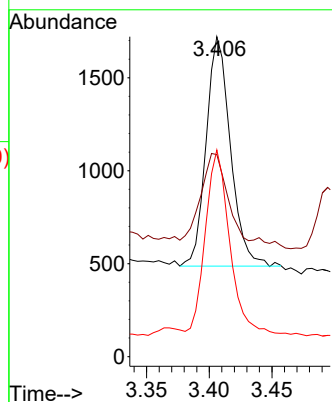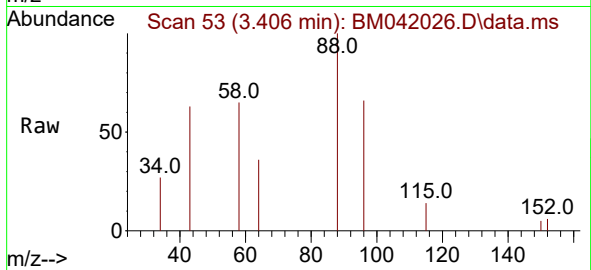

#5
Naphthalene
Concen: 0.039 ng/ul
RT: 10.812 min Scan# 1767
Delta R.T. -0.005 min
Lab File: BM042026.D
Acq: 25 Sep 2023 10:43

Tgt Ion: 128 Resp: 1737
Ion Ratio Lower Upper
128 100
129 19.0 9.2 13.8#
127 18.5 10.8 16.2#

