

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092523\
 Data File : BM042028.D
 Acq On : 25 Sep 2023 11:56
 Operator : MA/JU
 Sample : 04387-16
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AJ8

Quant Time: Sep 25 12:29:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 13:50:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.950	152	6189	0.400	ng/ul	0.00
4) Naphthalene-d8	10.762	136	15531	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.597	164	7076	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.350	188	13312	0.400	ng/ul	0.00
17) Chrysene-d12	21.521	240	4811	0.400	ng/ul	0.00
23) Perylene-d12	23.927	264	4742	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	31182	3.697	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.346	152	5447	0.280	ng/ul	0.00
18) Fluoranthene-d10	19.371	212	7863	0.397	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.406	88	1391	0.157	ng/ul#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092523\
Data File : BM042028.D
Acq On : 25 Sep 2023 11:56
Operator : MA/JU
Sample : 04387-16
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AJ8


Quant Time: Sep 25 12:29:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 13:50:58 2023
Response via : Initial Calibration

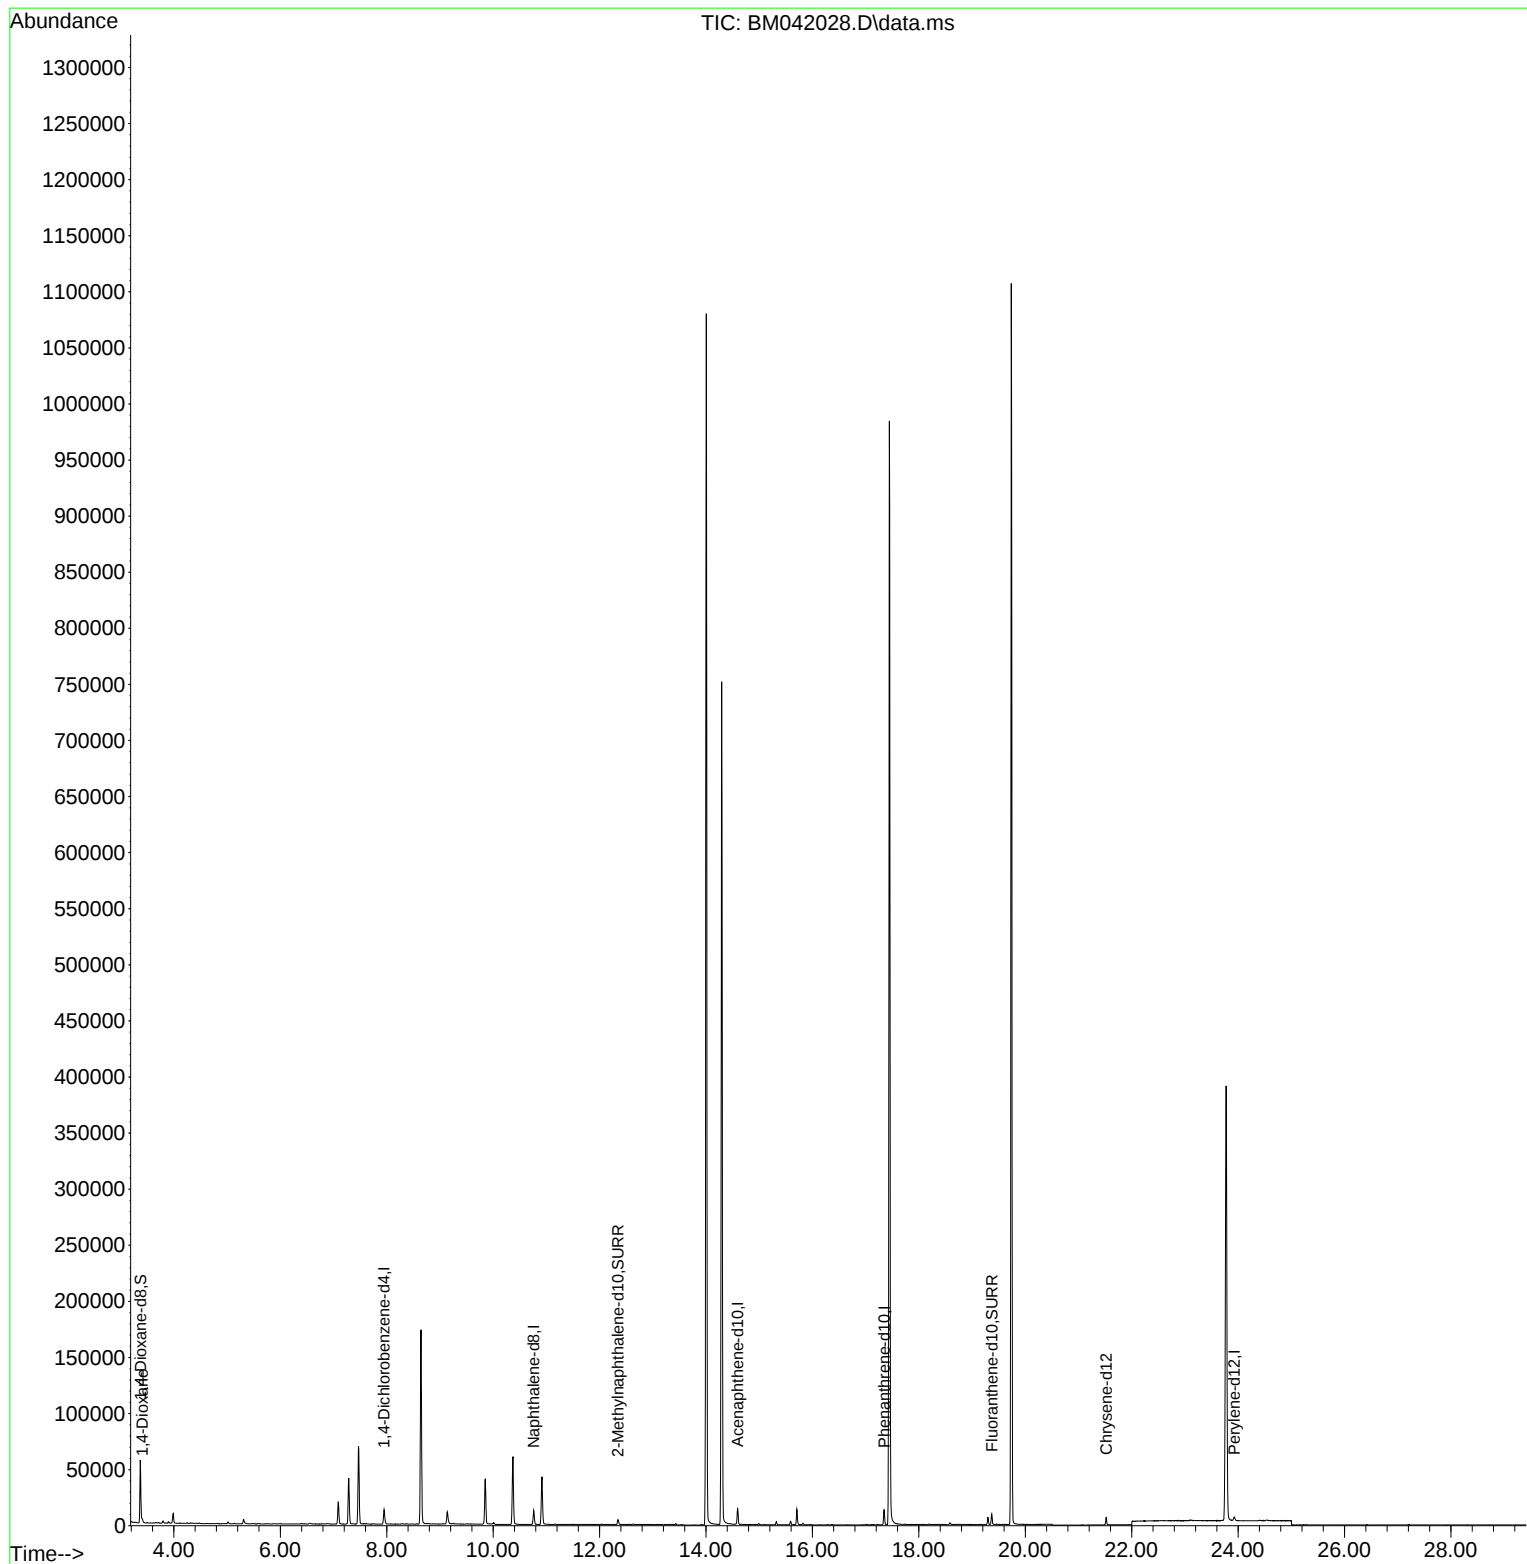

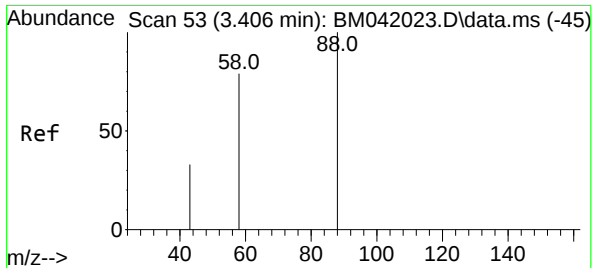

#2
 1,4-Dioxane
 Concen: 0.157 ng/ul
 RT: 3.406 min Scan# 51
 Delta R.T. -0.004 min
 Lab File: BM042028.D
 Acq: 25 Sep 2023 11:56

Instrument :
 BNA_M
 ClientSampleId :
 C0AJ8

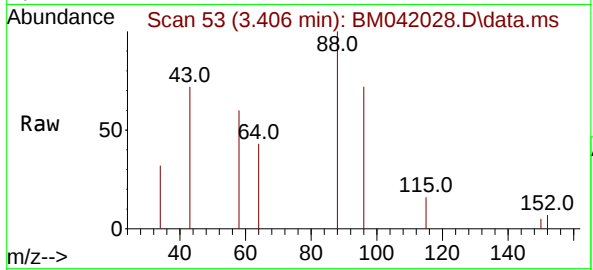

Tgt Ion: 88 Resp: 1391

Ion	Ratio	Lower	Upper
88	100		
43	72.1	42.9	64.3#
58	60.3	56.4	84.6

