

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092523\
 Data File : BM042047.D
 Acq On : 26 Sep 2023 00:01
 Operator : MA/JU
 Sample : 04429-16
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJ42

Quant Time: Sep 26 02:21:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 13:50:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.950	152	6065	0.400	ng/ul	0.00
4) Naphthalene-d8	10.763	136	14955	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.592	164	6847	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.345	188	14847	0.400	ng/ul	0.00
17) Chrysene-d12	21.518	240	7746	0.400	ng/ul	0.00
23) Perylene-d12	23.924	264	7861	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.368	96	28259	3.419	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.346	152	4984	0.266	ng/ul	0.00
18) Fluoranthene-d10	19.366	212	9846	0.309	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.406	88	19805	2.278	ng/ul#	87
5) Naphthalene	10.812	128	1159	0.023	ng/ul#	60
7) 2-Methylnaphthalene	12.418	142	713	0.024	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092523\
Data File : BM042047.D
Acq On : 26 Sep 2023 00:01
Operator : MA/JU
Sample : 04429-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJ42

Quant Time: Sep 26 02:21:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 13:50:58 2023
Response via : Initial Calibration




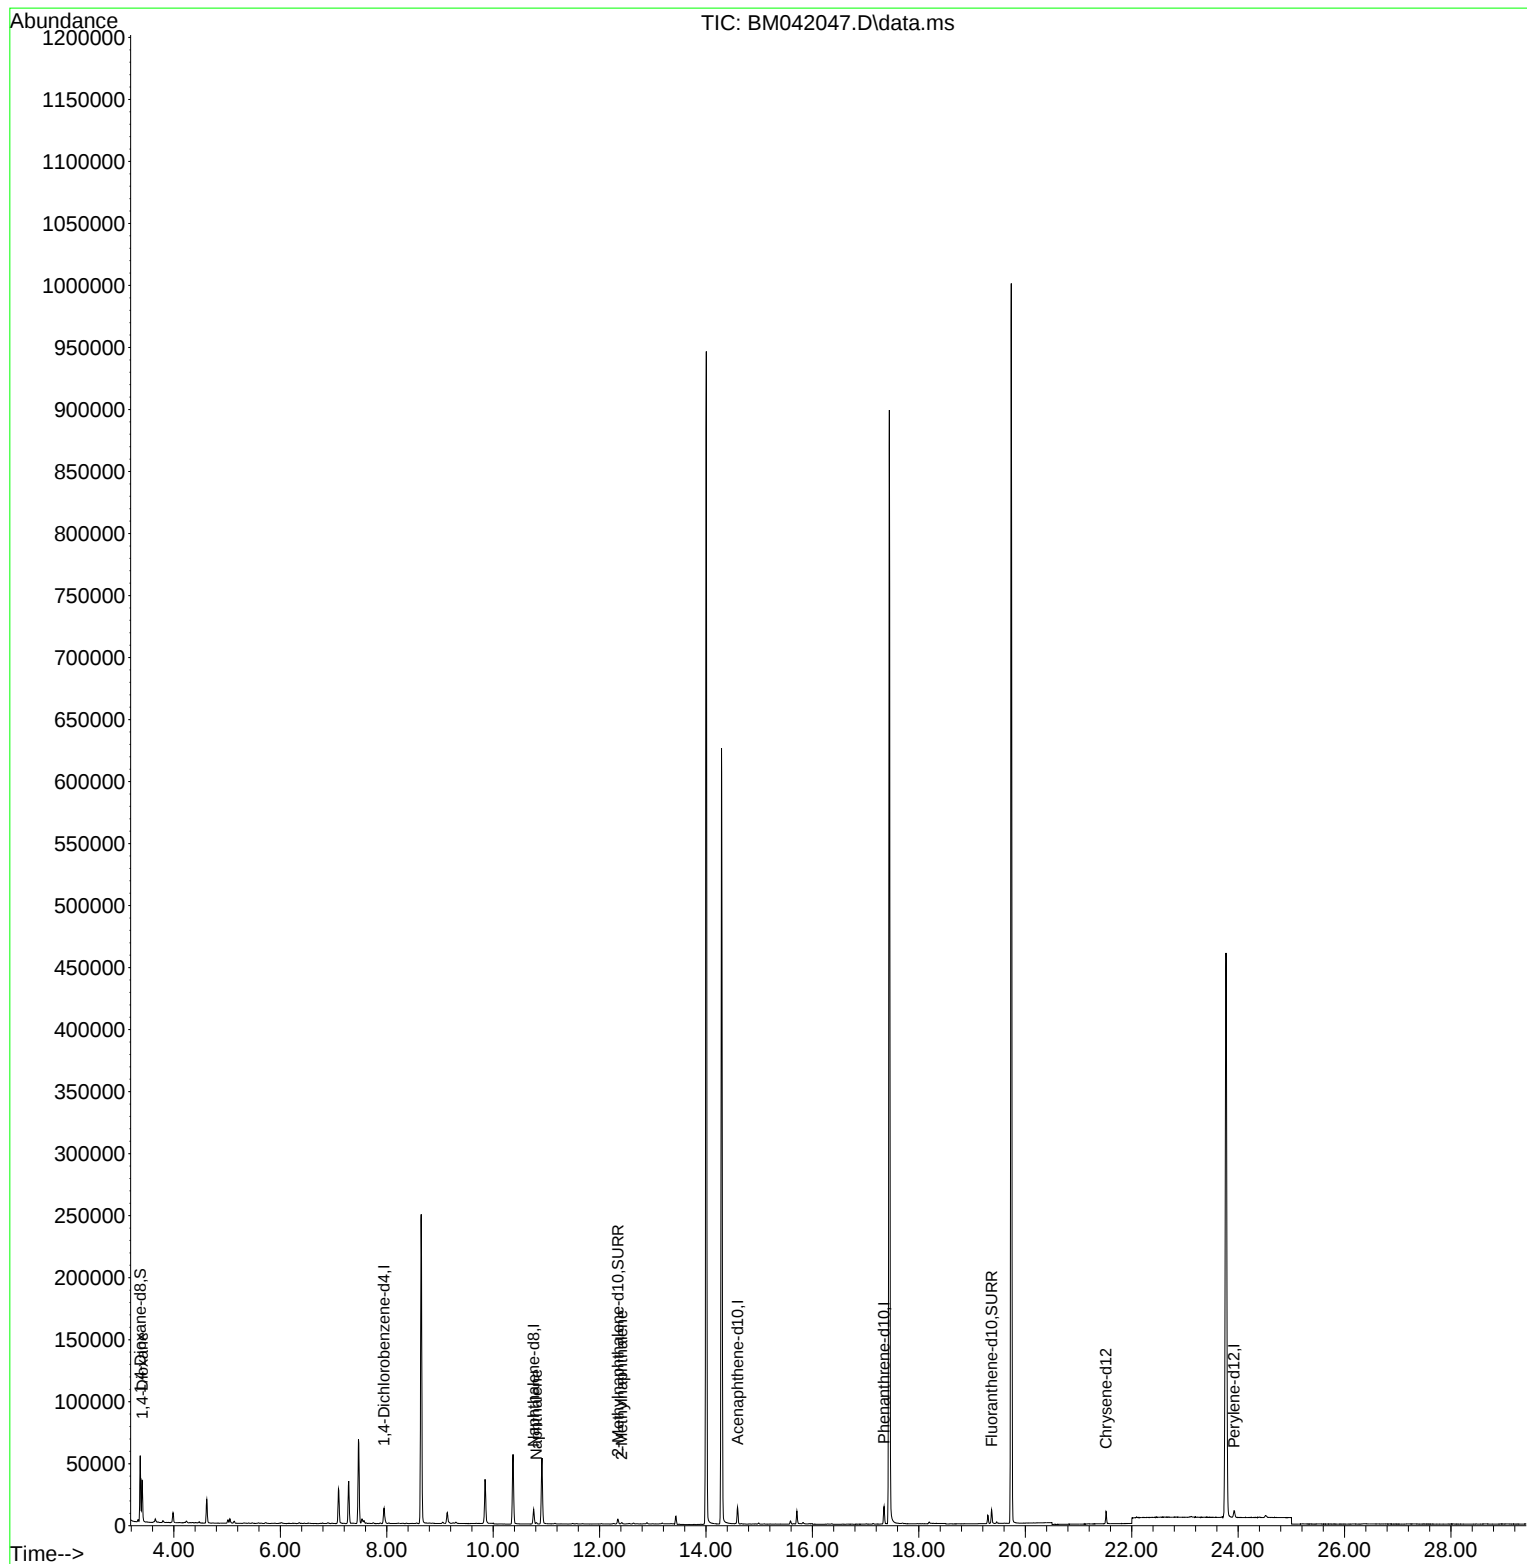


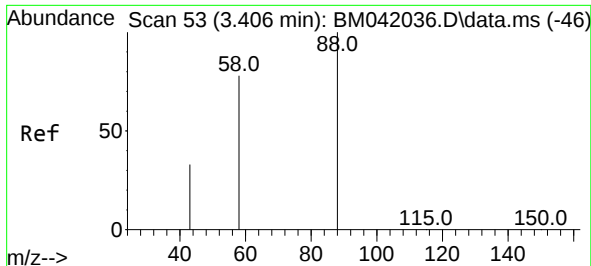

#2
 1,4-Dioxane
 Concen: 2.278 ng/ul
 RT: 3.406 min Scan# 51
 Delta R.T. -0.004 min
 Lab File: BM042047.D
 Acq: 26 Sep 2023 00:01




Instrument :
 BNA_M
 ClientSampleId :
 BBJ42


Tgt Ion: 88 Resp: 19805
 Ion Ratio Lower Upper
 88 100
 43 36.4 42.9 64.3#
 58 73.9 56.4 84.6

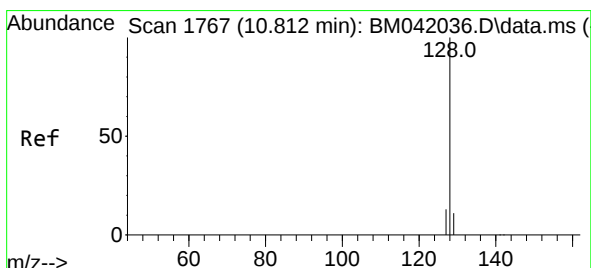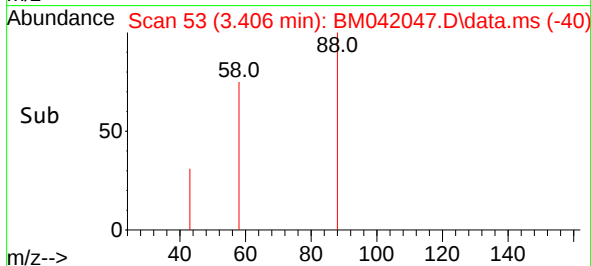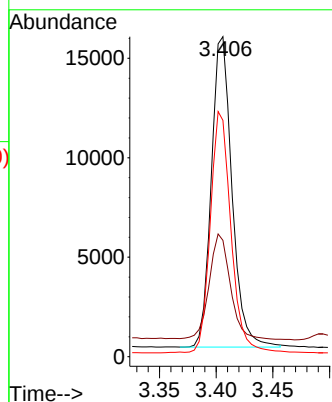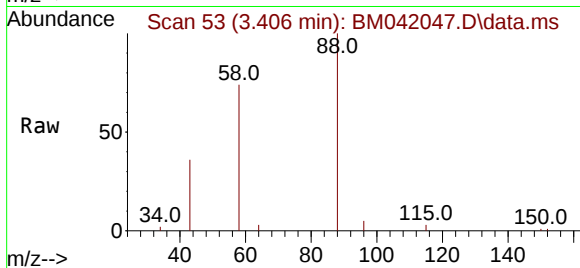

#5
 Naphthalene
 Concen: 0.023 ng/ul
 RT: 10.812 min Scan# 1767
 Delta R.T. -0.005 min
 Lab File: BM042047.D
 Acq: 26 Sep 2023 00:01

Tgt Ion: 128 Resp: 1159
 Ion Ratio Lower Upper
 128 100
 129 27.5 9.2 13.8#
 127 29.0 10.8 16.2#

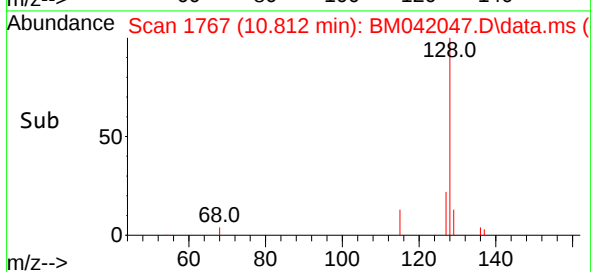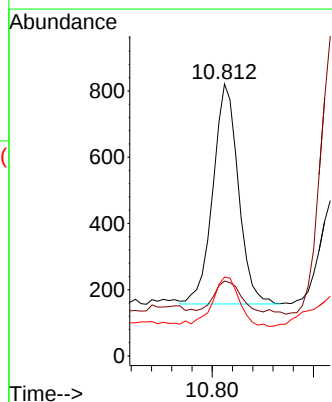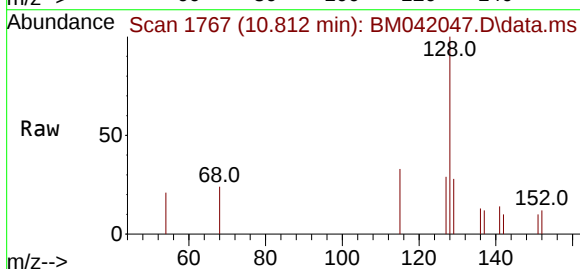

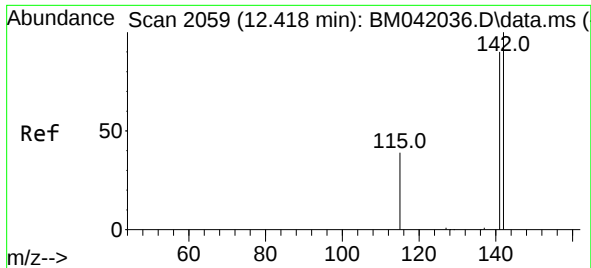

#7
 2-Methylnaphthalene
 Concen: 0.024 ng/ul
 RT: 12.418 min Scan# 2059
 Delta R.T. -0.005 min
 Lab File: BM042047.D
 Acq: 26 Sep 2023 00:01

Instrument :
 BNA_M
 ClientSampleId :
 BBJ42

Tgt Ion:142 Resp: 713
 Ion Ratio Lower Upper
 142 100
 141 93.7 72.1 108.1

