

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092523\
 Data File : BM042048.D
 Acq On : 26 Sep 2023 00:37
 Operator : MA/JU
 Sample : 04429-17
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJC6

Quant Time: Sep 26 02:21:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 13:50:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.950	152	5458	0.400	ng/ul	0.00
4) Naphthalene-d8	10.762	136	13559	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.592	164	6312	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.345	188	13411	0.400	ng/ul	0.00
17) Chrysene-d12	21.518	240	6844	0.400	ng/ul	0.00
23) Perylene-d12	23.927	264	6836	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.368	96	27957	3.759	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.346	152	5673	0.334	ng/ul	0.00
18) Fluoranthene-d10	19.366	212	10415	0.370	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.406	88	10822	1.383	ng/ul#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092523\
Data File : BM042048.D
Acq On : 26 Sep 2023 00:37
Operator : MA/JU
Sample : 04429-17
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJC6

Quant Time: Sep 26 02:21:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 13:50:58 2023
Response via : Initial Calibration

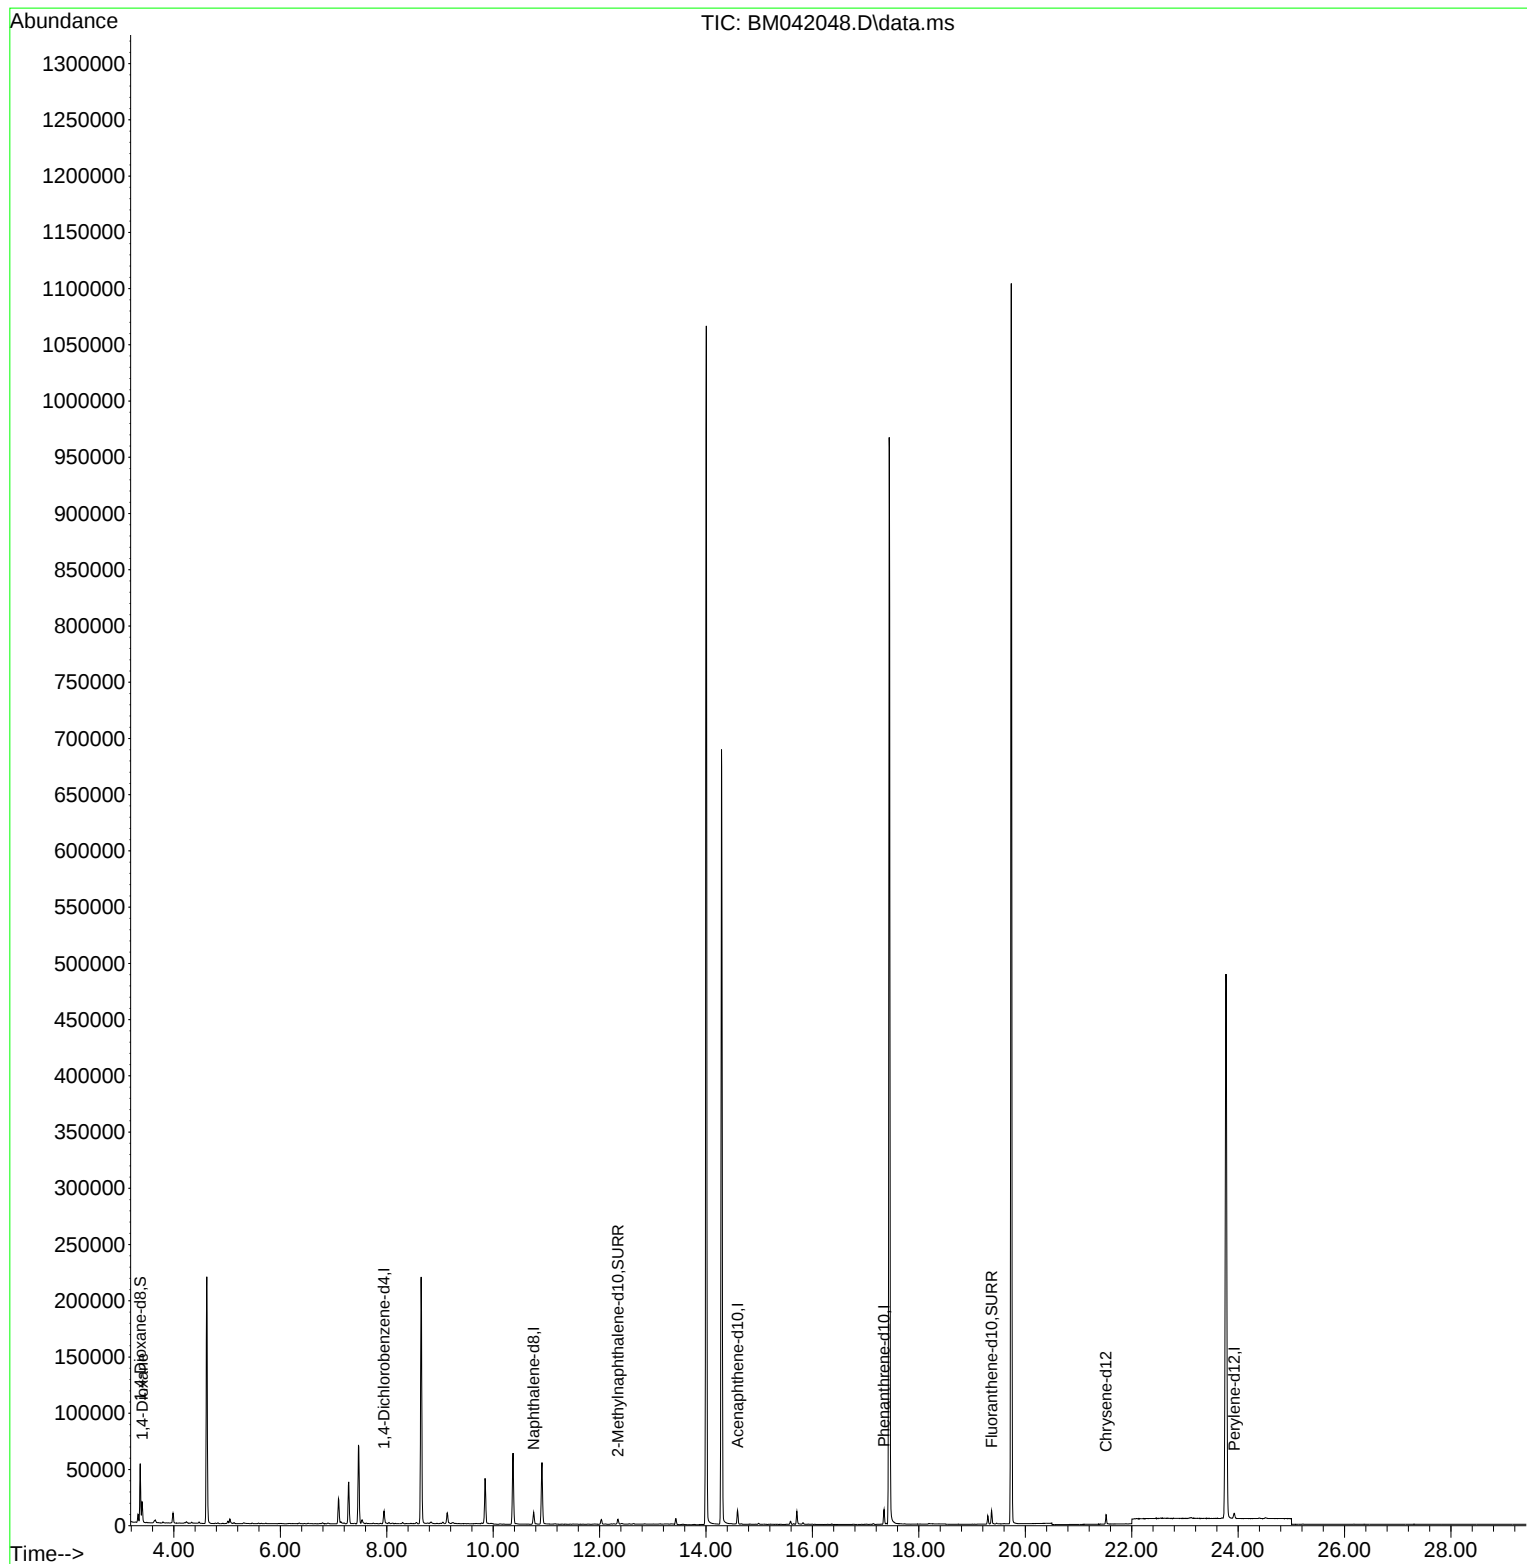

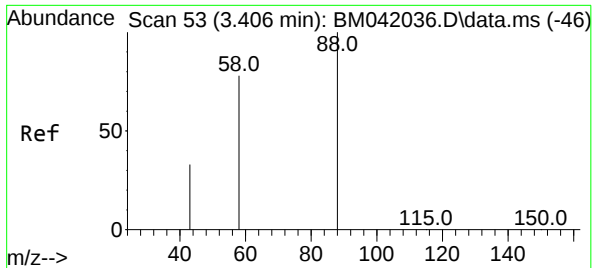

#2
 1,4-Dioxane
 Concen: 1.383 ng/ul
 RT: 3.406 min Scan# 51
 Delta R.T. -0.004 min
 Lab File: BM042048.D
 Acq: 26 Sep 2023 00:37

Instrument :
 BNA_M
 ClientSampleId :
 BBJC6

Tgt Ion:	88	Resp:	10822
Ion	Ratio	Lower	Upper
88	100		
43	39.1	42.9	64.3#
58	74.4	56.4	84.6

