

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092523\
 Data File : BM042049.D
 Acq On : 26 Sep 2023 01:13
 Operator : MA/JU
 Sample : 04429-18
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJ52

Quant Time: Sep 26 02:21:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 13:50:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.950	152	5647	0.400	ng/u1	0.00
4) Naphthalene-d8	10.763	136	14273	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.592	164	6647	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.346	188	14102	0.400	ng/u1	0.00
17) Chrysene-d12	21.518	240	7014	0.400	ng/u1	0.00
23) Perylene-d12	23.924	264	7108	0.400	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.368	96	28224	3.668	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.346	152	6409	0.359	ng/u1	0.00
18) Fluoranthene-d10	19.366	212	11360	0.393	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.406	88	3687	0.455	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092523\
Data File : BM042049.D
Acq On : 26 Sep 2023 01:13
Operator : MA/JU
Sample : 04429-18
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJ52

Quant Time: Sep 26 02:21:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 13:50:58 2023
Response via : Initial Calibration

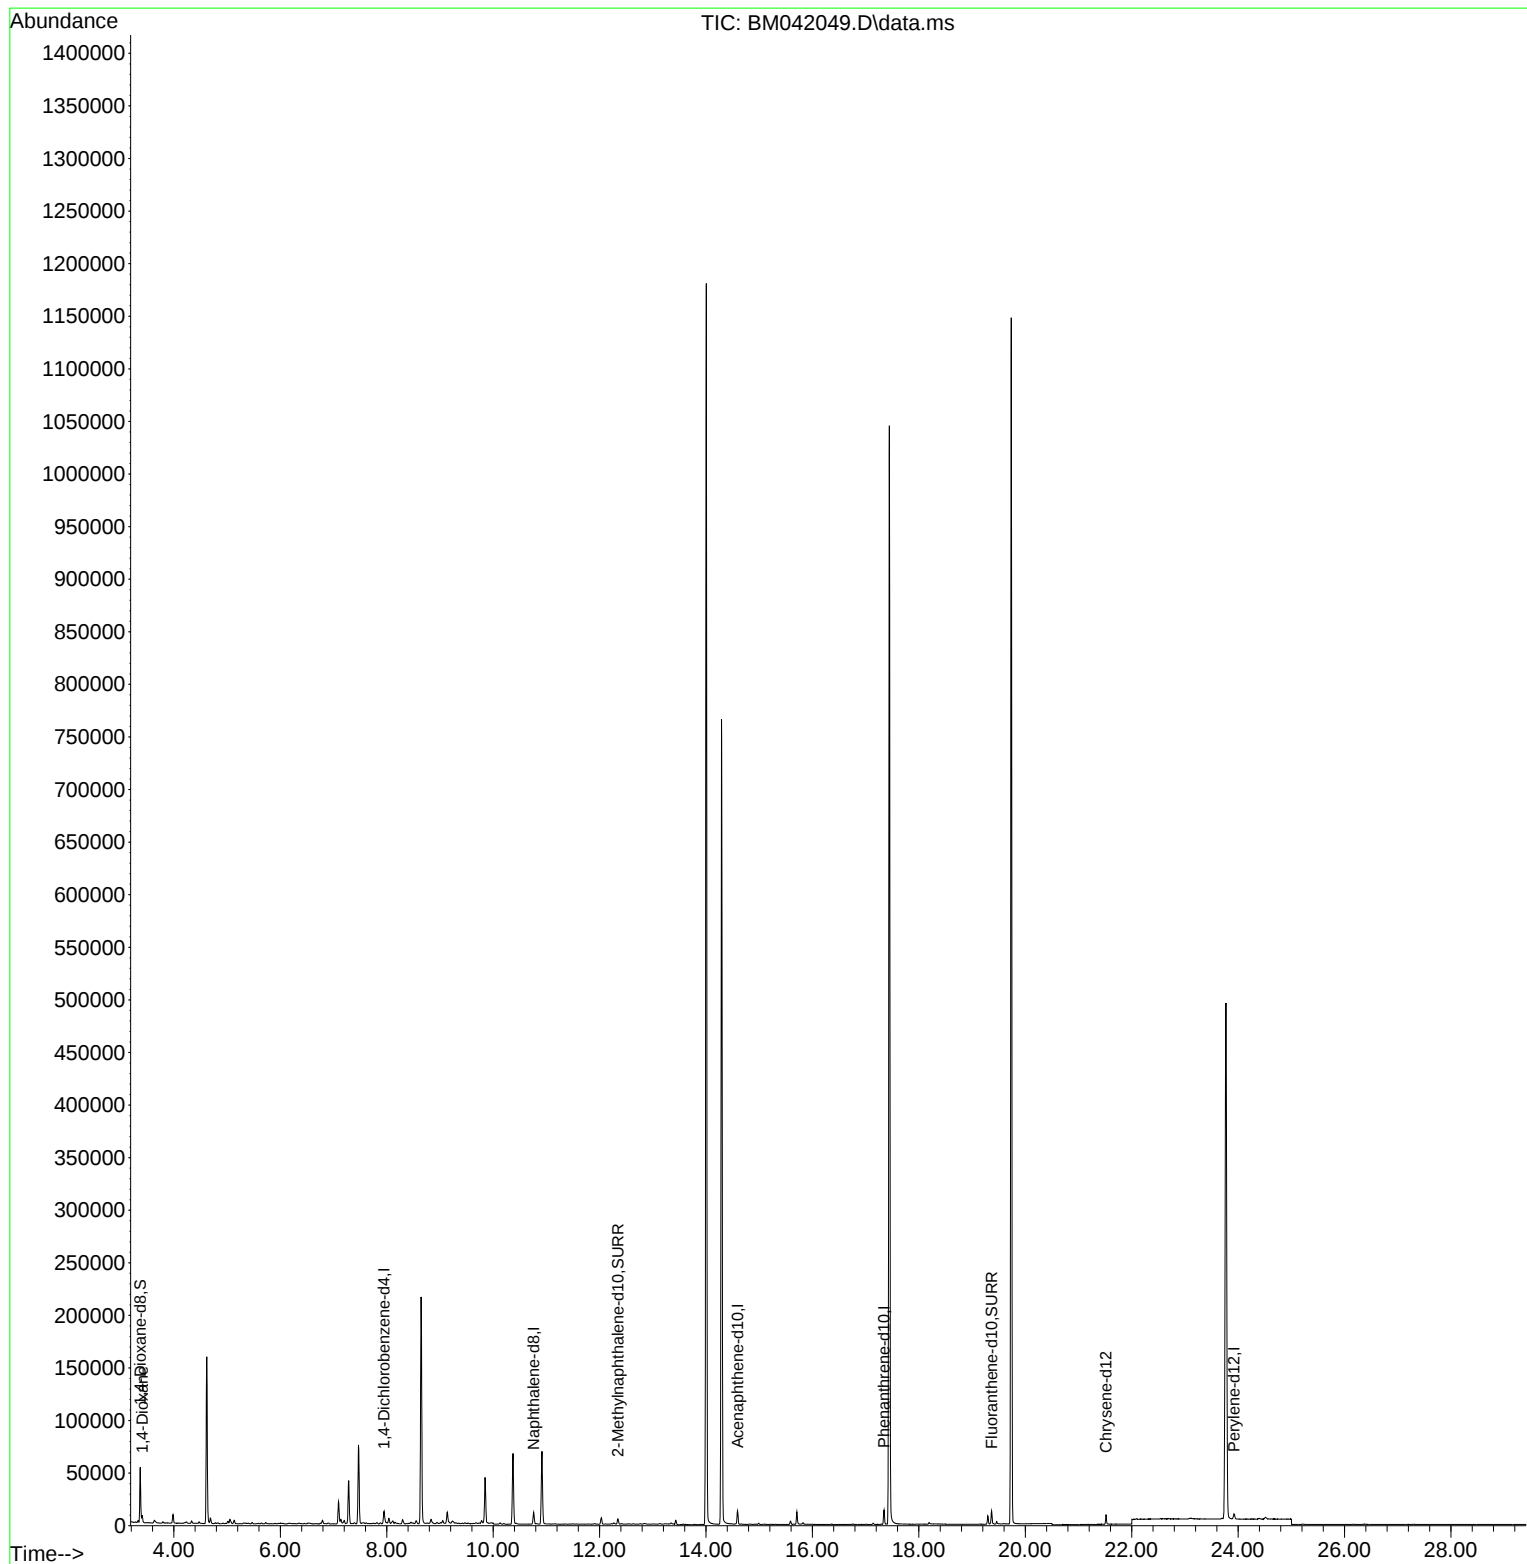

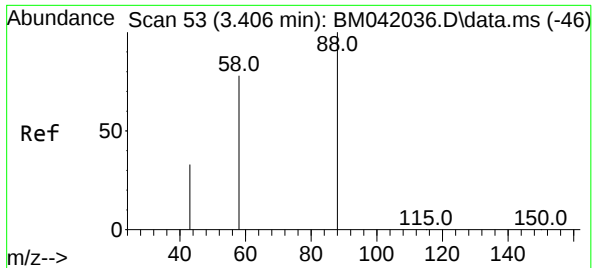

#2
 1,4-Dioxane
 Concen: 0.455 ng/ul
 RT: 3.406 min Scan# 51
 Delta R.T. -0.004 min
 Lab File: BM042049.D
 Acq: 26 Sep 2023 01:13

Instrument :
 BNA_M
 ClientSampleId :
 BBJ52

Tgt Ion: 88 Resp: 3687

Ion	Ratio	Lower	Upper
88	100		
43	52.5	42.9	64.3
58	71.4	56.4	84.6

