

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092523\
 Data File : BM042057.D
 Acq On : 26 Sep 2023 06:36
 Operator : MA/JU
 Sample : 04429-20
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJN6

Quant Time: Sep 26 07:09:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 13:50:58 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	6546	0.400	ng/ul	0.00
4) Naphthalene-d8	10.757	136	16211	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.592	164	7143	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.346	188	14853	0.400	ng/ul	0.00
17) Chrysene-d12	21.515	240	6829	0.400	ng/ul	0.00
23) Perylene-d12	23.921	264	7038	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.368	96	32234	3.614	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.341	152	7713	0.380	ng/ul	-0.01
18) Fluoranthene-d10	19.366	212	12546	0.446	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.402	88	7556	0.805	ng/ul#	89
15) Phenanthrene	17.384	178	1621	0.024	ng/ul#	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Quant Time: Sep 26 07:09:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 13:50:58 2023
Response via : Initial Calibration





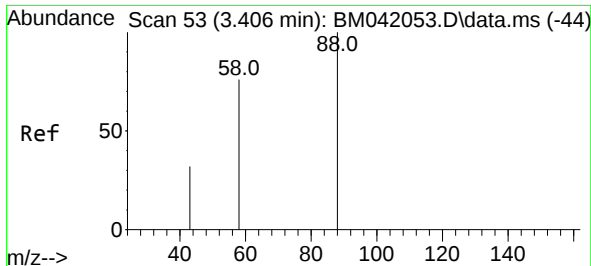


#2
1,4-Dioxane
Concen: 0.805 ng/ul
RT: 3.402 min Scan# 51
Delta R.T. -0.008 min
Lab File: BM042057.D
Acq: 26 Sep 2023 06:36


Instrument :
BNA_M
ClientSampleId :
BBJN6

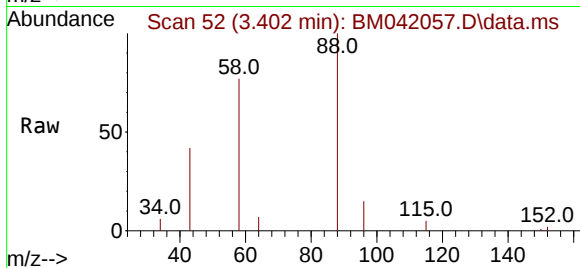

Tgt Ion: 88 Resp: 7556
Ion Ratio Lower Upper
88 100
43 41.7 42.9 64.3#
58 76.5 56.4 84.6

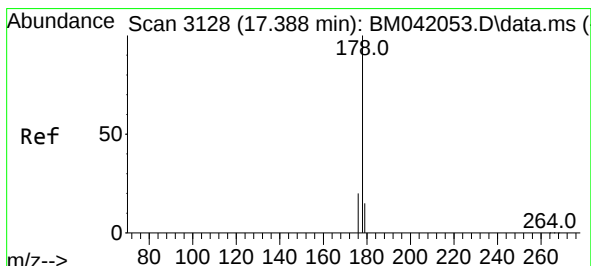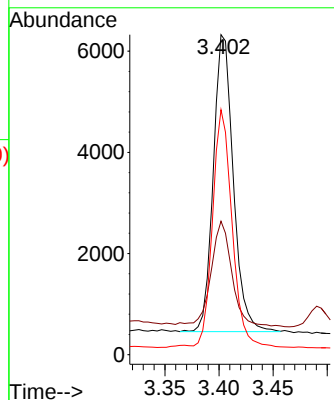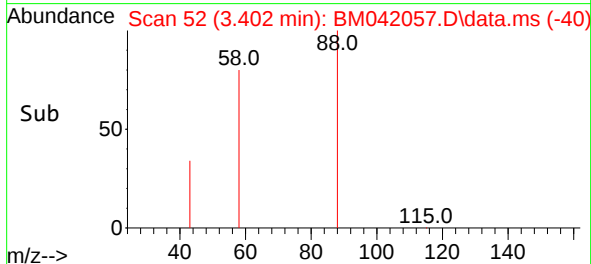

#15
Phenanthrene
Concen: 0.024 ng/ul
RT: 17.384 min Scan# 3127
Delta R.T. -0.013 min
Lab File: BM042057.D
Acq: 26 Sep 2023 06:36

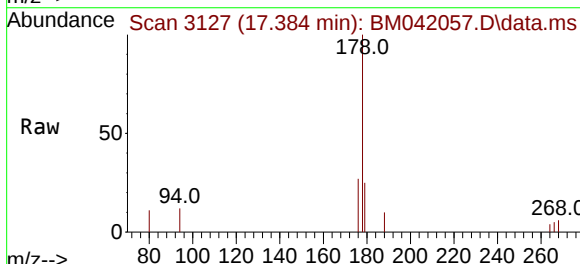

Tgt Ion: 178 Resp: 1621
Ion Ratio Lower Upper
178 100
179 24.7 12.7 19.1#
176 27.0 16.6 24.8#

