

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092524\
 Data File : BM047631.D
 Acq On : 25 Sep 2024 18:56
 Operator : RC/JU
 Sample : P4130-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0H10

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/26/2024
 Supervised By :mohammad ahmed 09/27/2024

Quant Time: Sep 26 02:53:25 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 25 16:27:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.830	152	5452	0.400	ng/u1	0.00
4) Naphthalene-d8	10.622	136	16583	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.459	164	8769	0.400	ng/u1	# 0.00
13) Phenanthrene-d10	17.195	188	17952m	0.400	ng/u1	0.00
17) Chrysene-d12	21.359	240	13352	0.400	ng/u1	0.00
23) Perylene-d12	23.639	264	13045m	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	36843	5.260	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.211	152	6234	0.282	ng/u1	0.00
18) Fluoranthene-d10	19.215	212	16640	0.407	ng/u1	0.00
Target Compounds						Qvalue
14) Pentachlorophenol	16.845	266	984	0.182	ng/u1	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092524\
Data File : BM047631.D
Acq On : 25 Sep 2024 18:56
Operator : RC/JU
Sample : P4130-06
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
H0H10

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/26/2024
Supervised By :mohammad ahmed 09/27/2024


Quant Time: Sep 26 02:53:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 25 16:27:08 2024
Response via : Initial Calibration

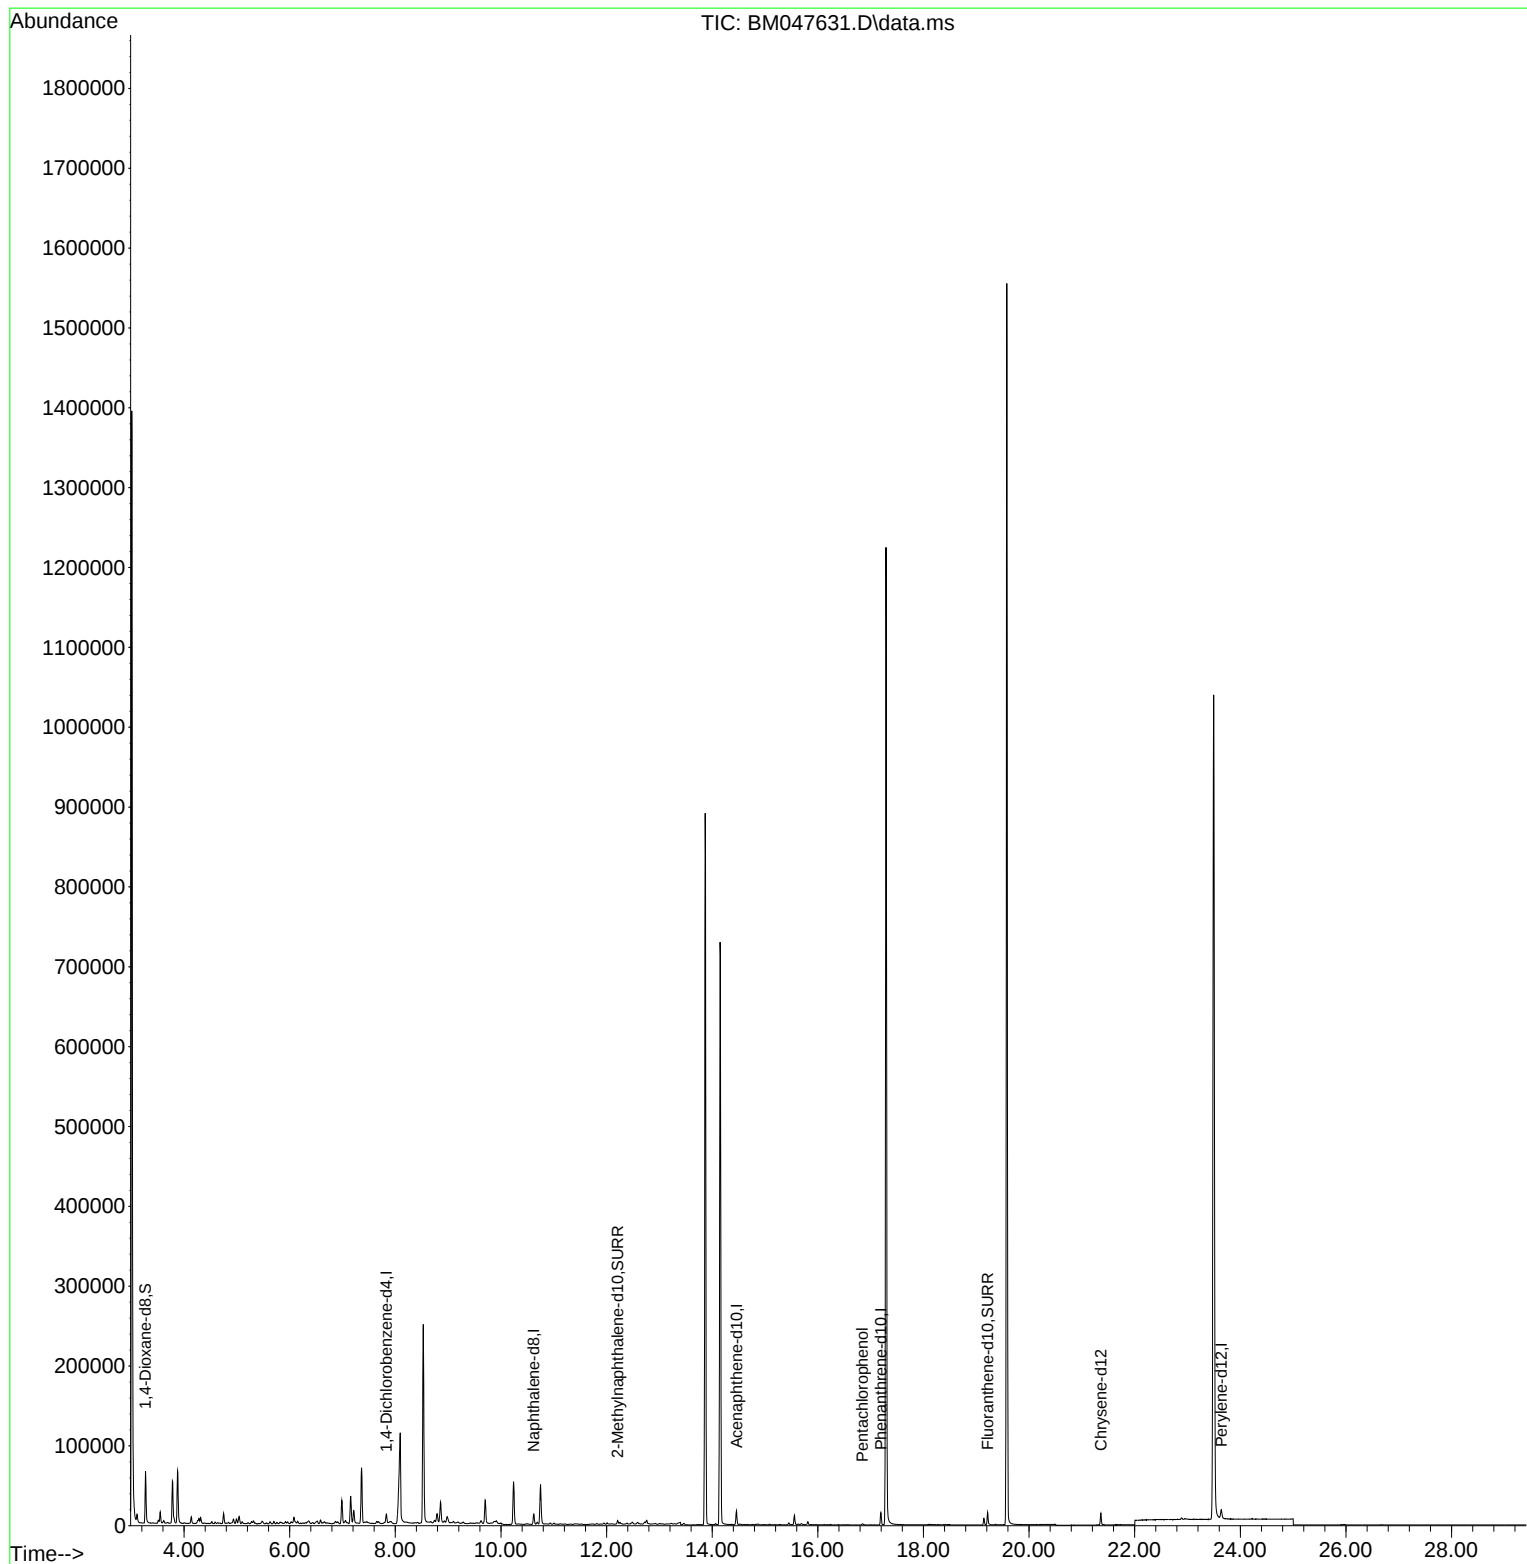

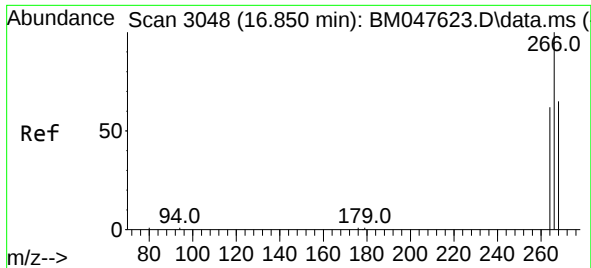

#14
 Pentachlorophenol
 Concen: 0.182 ng/ul
 RT: 16.845 min Scan# 3047
 Delta R.T. -0.005 min
 Lab File: BM047631.D
 Acq: 25 Sep 2024 18:56

Instrument :
 BNA_M
 ClientSampleId :
 H0H10

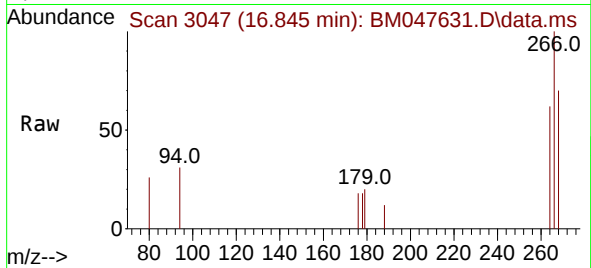

Tgt Ion:266	Resp:	984
Ion Ratio	Lower	Upper
266	100	
264	60.4	49.8 74.8
268	65.8	51.2 76.8

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/26/2024
 Supervised By :mohammad ahmed 09/27/2024

