

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092618\
 Data File : BM016905.D
 Acq On : 26 Sep 2018 18:37
 Operator : MJ/SJ
 Sample : J5040-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Sep 27 02:43:27 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 27 02:42:56 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	295740	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	1211058	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.36	164	639301	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	1426016	20.00	ng/ul	0.00
78) Chrysene-d12	21.29	240	1571705	20.00	ng/ul	0.00
86) Perylene-d12	23.53	264	1688233	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.26	96	16508	2.39	ng/uL	0.00
5) Phenol-d5	6.89	99	392940	15.75	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	238409	15.43	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	333989	16.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	287359	14.89	ng/ul	0.00
19) Nitrobenzene-d5	8.87	128	154344	19.39	ng/ul	0.00
22) 2-Nitrophenol-d4	9.58	143	156961	21.70	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	309207	16.82	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	344052	15.50	ng/ul	0.00
44) Dimethylphthalate-d6	13.77	166	884324	17.23	ng/ul	0.00
47) Acenaphthylene-d8	14.04	160	1139688	17.19	ng/ul	0.00
52) 4-Nitrophenol-d4	14.56	143	108689	12.90	ng/ul	0.00
58) Fluorene-d10	15.35	176	799917	17.85	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.47	200	66719	11.40	ng/ul	0.00
71) Anthracene-d10	17.20	188	1197065	17.40	ng/ul	0.00
79) Pyrene-d10	19.50	212	1389612	18.22	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.39	264	1589840	18.05	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.82	163	286708	5.715	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092618\
Data File : BM016905.D
Acq On : 26 Sep 2018 18:37
Operator : MJ/SJ
Sample : J5040-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Sep 27 02:43:27 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 27 02:42:56 2018
Response via : Initial Calibration

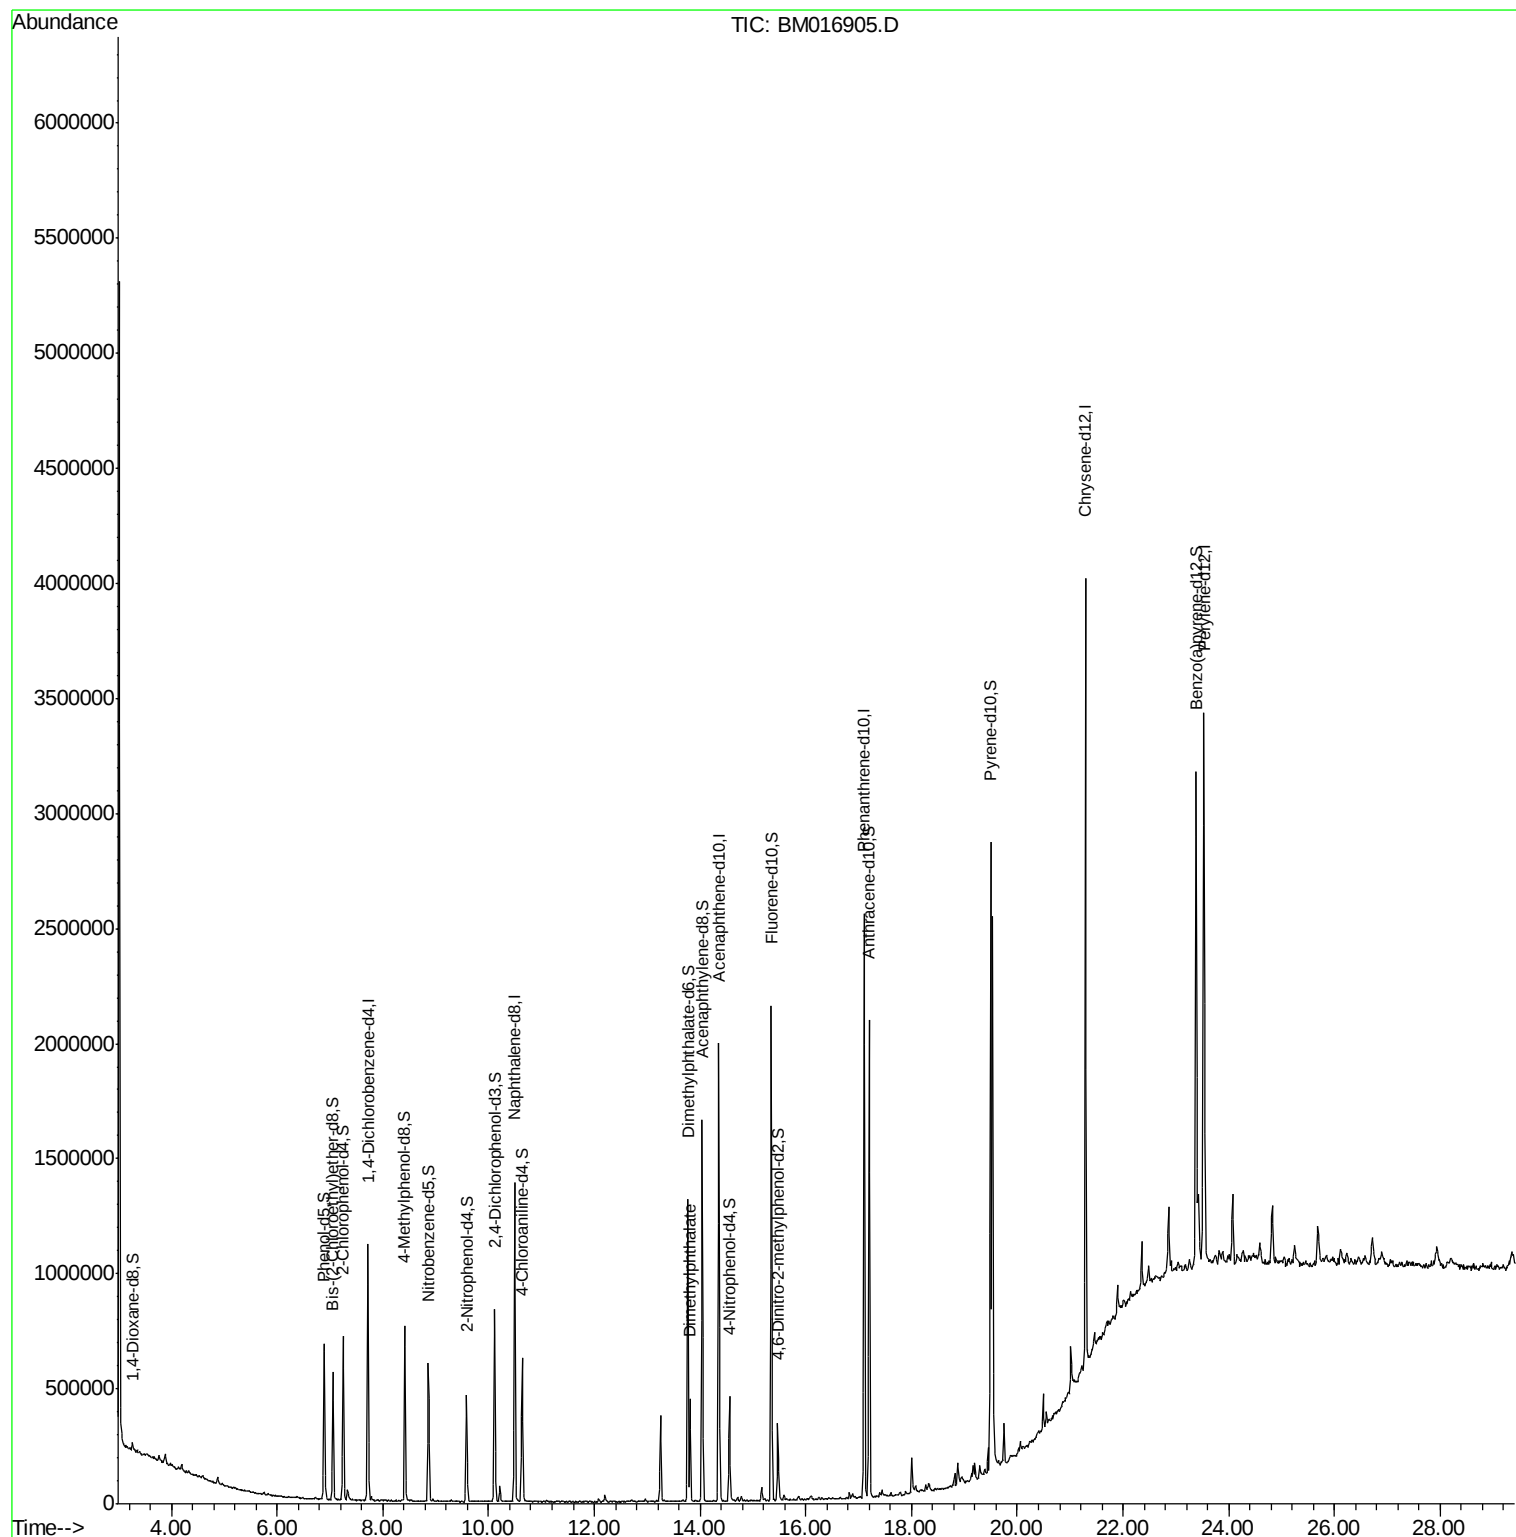


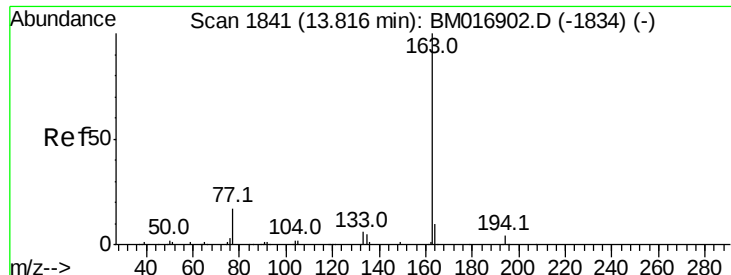

#45
 Dimethylphthalate
 Concen: 5.715 ng/ul
 RT: 13.82 min Scan# 1841
 Delta R.T. 0.00 min
 Lab File: BM016905.D
 Acq: 26 Sep 2018 18:37

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.3	4.0	6.0
164	10.0	8.4	12.6

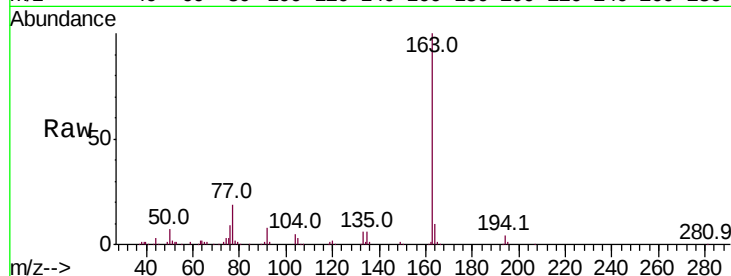

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

