

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092618\
 Data File : BM016897.D
 Acq On : 26 Sep 2018 13:46
 Operator : MJ/SJ
 Sample : J5011-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BE9G3

Quant Time: Sep 27 01:23:17 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 27 01:22:07 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	219734	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	920216	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.35	164	490950	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	1072013	20.00	ng/ul	0.00
78) Chrysene-d12	21.29	240	1206472	20.00	ng/ul	0.00
86) Perylene-d12	23.52	264	1343385	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.26	96	14144	2.75	ng/uL	0.00
5) Phenol-d5	6.89	99	304596	16.44	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	197357	17.20	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	258197	17.07	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	239643	16.71	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	119291	19.73	ng/ul	0.00
22) 2-Nitrophenol-d4	9.58	143	113243	20.60	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.11	165	229606	16.44	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	326169	19.34	ng/ul	0.00
44) Dimethylphthalate-d6	13.76	166	677419	17.18	ng/ul	0.00
47) Acenaphthylene-d8	14.05	160	873749	17.16	ng/ul	0.00
52) 4-Nitrophenol-d4	14.55	143	72226	11.16	ng/ul	0.00
58) Fluorene-d10	15.35	176	628611	18.27	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.46	200	54266	12.33	ng/ul	0.00
71) Anthracene-d10	17.20	188	942117	18.22	ng/ul	0.00
79) Pyrene-d10	19.50	212	1052947	17.99	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.38	264	1255315	17.91	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.81	163	290840	7.549	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092618\
Data File : BM016897.D
Acq On : 26 Sep 2018 13:46
Operator : MJ/SJ
Sample : J5011-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE9G3

Quant Time: Sep 27 01:23:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 27 01:22:07 2018
Response via : Initial Calibration

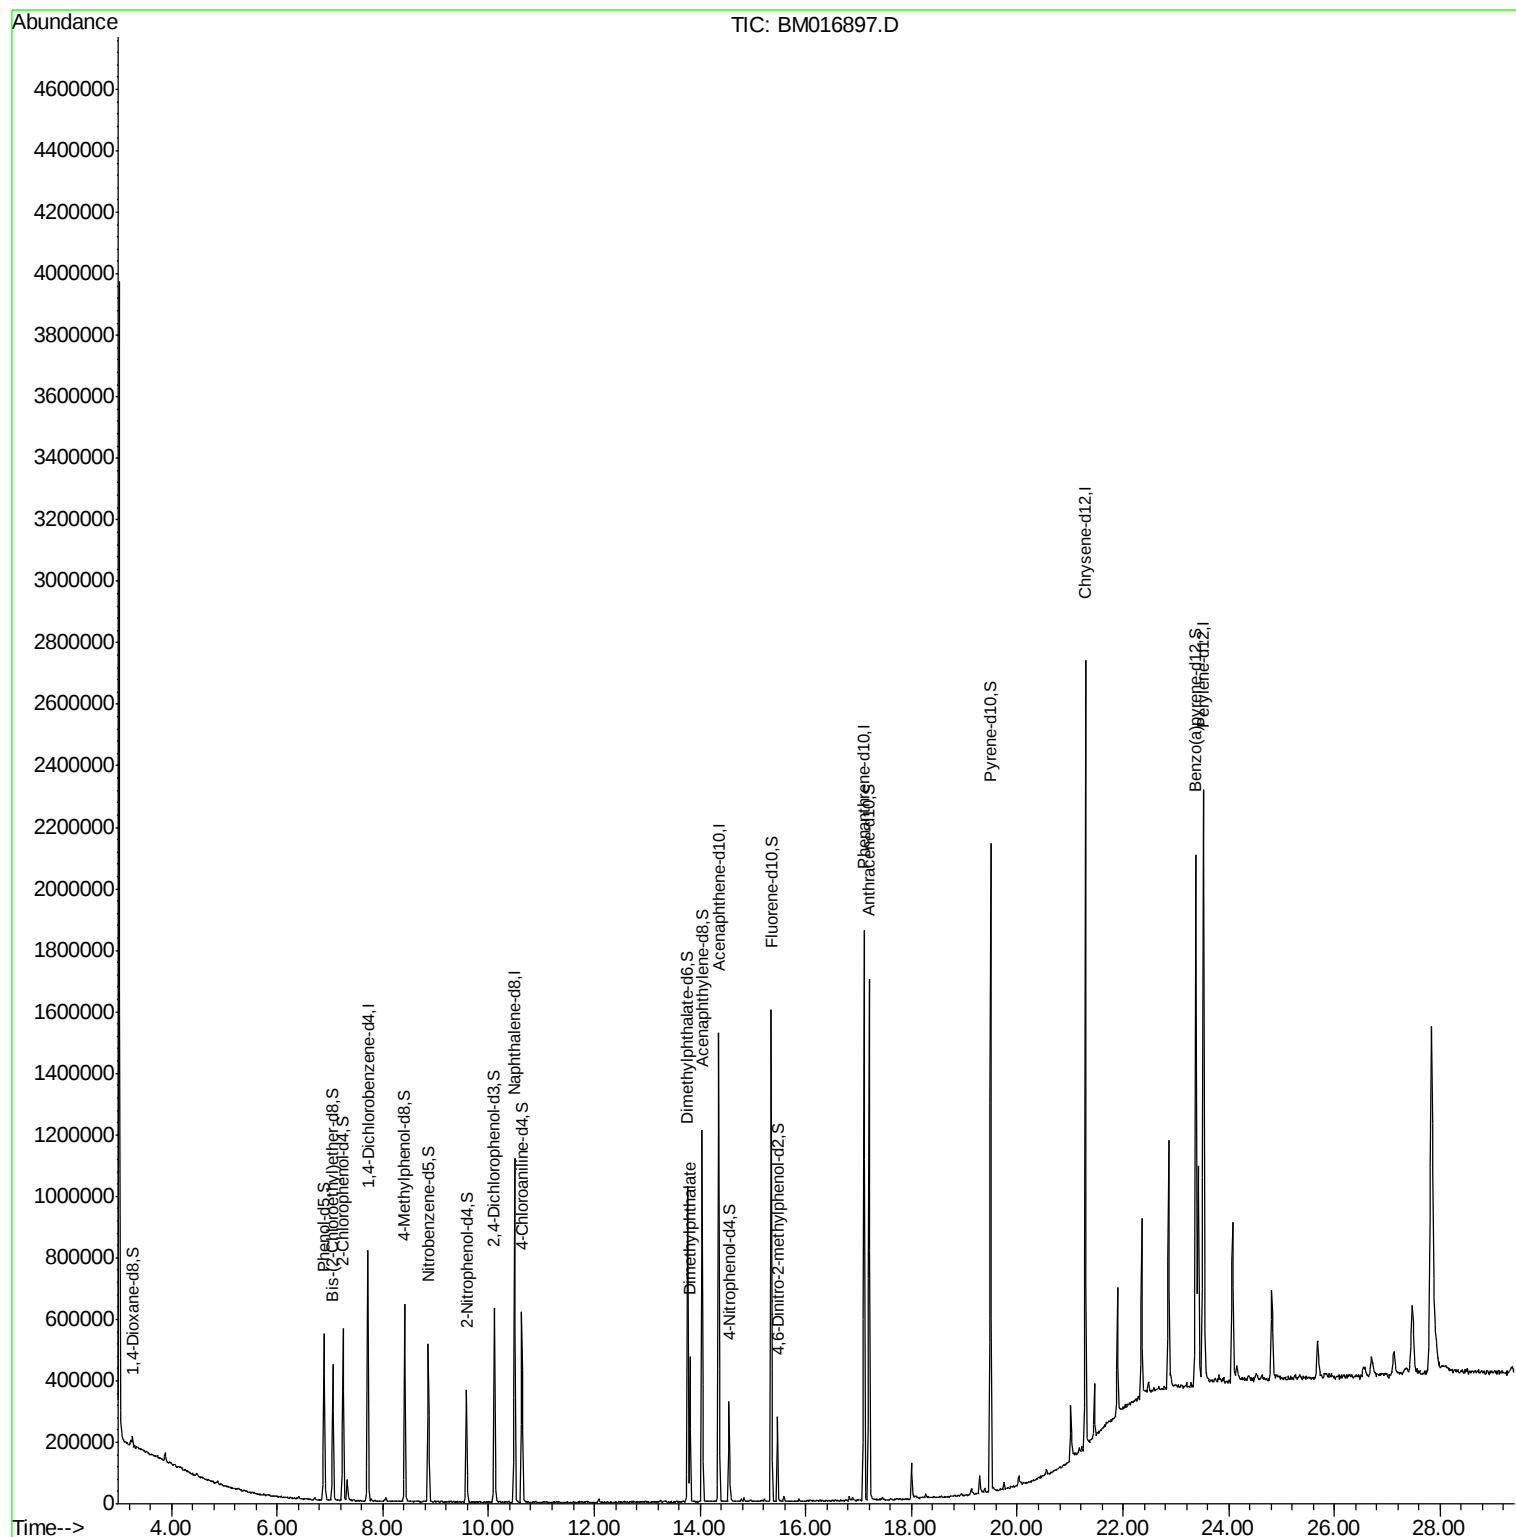

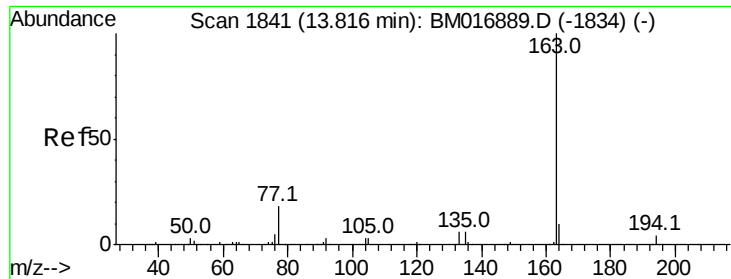

#45

Dimethylphthalate

Concen: 7.549 ng/ul

RT: 13.81 min Scan# 1840

Delta R.T. -0.01 min

Lab File: BM016897.D

Acq: 26 Sep 2018 13:46

Instrument :

BNA_M

ClientSampleId :

BE9G3


Tot Ion:163 Resp: 290840

Ion Ratio Lower Upper

163 100

194 4.1 4.0 6.0

164 9.9 8.4 12.6

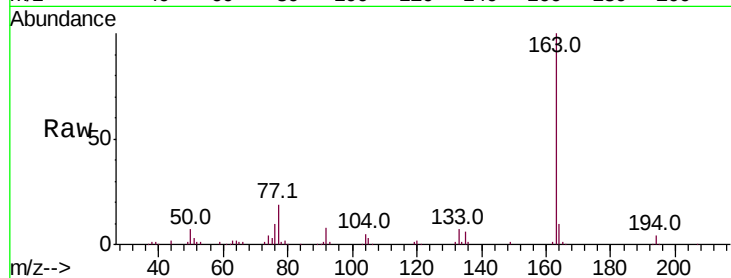

Abundance Ion 163.00 (162.70 to 163.70): E

300000 Ion 194.00 (193.70 to 194.70): E

250000 Ion 164.00 (163.70 to 164.70): E

200000

150000

100000

50000

0

13.75

13.80

13.85

