

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092618\
 Data File : BM016904.D
 Acq On : 26 Sep 2018 18:01
 Operator : MJ/SJ
 Sample : J5040-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E8JE2

Quant Time: Oct 01 17:26:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 27 02:42:56 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	266418	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	1109763	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.36	164	586938	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	1316772	20.00	ng/ul	0.00
78) Chrysene-d12	21.29	240	1455666	20.00	ng/ul	0.00
86) Perylene-d12	23.53	264	1585550	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.27	96	21434	3.44	ng/uL	0.00
5) Phenol-d5	6.89	99	479425	21.34	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	294696	21.18	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	413648	22.56	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	371447	21.36	ng/ul	0.00
19) Nitrobenzene-d5	8.87	128	196947	27.01	ng/ul	0.00
22) 2-Nitrophenol-d4	9.59	143	202142	30.49	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	377834	22.43	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	498399	24.51	ng/ul	0.00
44) Dimethylphthalate-d6	13.77	166	1105991	23.47	ng/ul	0.00
47) Acenaphthylene-d8	14.05	160	1435408	23.58	ng/ul	0.00
52) 4-Nitrophenol-d4	14.56	143	134828	17.43	ng/ul	0.00
58) Fluorene-d10	15.35	176	998772	24.28	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.47	200	84947	15.71	ng/ul	0.00
71) Anthracene-d10	17.20	188	1533234	24.13	ng/ul	0.00
79) Pyrene-d10	19.50	212	1760403	24.92	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.39	264	2061881	24.93	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.82	163	489700	10.632	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092618\
Data File : BM016904.D
Acq On : 26 Sep 2018 18:01
Operator : MJ/SJ
Sample : J5040-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E8JE2

Quant Time: Oct 01 17:26:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 27 02:42:56 2018
Response via : Initial Calibration

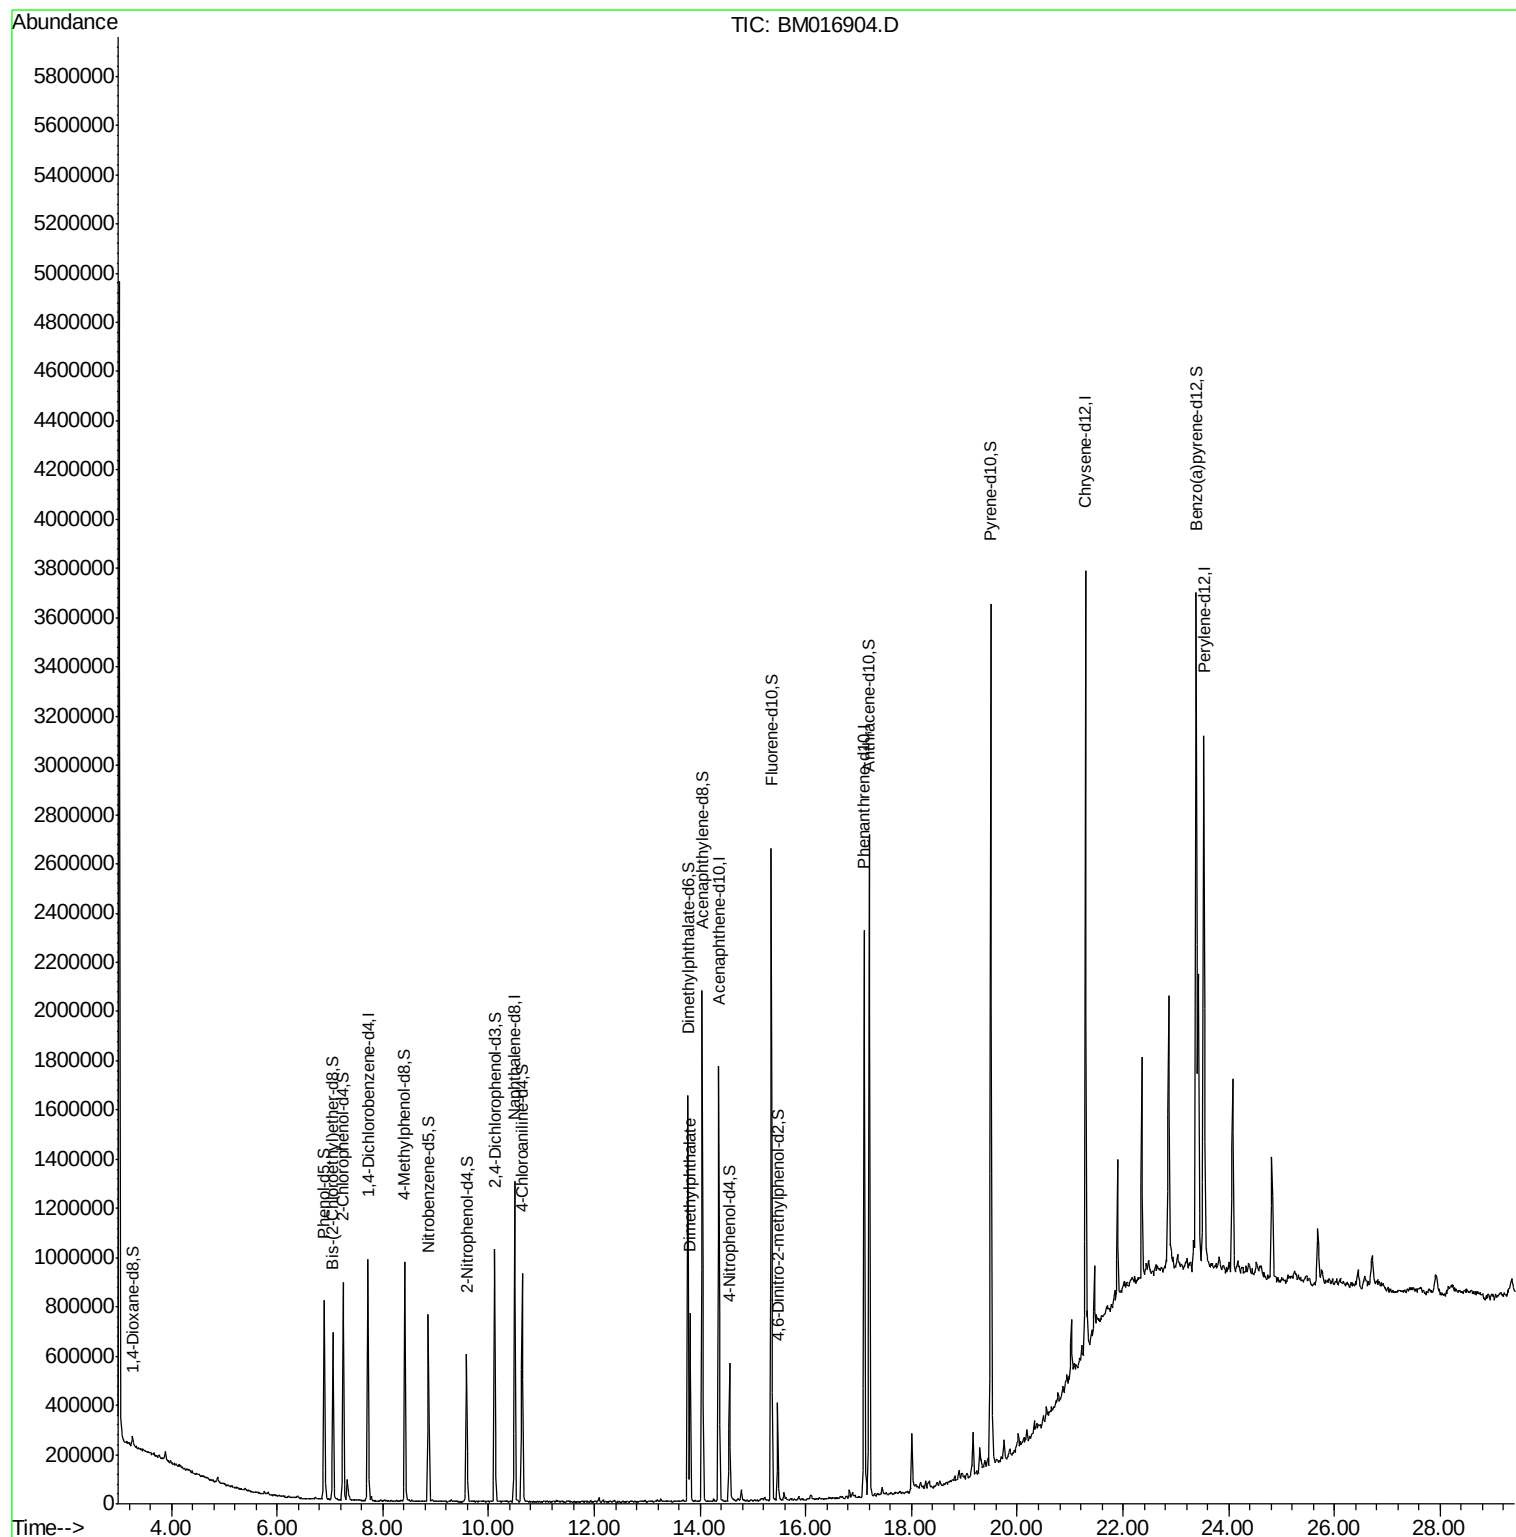

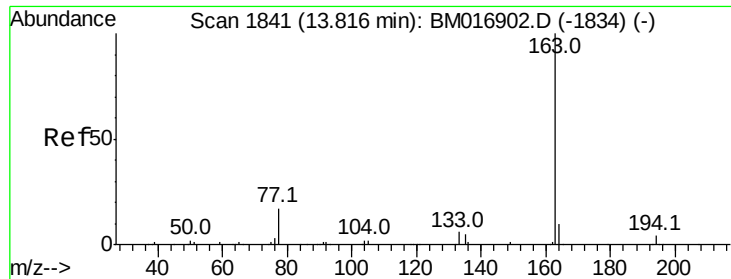

#45

Dimethylphthalate

Concen: 10.632 ng/ul

RT: 13.82 min Scan# 1841

Delta R.T. 0.00 min

Lab File: BM016904.D

Acq: 26 Sep 2018 18:01

Instrument :

BNA_M

ClientSampleId :

E8JE2

Tot Ion:163 Resp: 489700

Ion Ratio Lower Upper

163 100

194 4.1 4.0 6.0

164 9.7 8.4 12.6

