

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092618\
 Data File : BM016906.D
 Acq On : 26 Sep 2018 19:13
 Operator : MJ/SJ
 Sample : J5040-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E8JD5

Manual Integrations
 APPROVED

Sohil
 9/27/2018 5:26:27 PM

Quant Time: Sep 27 02:59:04 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 27 02:42:56 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	277262	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	1159676	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.36	164	614917	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	1373891	20.00	ng/ul	0.00
78) Chrysene-d12	21.29	240	1512545	20.00	ng/ul	0.00
86) Perylene-d12	23.53	264	1626582	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	17473m	2.69	ng/uL	0.00
5) Phenol-d5	6.89	99	575811	24.62	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	323715	22.35	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	479033	25.10	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	447562	24.73	ng/ul	0.00
19) Nitrobenzene-d5	8.87	128	232608	30.52	ng/ul	0.00
22) 2-Nitrophenol-d4	9.58	143	247575	35.74	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	483270	27.45	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	516267	24.29	ng/ul	0.00
44) Dimethylphthalate-d6	13.77	166	1379431	27.94	ng/ul	0.00
47) Acenaphthylene-d8	14.05	160	1799726	28.22	ng/ul	0.00
52) 4-Nitrophenol-d4	14.56	143	201549	24.87	ng/ul	0.00
58) Fluorene-d10	15.35	176	1249657	29.00	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.47	200	121717	21.58	ng/ul	0.00
71) Anthracene-d10	17.20	188	1874167	28.27	ng/ul	0.00
79) Pyrene-d10	19.50	212	2125484	28.96	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.39	264	2445822	28.83	ng/ul	0.00

Target Compounds				Ovalue
45) Dimethylphthalate	13.82	163	450176	9.329 ng/ul# 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092618\
Data File : BM016906.D
Acq On : 26 Sep 2018 19:13
Operator : MJ/SJ
Sample : J5040-03
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
E8JD5

Quant Time: Sep 27 02:59:04 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 27 02:42:56 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
9/27/2018 5:26:27 PM

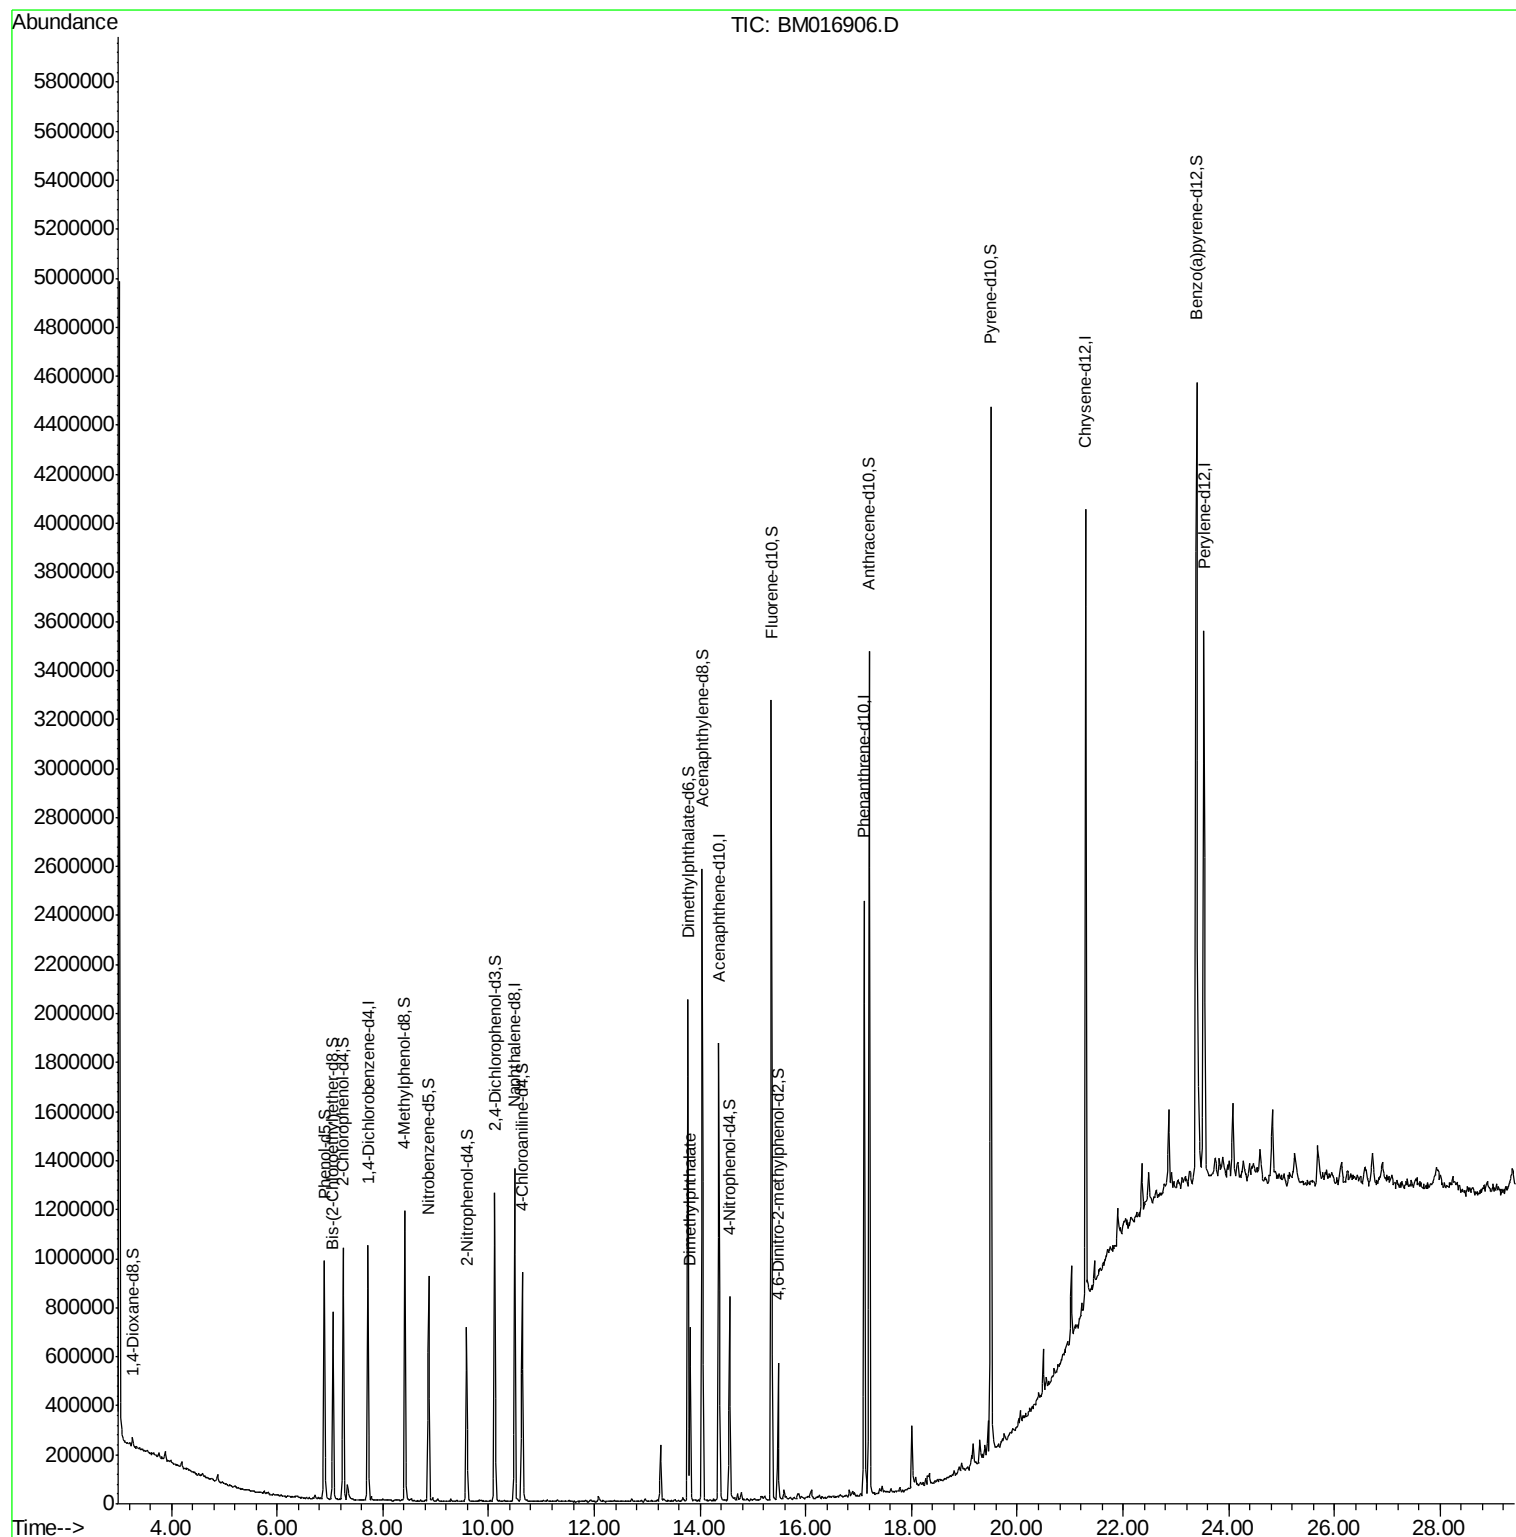

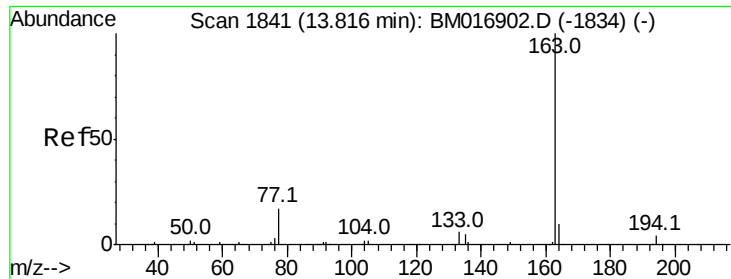

#45

Dimethylphthalate

Concen: 9.329 ng/ul

RT: 13.82 min Scan# 1841

Delta R.T. 0.00 min

Lab File: BM016906.D

Acq: 26 Sep 2018 19:13

Instrument :

BNA_M

ClientSampleId :

E8JD5

Tot Ion:163 Resp: 450176

Ion Ratio Lower Upper

163 100

194 3.9 4.0 6.0#

164 10.1 8.4 12.6

Manual Integrations

APPROVED

Sohil

9/27/2018 5:26:27 PM

