

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092618\
 Data File : BM016891.D
 Acq On : 26 Sep 2018 10:09
 Operator : MJ/SJ
 Sample : PB113141BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK41

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	44	47	52	rVB2	64844	80065	1.38%	0.146%
2	6.887	656	663	673	rBV	1007873	1531573	26.39%	2.794%
3	7.057	685	692	699	rVB	803938	1217498	20.98%	2.221%
4	7.245	718	724	740	rVB	1041396	1616888	27.86%	2.949%
5	7.716	796	804	811	rBV	776550	1256813	21.66%	2.293%
6	8.416	914	923	933	rBV	1181661	1879691	32.39%	3.429%
7	8.863	992	999	1008	rBV	943017	1521403	26.22%	2.775%
8	9.581	1112	1121	1134	rBV	685322	1104175	19.03%	2.014%
9	10.110	1204	1211	1222	rBV	1150400	1907101	32.87%	3.479%
10	10.492	1268	1276	1286	rBV	1082317	1767576	30.46%	3.224%
11	10.628	1292	1299	1312	rBV	1176242	1943974	33.50%	3.546%
12	12.086	1542	1547	1552	rVB	20738	31730	0.55%	0.058%
13	13.763	1826	1832	1844	rVB	1857426	2673014	46.07%	4.876%
14	14.045	1871	1880	1890	rBV	2332412	3446798	59.40%	6.287%
15	14.351	1925	1932	1941	rBV2	1442373	2188864	37.72%	3.993%
16	14.551	1959	1966	1980	rBV	815647	1127510	19.43%	2.057%
17	15.351	2095	2102	2111	rBV	3068164	4286825	73.88%	7.820%
18	15.463	2116	2121	2131	rBV	589225	840216	14.48%	1.533%
19	15.586	2138	2142	2148	rBV	30875	42350	0.73%	0.077%
20	16.886	2358	2363	2368	rBV2	6941	10057	0.17%	0.018%
21	17.098	2393	2399	2406	rBV2	1719929	2489480	42.90%	4.541%
22	17.198	2410	2416	2427	rBV	3218346	4507019	77.67%	8.221%
23	19.127	2740	2744	2749	rVB	31086	43538	0.75%	0.079%
24	19.380	2784	2787	2793	rBV	21635	26395	0.45%	0.048%
25	19.498	2801	2807	2813	rBV	3722264	5157519	88.88%	9.408%
26	21.286	3106	3111	3119	rBV	2438868	3076268	53.02%	5.611%
27	23.380	3460	3467	3481	rBV	3118088	5802583	100.00%	10.584%
28	23.521	3484	3491	3501	rVV	1760081	3245271	55.93%	5.920%


Sum of corrected areas: 54822194

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092618\
Data File : BM016891.D
Acq On : 26 Sep 2018 10:09
Operator : MJ/SJ
Sample : PB113141BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK41

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

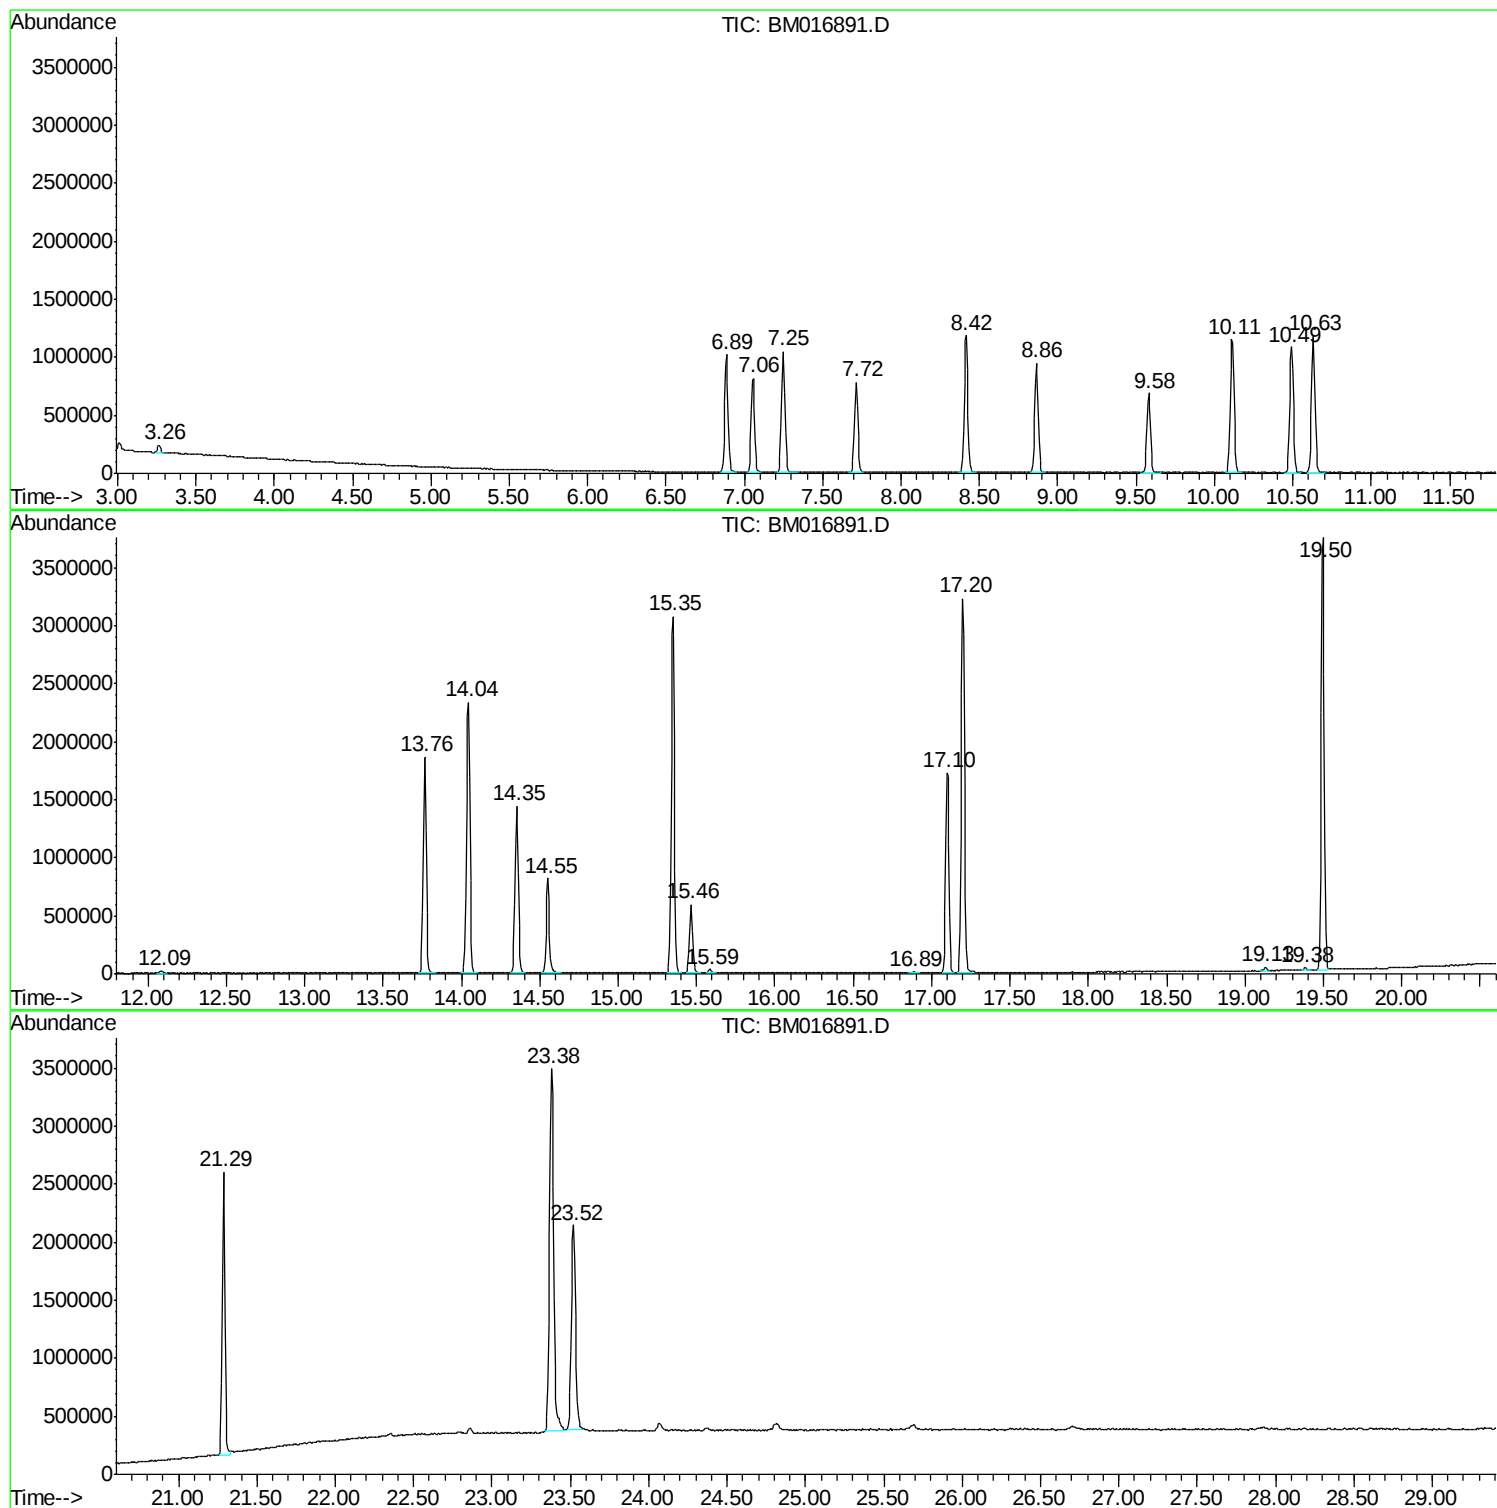

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM092618\
Data File : BM016891.D
Acq On : 26 Sep 2018 10:09
Operator : MJ/SJ
Sample : PB113141BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK41

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM092618\
Data File : BM016891.D
Acq On : 26 Sep 2018 10:09
Operator : MJ/SJ
Sample : PB113141BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK41

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc