




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092624\
 Data File : BM047666.D
 Acq On : 27 Sep 2024 05:29
 Operator : RC/JU
 Sample : PB163687BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK687

Manual IntegrationsAPPROVED

Quant Time: Sep 27 06:45:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 25 16:27:08 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/27/2024
 Supervised By :mohammad ahmed 09/28/2024

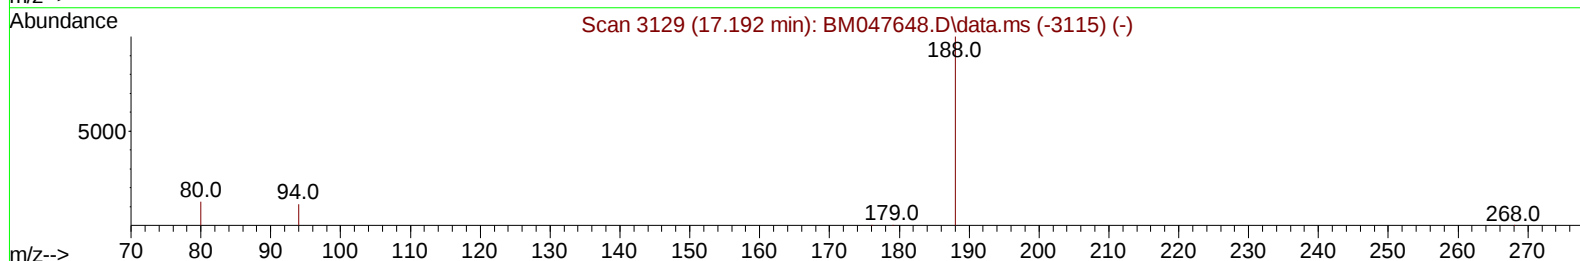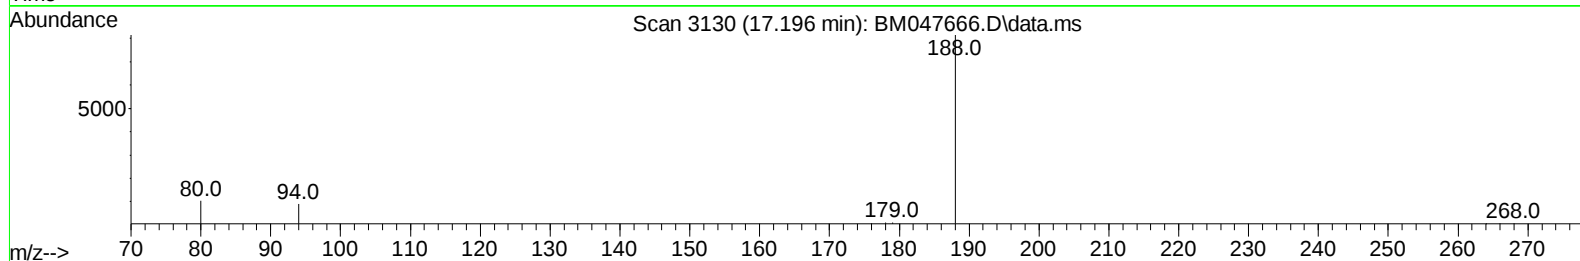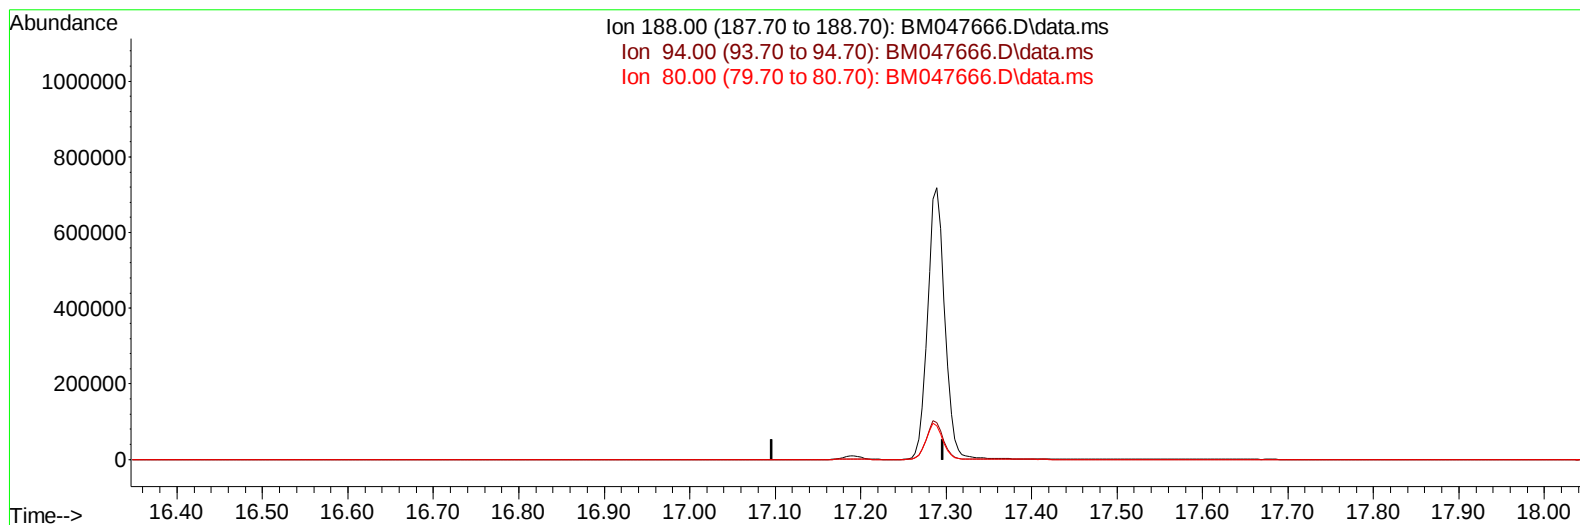

TIC: BM047666.D\data.ms

(13) Phenanthrene-d10 (I)

17.196min (-17.196) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	12.20	0.00#
80.00	13.00	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092624\
Data File : BM047666.D
Acq On : 27 Sep 2024 05:29
Operator : RC/JU
Sample : PB163687BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK687

Manual IntegrationsAPPROVED

Quant Time: Sep 27 06:45:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 25 16:27:08 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/27/2024
Supervised By :mohammad ahmed 09/28/2024

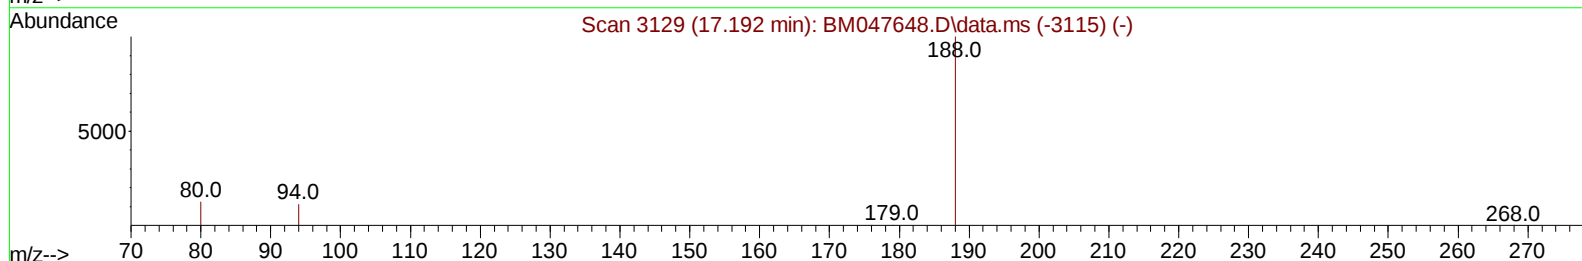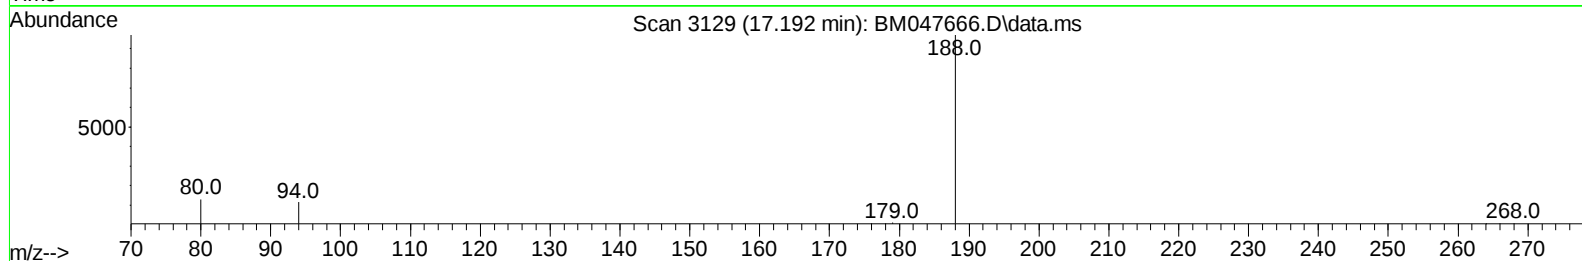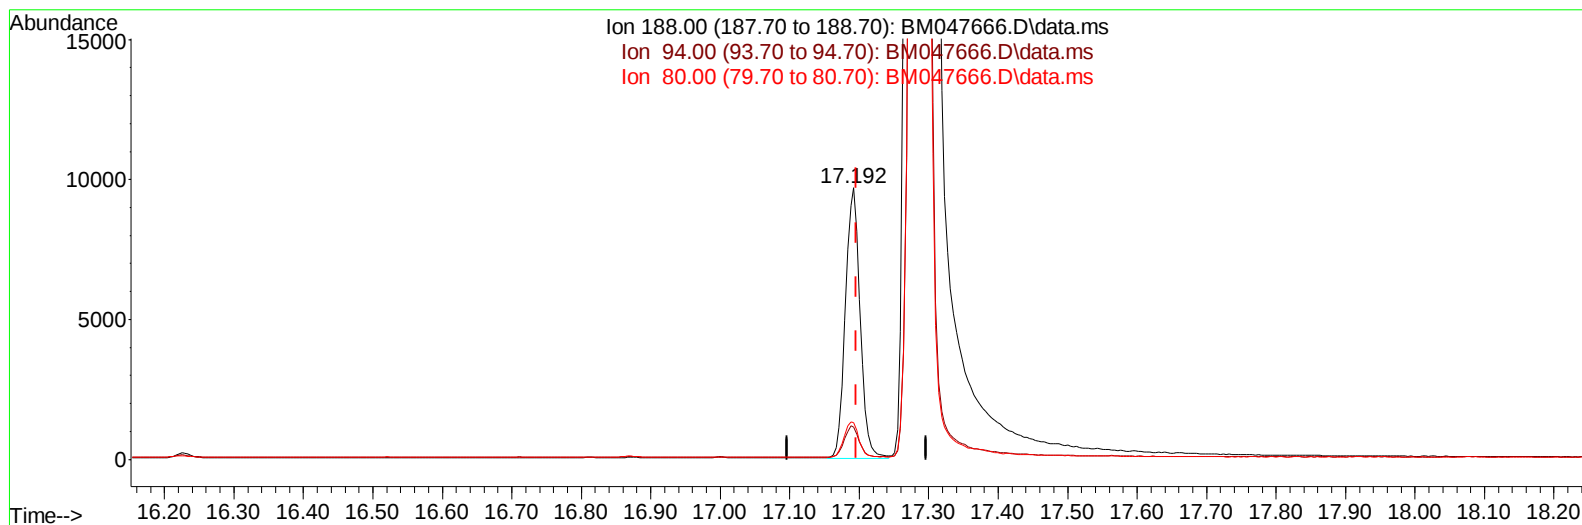

TIC: BM047666.D\data.ms

(13) Phenanthrene-d10 (I)

17.192min (-0.004) 0.40 ng/ul m

response 14247

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.20	11.85
80.00	13.00	13.46
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092624\
Data File : BM047666.D
Acq On : 27 Sep 2024 05:29
Operator : RC/JU
Sample : PB163687BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK687

Manual IntegrationsAPPROVED

Quant Time: Sep 27 06:45:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 25 16:27:08 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/27/2024
Supervised By :mohammad ahmed 09/28/2024

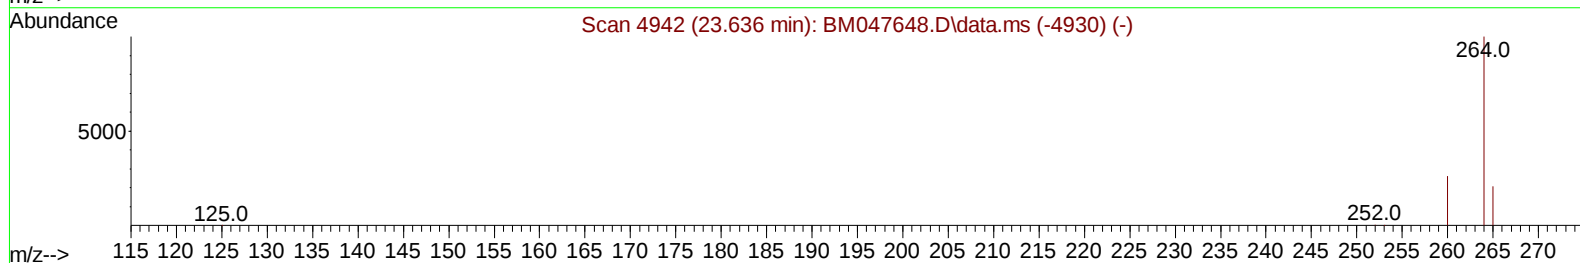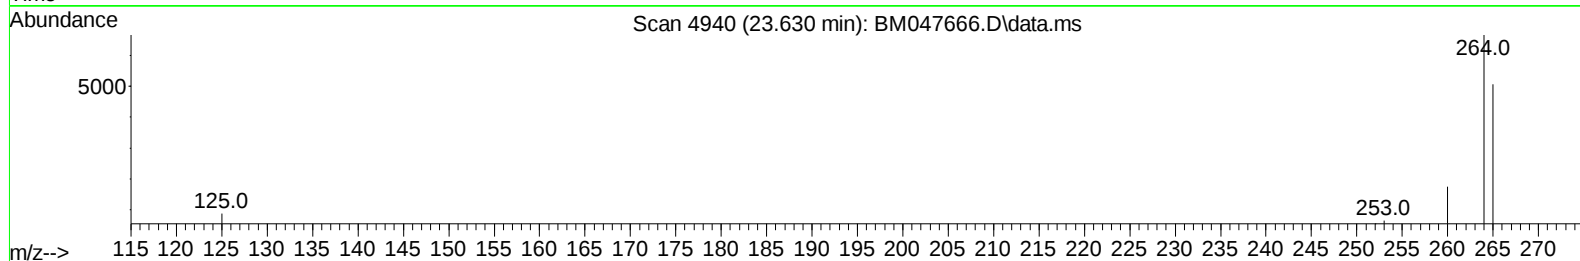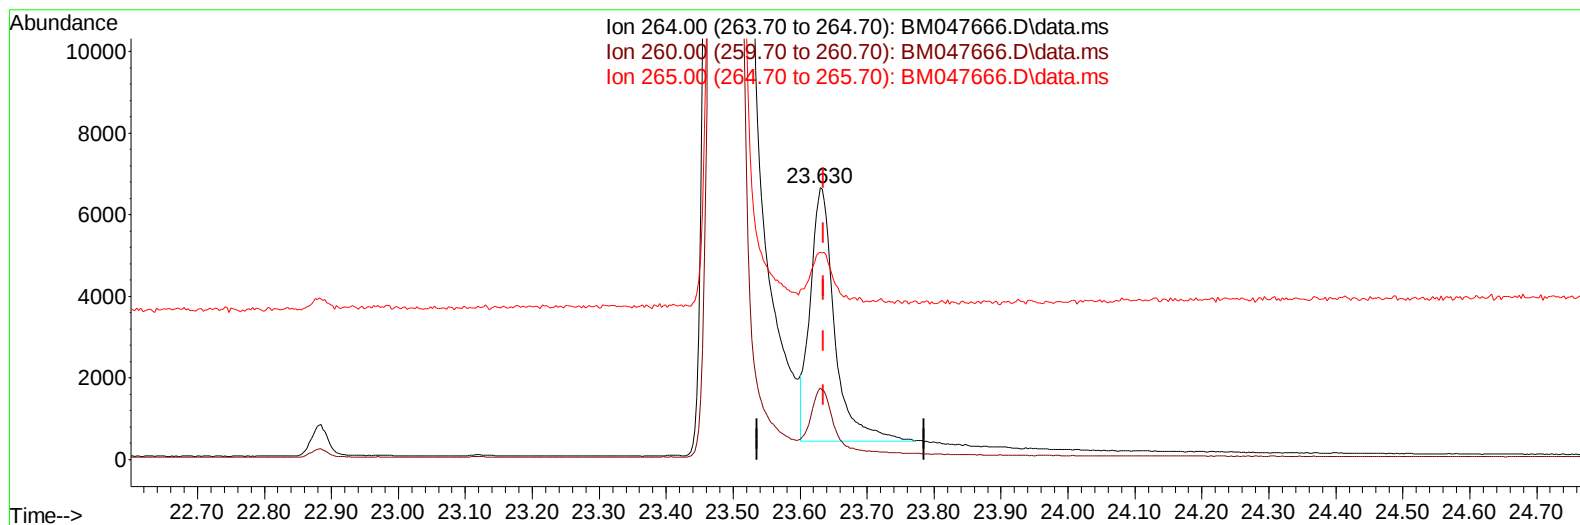

TIC: BM047666.D\data.ms

(23) Perylene-d12 (I)

23.630min (-0.006) 0.40 ng/u1

response 15798

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	26.23
265.00	85.70	76.20
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092624\
Data File : BM047666.D
Acq On : 27 Sep 2024 05:29
Operator : RC/JU
Sample : PB163687BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK687

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/27/2024
Supervised By :mohammad ahmed 09/28/2024

Quant Time: Sep 27 06:45:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 25 16:27:08 2024
Response via : Initial Calibration

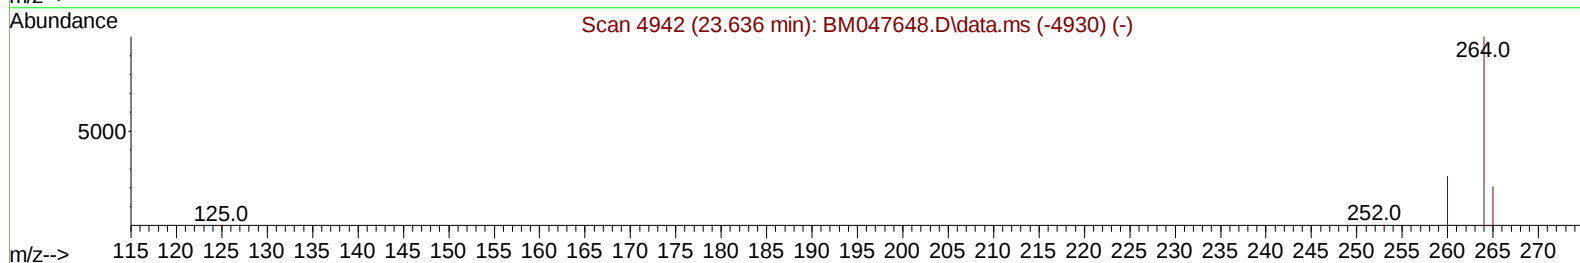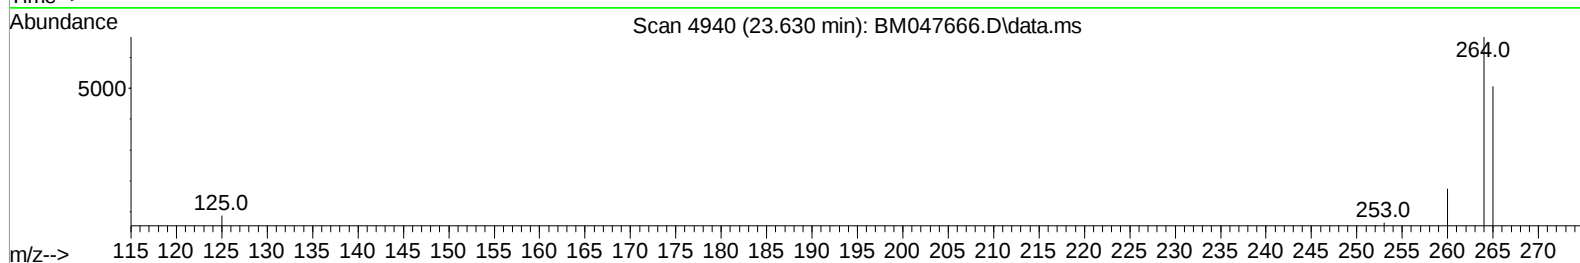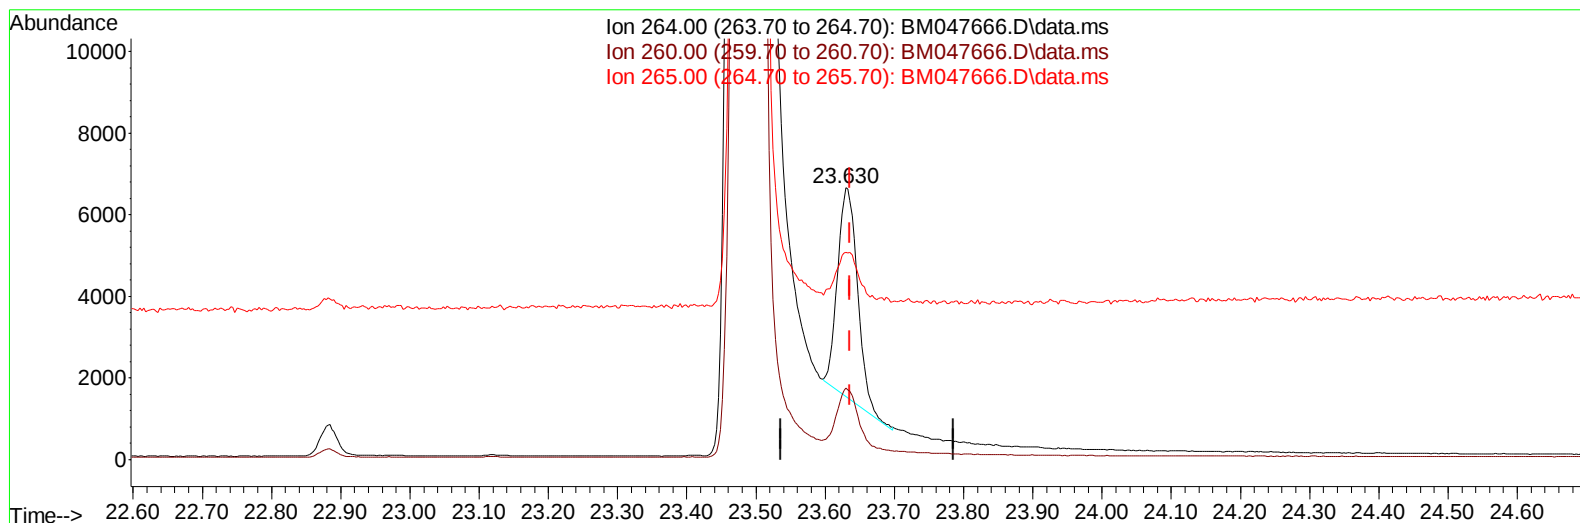

TIC: BM047666.D\data.ms

(23) Perylene-d12 (I)

23.630min (-0.006) 0.40 ng/ul m

response 10226

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	26.23
265.00	85.70	76.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092624\
 Data File : BM047666.D
 Acq On : 27 Sep 2024 05:29
 Operator : RC/JU
 Sample : PB163687BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK687

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/27/2024
 Supervised By :mohammad ahmed 09/28/2024

Quant Time: Sep 27 06:45:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 25 16:27:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.826	152	5175	0.400	ng/ul	0.00
4) Naphthalene-d8	10.618	136	15035	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.456	164	7356	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.192	188	14247m	0.400	ng/ul	0.00
17) Chrysene-d12	21.356	240	10478	0.400	ng/ul	0.00
23) Perylene-d12	23.630	264	10226m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	41345	6.218	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.207	152	5660	0.282	ng/ul	0.00
18) Fluoranthene-d10	19.211	212	10106	0.315	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092624\
Data File : BM047666.D
Acq On : 27 Sep 2024 05:29
Operator : RC/JU
Sample : PB163687BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK687

Manual IntegrationsAPPROVED

Quant Time: Sep 27 06:45:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 25 16:27:08 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/27/2024
Supervised By :mohammad ahmed 09/28/2024

