

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092624\
 Data File : BM047645.D
 Acq On : 26 Sep 2024 15:56
 Operator : RC/JU
 Sample : P4187-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EY047

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 09/27/2024
 Supervised By :mohammad ahmed 09/28/2024

Quant Time: Sep 26 16:36:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 25 16:27:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.830	152	6334	0.400	ng/ul	0.00
4) Naphthalene-d8	10.617	136	19056	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.456	164	9540	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.192	188	19331m	0.400	ng/ul	0.00
17) Chrysene-d12	21.356	240	14894	0.400	ng/ul	0.00
23) Perylene-d12	23.639	264	14417m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	37249	4.577	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.212	152	5409	0.213	ng/ul	0.00
18) Fluoranthene-d10	19.211	212	14400	0.316	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.307	88	6005	0.617	ng/ul#	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092624\
Data File : BM047645.D
Acq On : 26 Sep 2024 15:56
Operator : RC/JU
Sample : P4187-03
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
EY047

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 09/27/2024
Supervised By :mohammad ahmed 09/28/2024


Quant Time: Sep 26 16:36:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 25 16:27:08 2024
Response via : Initial Calibration

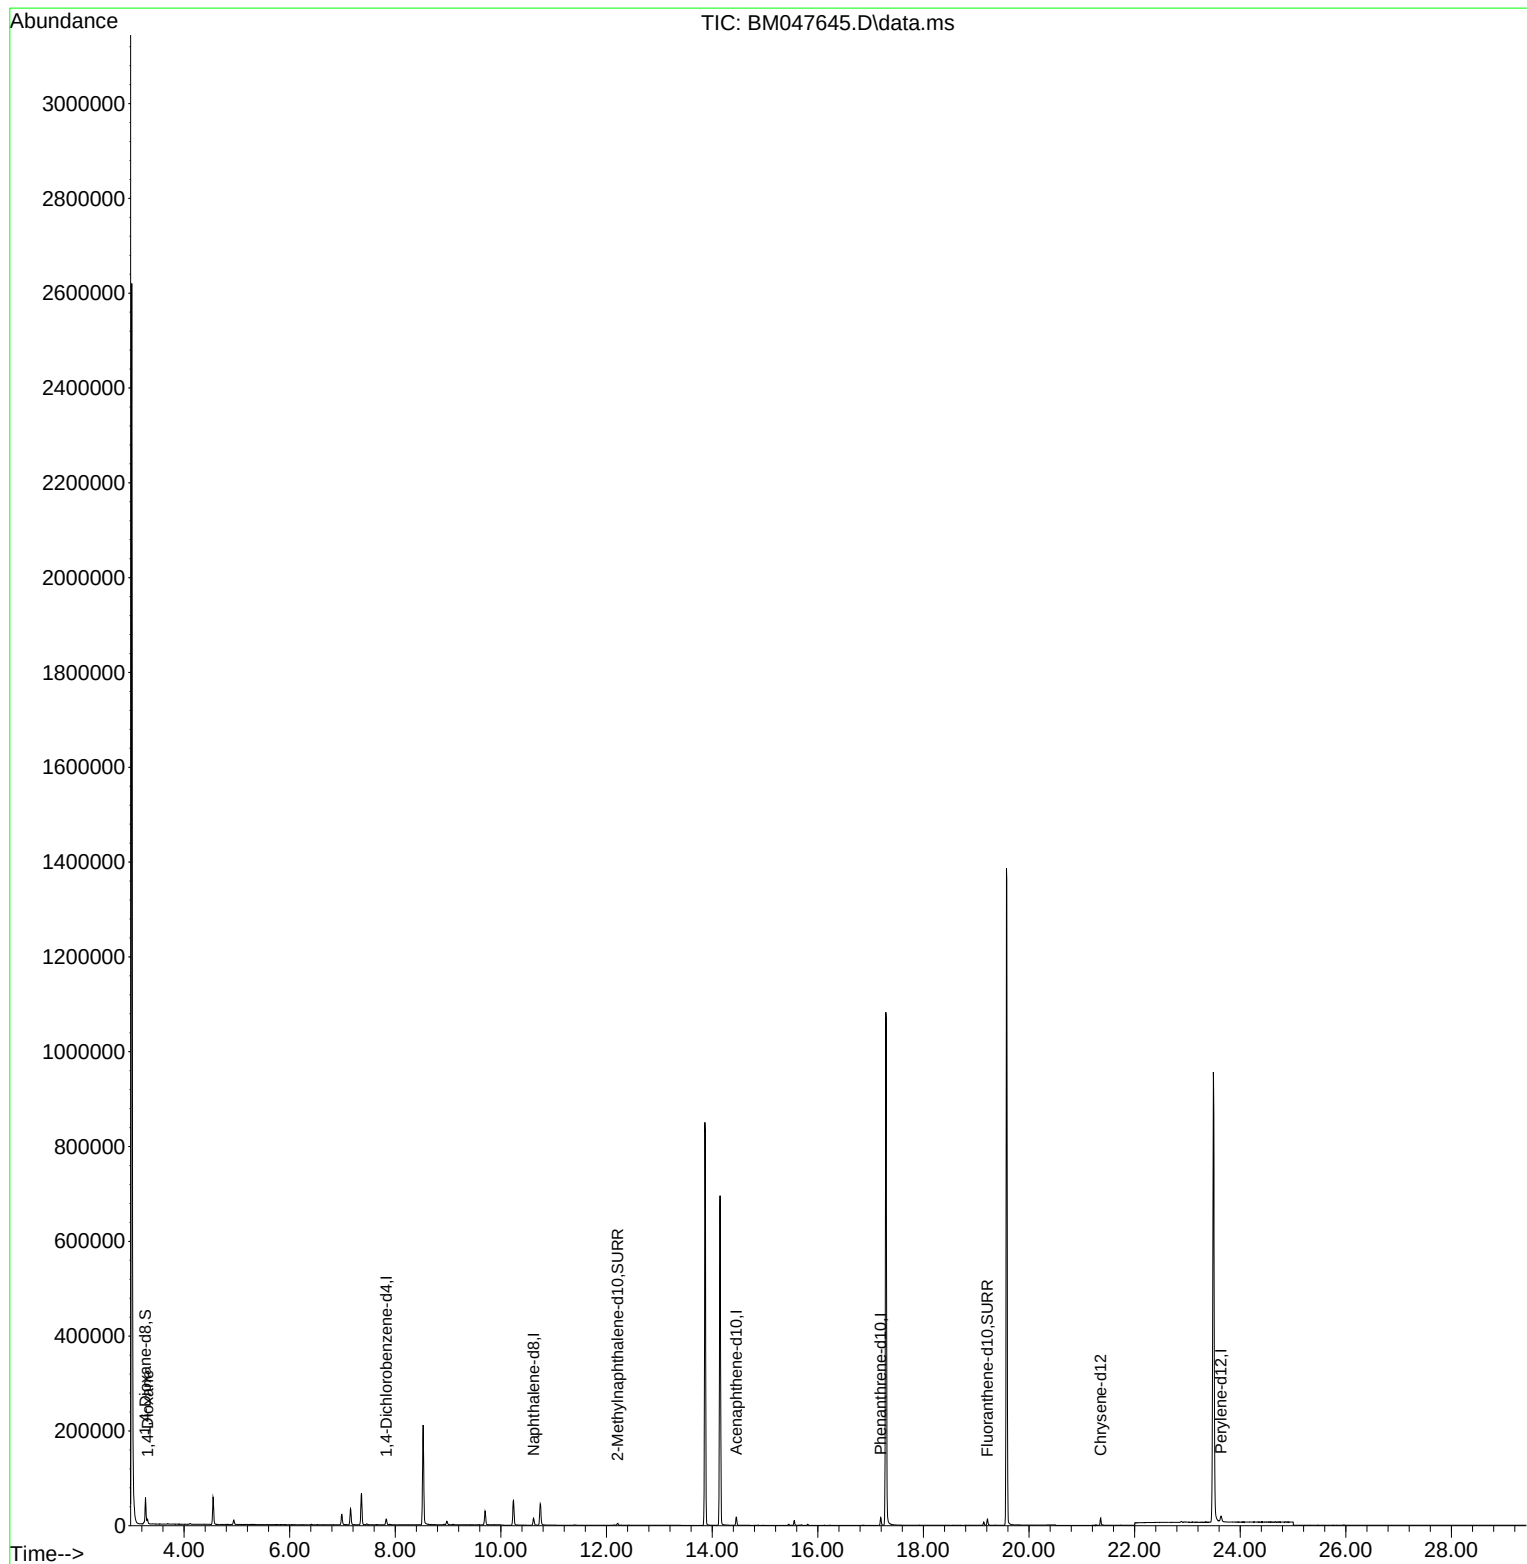

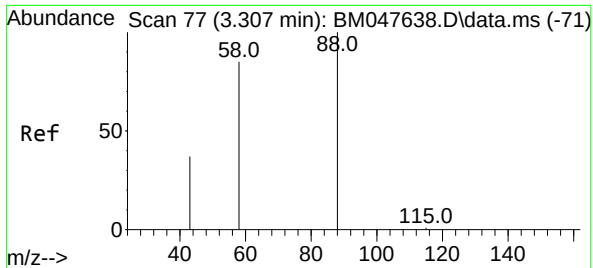

#2
 1,4-Dioxane
 Concen: 0.617 ng/ul
 RT: 3.307 min Scan# 71
 Delta R.T. -0.000 min
 Lab File: BM047645.D
 Acq: 26 Sep 2024 15:56

Instrument :
 BNA_M
 ClientSampleId :
 EY047

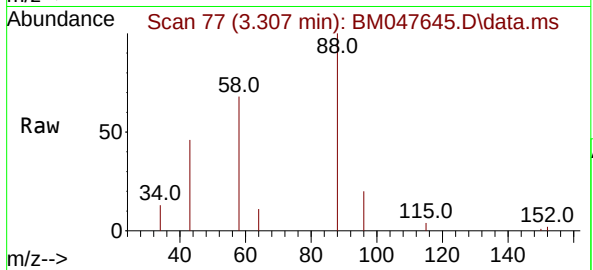

Tgt Ion: 88 Resp: 600

Ion	Ratio	Lower	Upper
88	100		
43	46.5	30.9	46.3
58	68.3	42.5	63.7

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 09/27/2024
 Supervised By :mohammad ahmed 09/28/2024

