

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM092624\  
 Data File : BM047646.D  
 Acq On : 26 Sep 2024 16:33  
 Operator : RC/JU  
 Sample : P4187-04  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 EY048

Manual Integrations  
 APPROVED

Reviewed By :Jagrut Upadhyay 09/27/2024  
 Supervised By :mohammad ahmed 09/28/2024

Quant Time: Sep 26 17:16:57 2024  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM092524.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Sep 25 16:27:08 2024  
 Response via : Initial Calibration

| Compound                    | R.T.   | QIon | Response | Conc  | Units  | Dev(Min) |
|-----------------------------|--------|------|----------|-------|--------|----------|
| -----                       |        |      |          |       |        |          |
| Internal Standards          |        |      |          |       |        |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.826  | 152  | 4946     | 0.400 | ng/ul  | 0.00     |
| 4) Naphthalene-d8           | 10.622 | 136  | 14681    | 0.400 | ng/ul  | 0.00     |
| 9) Acenaphthene-d10         | 14.459 | 164  | 7428     | 0.400 | ng/ul  | 0.00     |
| 13) Phenanthrene-d10        | 17.190 | 188  | 14953m   | 0.400 | ng/ul  | 0.00     |
| 17) Chrysene-d12            | 21.359 | 240  | 11348    | 0.400 | ng/ul  | 0.00     |
| 23) Perylene-d12            | 23.633 | 264  | 10790m   | 0.400 | ng/ul  | 0.00     |
| System Monitoring Compounds |        |      |          |       |        |          |
| 3) 1,4-Dioxane-d8           | 3.269  | 96   | 32183    | 5.065 | ng/ul  | 0.00     |
| 6) 2-Methylnaphthalene-d10  | 12.211 | 152  | 5892     | 0.301 | ng/ul  | 0.00     |
| 18) Fluoranthene-d10        | 19.214 | 212  | 14206    | 0.409 | ng/ul  | 0.00     |
| Target Compounds            |        |      |          |       |        |          |
|                             |        |      |          |       | Qvalue |          |
| 2) 1,4-Dioxane              | 3.307  | 88   | 15274    | 2.008 | ng/ul# | 80       |
| -----                       |        |      |          |       |        |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM092624\  
Data File : BM047646.D  
Acq On : 26 Sep 2024 16:33  
Operator : RC/JU  
Sample : P4187-04  
Misc :  
ALS Vial : 10 Sample Multiplier: 1


Instrument :  
BNA\_M  
ClientSampleId :  
EY048

Manual Integrations  
APPROVED

Reviewed By :Jagrut Upadhyay 09/27/2024  
Supervised By :mohammad ahmed 09/28/2024


Quant Time: Sep 26 17:16:57 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-SIM-BM092524.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Sep 25 16:27:08 2024  
Response via : Initial Calibration

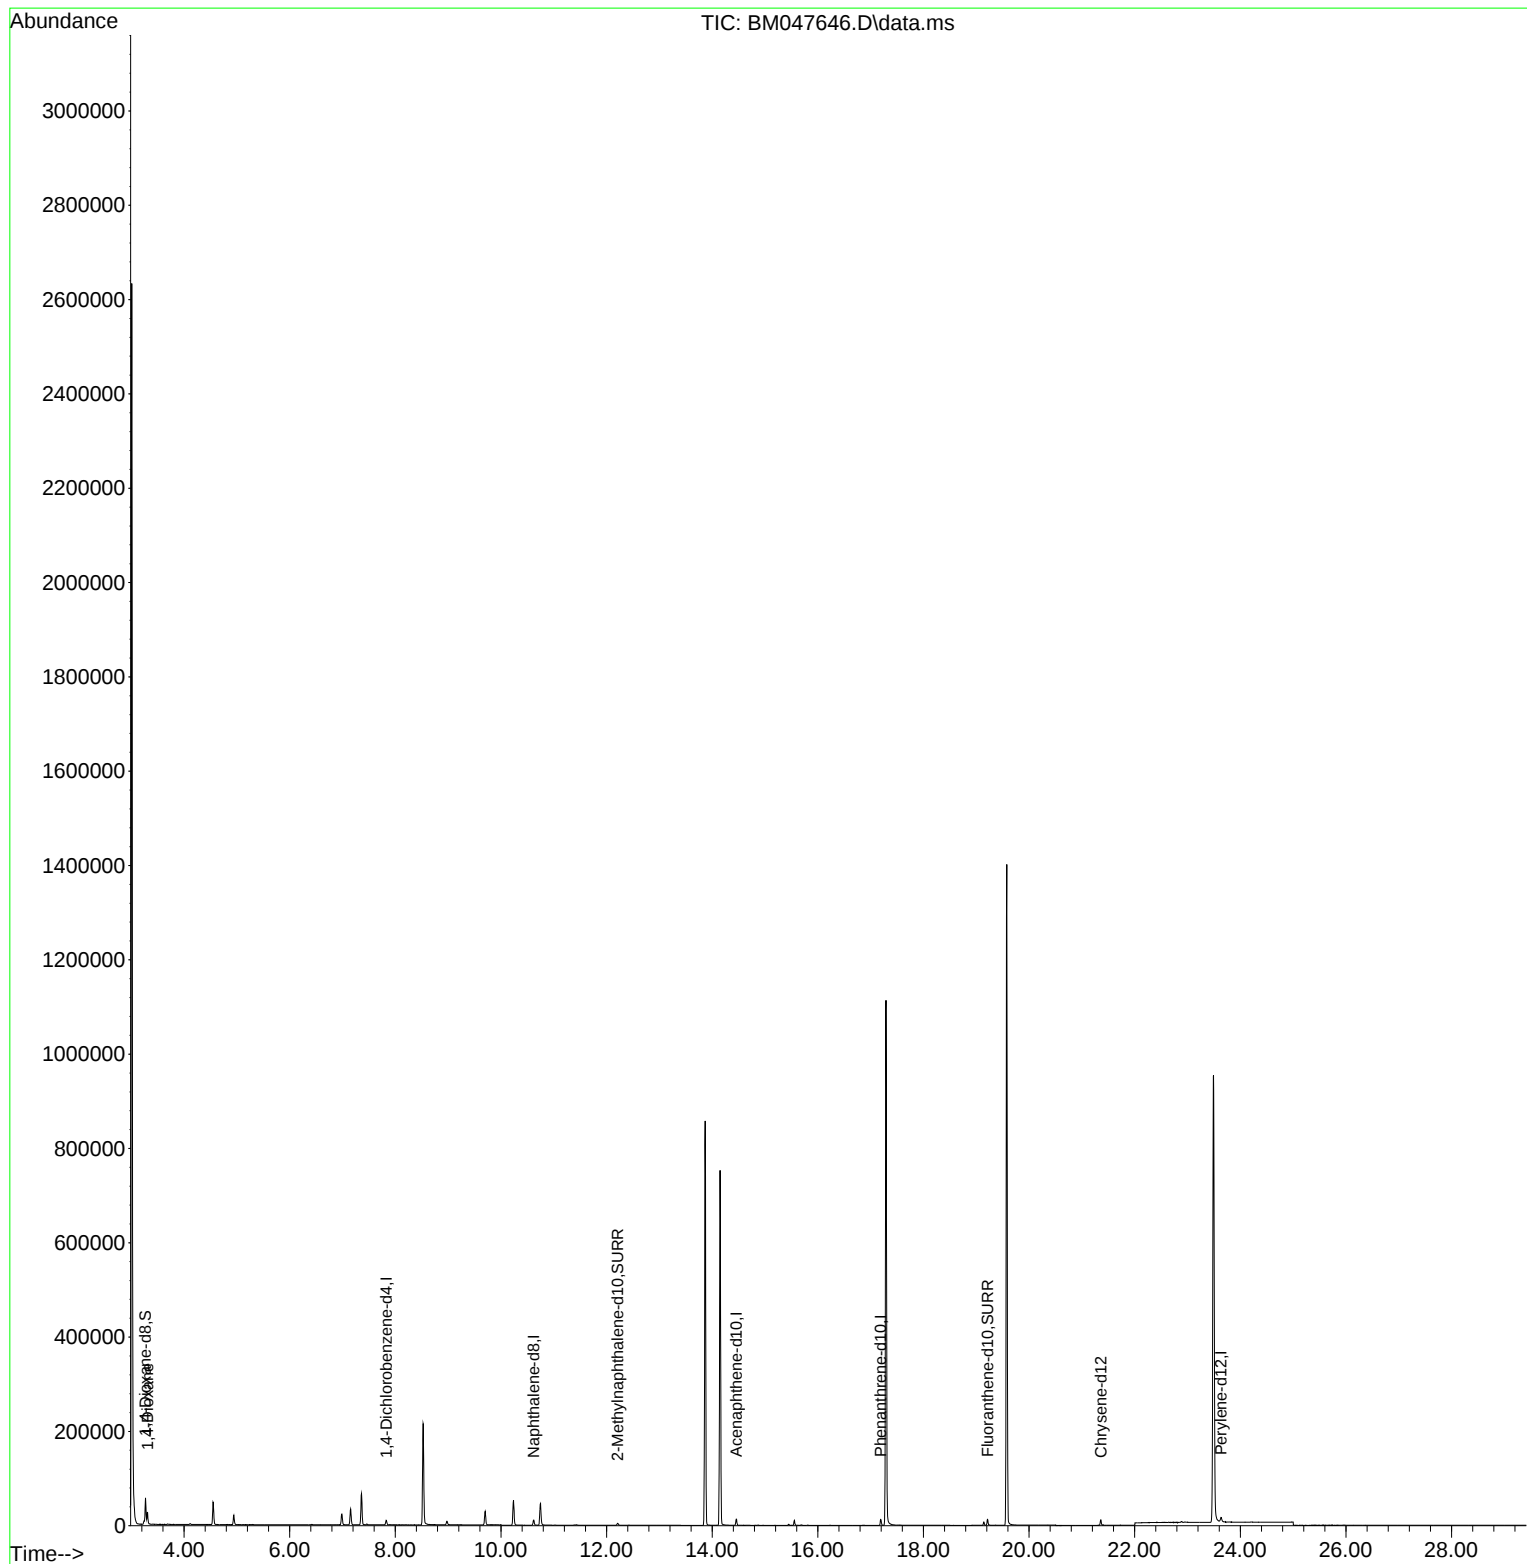

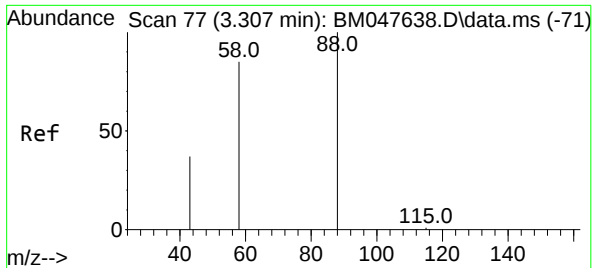

#2  
 1,4-Dioxane  
 Concen: 2.008 ng/ul  
 RT: 3.307 min Scan# 71  
 Delta R.T. -0.000 min  
 Lab File: BM047646.D  
 Acq: 26 Sep 2024 16:33

Instrument :  
 BNA\_M  
 ClientSampleId :  
 EY048

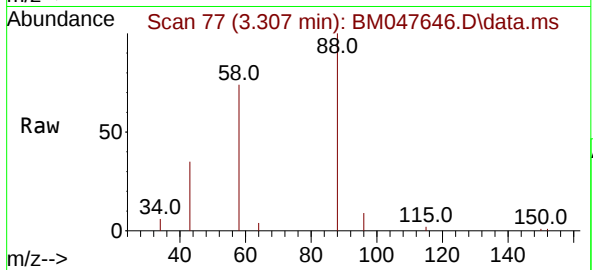

Tgt Ion: 88 Resp: 15274  
 Ion Ratio Lower Upper  
 88 100  
 43 34.9 30.9 46.3  
 58 74.1 42.5 63.7

Manual Integrations  
 APPROVED

Reviewed By :Jagrut Upadhyay 09/27/2024  
 Supervised By :mohammad ahmed 09/28/2024

