

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092624\
 Data File : BM047655.D
 Acq On : 26 Sep 2024 22:11
 Operator : RC/JU
 Sample : P4187-13
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EY072

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 09/27/2024
 Supervised By :mohammad ahmed 09/28/2024

Quant Time: Sep 27 00:25:17 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 25 16:27:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.826	152	4651	0.400	ng/ul	0.00
4) Naphthalene-d8	10.616	136	14331	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.455	164	7225	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.191	188	14517m	0.400	ng/ul	0.00
17) Chrysene-d12	21.357	240	11180	0.400	ng/ul	0.00
23) Perylene-d12	23.633	264	10726m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	31326	5.242	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.206	152	5883	0.308	ng/ul	0.00
18) Fluoranthene-d10	19.210	212	12406	0.362	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.303	88	832	0.116	ng/ul#	67

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092624\
Data File : BM047655.D
Acq On : 26 Sep 2024 22:11
Operator : RC/JU
Sample : P4187-13
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
EY072

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 09/27/2024
Supervised By :mohammad ahmed 09/28/2024


Quant Time: Sep 27 00:25:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 25 16:27:08 2024
Response via : Initial Calibration

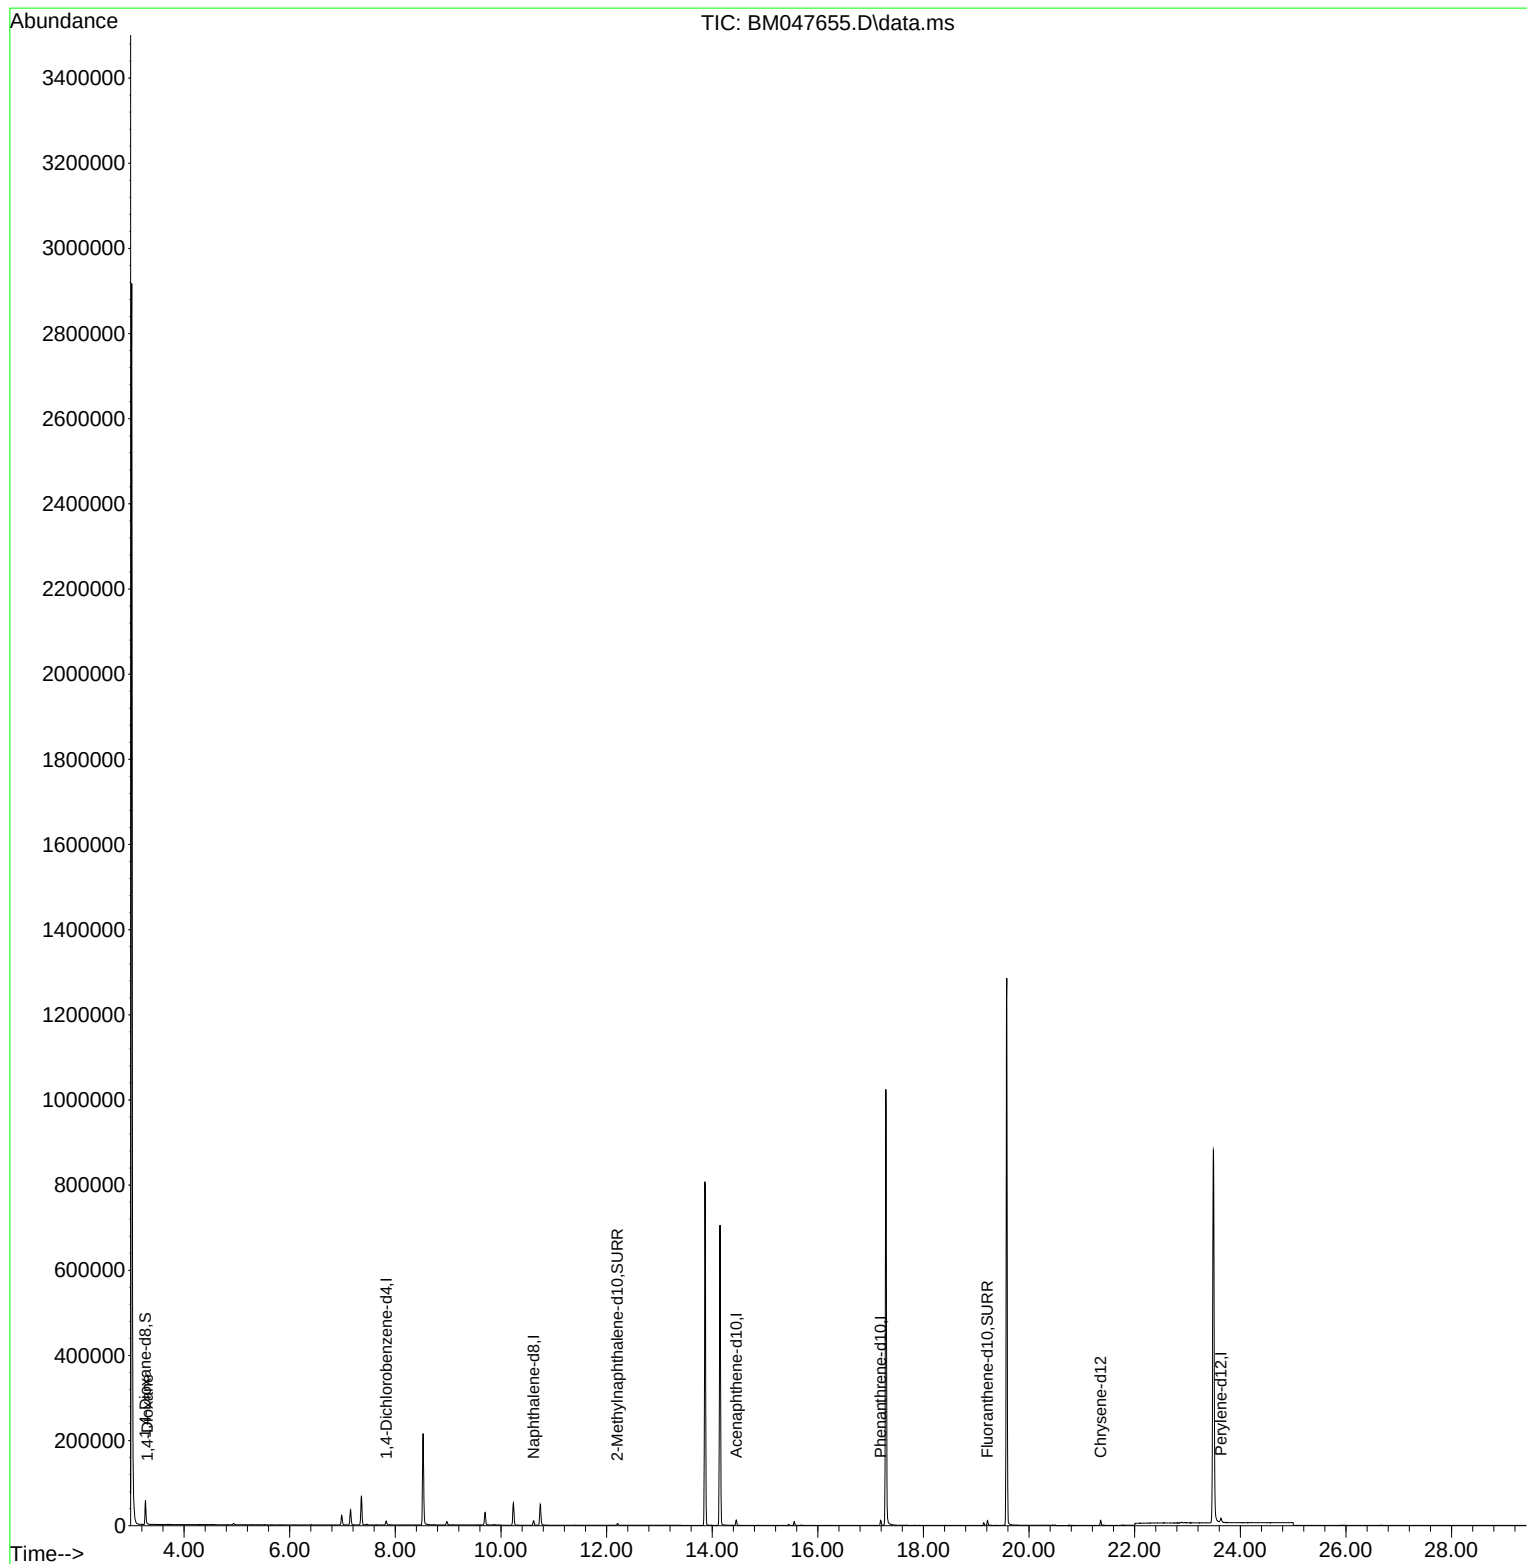

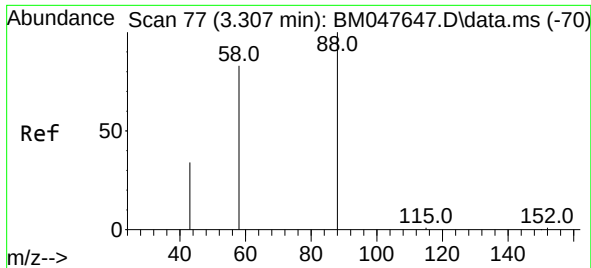

#2
 1,4-Dioxane
 Concen: 0.116 ng/ul
 RT: 3.303 min Scan# 70
 Delta R.T. -0.004 min
 Lab File: BM047655.D
 Acq: 26 Sep 2024 22:11

Instrument :
 BNA_M
 ClientSampleId :
 EY072

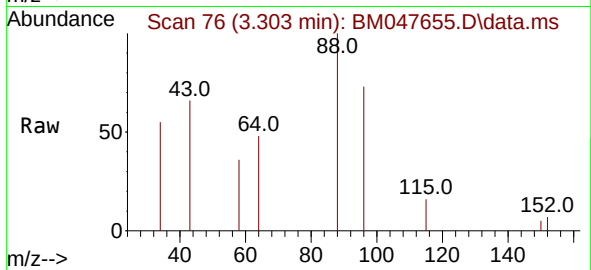

Tgt Ion: 88 Resp: 832

Ion	Ratio	Lower	Upper
88	100		
43	66.5	30.9	46.3
58	36.2	42.5	63.7

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 09/27/2024
 Supervised By :mohammad ahmed 09/28/2024

