

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092719\
 Data File : BM022807.D
 Acq On : 28 Sep 2019 03:41
 Operator : JU
 Sample : BL123325BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Sep 28 04:52:38 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 28 04:24:28 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	203847	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	913800	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.44	164	596398	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.18	188	1266954	20.00	ng/ul	0.00
78) Chrysene-d12	21.36	240	1280872	20.00	ng/ul	-0.01
86) Perylene-d12	23.63	264	1356681	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.27	96	33317	7.07	ng/uL	0.00
5) Phenol-d5	6.97	99	593662	32.96	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.14	67	363020	36.83	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	508145	35.03	ng/ul	0.00
13) 4-Methylphenol-d8	8.51	113	495389	33.59	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	252761	35.84	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	277665	36.06	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	506445	33.03	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	757726	40.68	ng/ul	0.00
44) Dimethylphthalate-d6	13.86	166	1712055	36.99	ng/ul	0.00
47) Acenaphthylene-d8	14.14	160	1929522	36.11	ng/ul	0.00
52) 4-Nitrophenol-d4	14.63	143	296569	32.43	ng/ul	0.00
58) Fluorene-d10	15.44	176	1436199	36.41	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.55	200	225597	27.36	ng/ul	0.00
71) Anthracene-d10	17.28	188	2304632	37.25	ng/ul	0.00
79) Pyrene-d10	19.57	212	2597652	37.68	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.49	264	2643494	37.67	ng/ul	-0.01

Target Compounds


				Ovalue		
15) N-Nitroso-di-n-propylamine	8.51	70	11791	1.018	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092719\
Data File : BM022807.D
Acq On : 28 Sep 2019 03:41
Operator : JU
Sample : BL123325BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Sep 28 04:52:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 28 04:24:28 2019
Response via : Initial Calibration

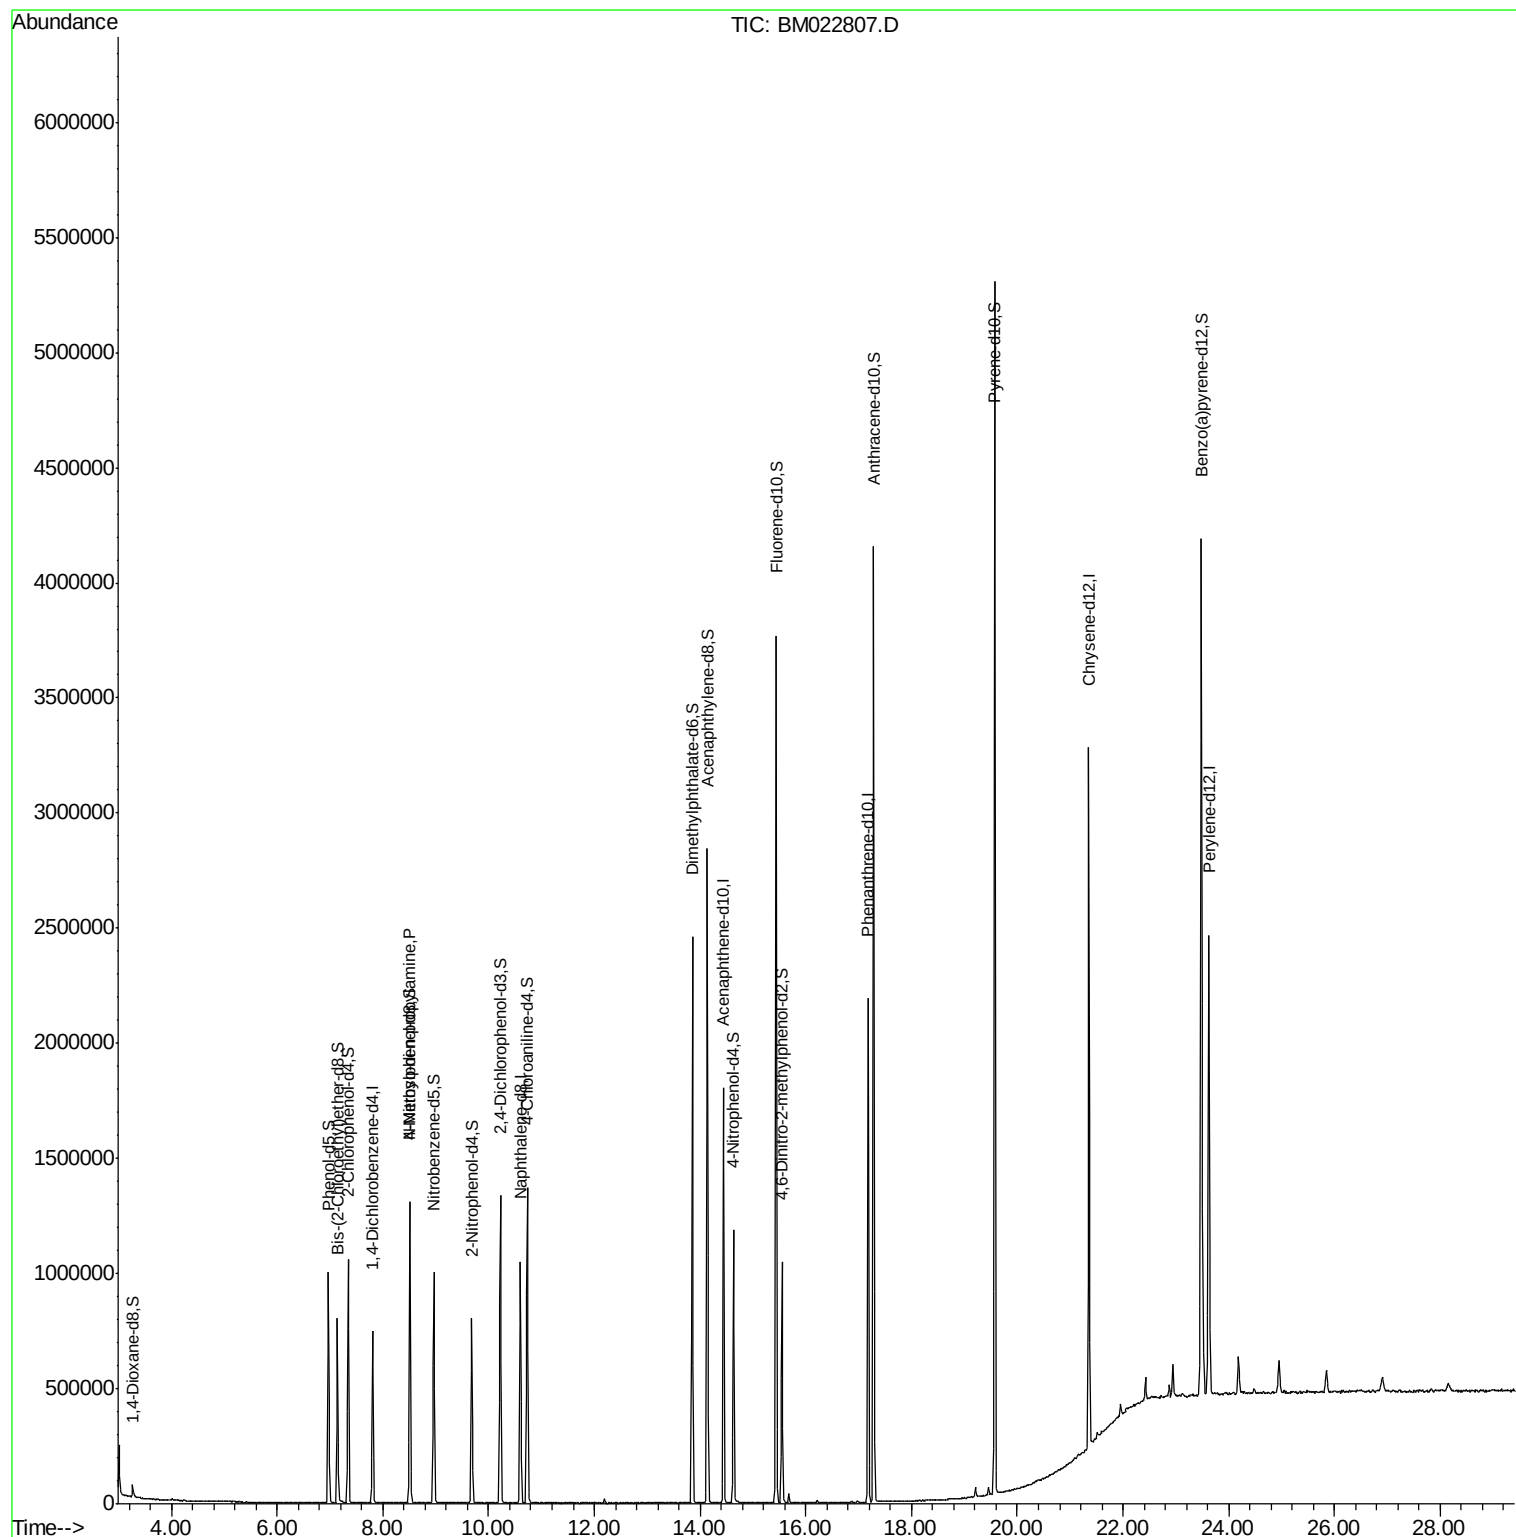

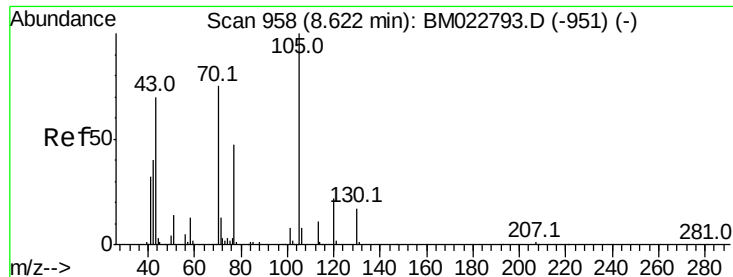

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.018 ng/ul
 RT: 8.51 min Scan# 939
 Delta R.T. -0.11 min
 Lab File: BM022807.D
 Acq: 28 Sep 2019 03:41

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ion	Ratio	Lower	Upper
70	100			
42	370.2	44.6	66.8#	
101	0.0	8.2	12.2#	
130	0.0	18.7	28.1#	

