

Data File : BM022808.D

Operator : JU

Misc :

Sample Multiplier: 1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM092719MA.M

QLast Update : Sat Sep 28 04:24:28 2019


Response via : Initial Calibration

BNA\_M

SSTD02004

**APPROVED**

mohammad  
9/30/2019 8:14:44 AM

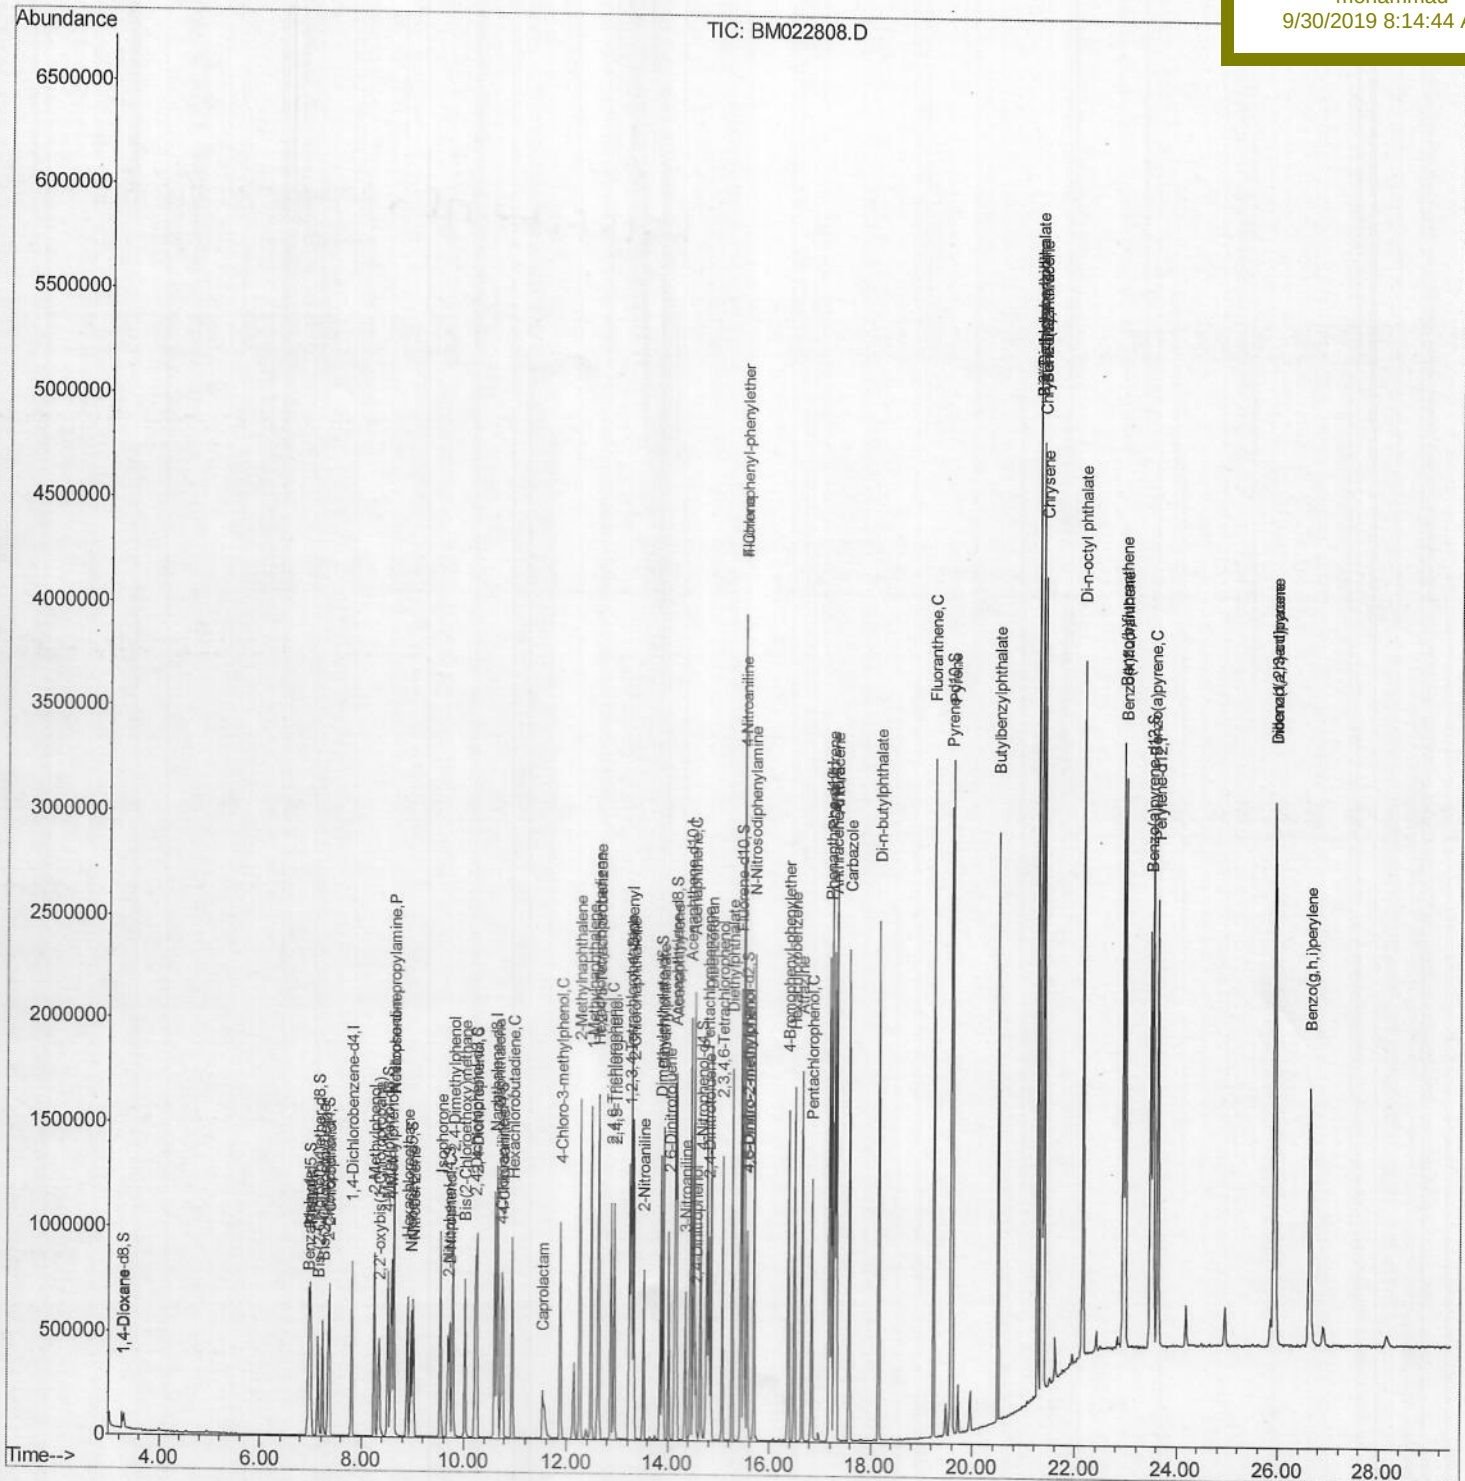




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092719\  
Data File : BM022808.D  
Acq On : 28 Sep 2019 04:18  
Operator : JU  
Sample : SSTDCCC020EC  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Sep 28 05:00:51 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM092719MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Sat Sep 28 04:24:28 2019  
Response via : Initial Calibration

Instrument :  
BNA\_M  
LabSampleId :  
SSTD02004

Manual Integrations  
APPROVED

mohammad  
9/30/2019 8:14:44 AM

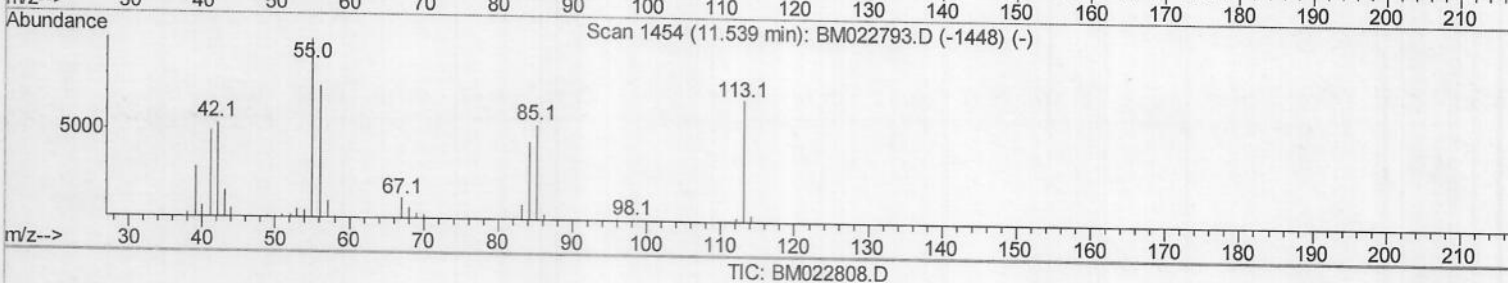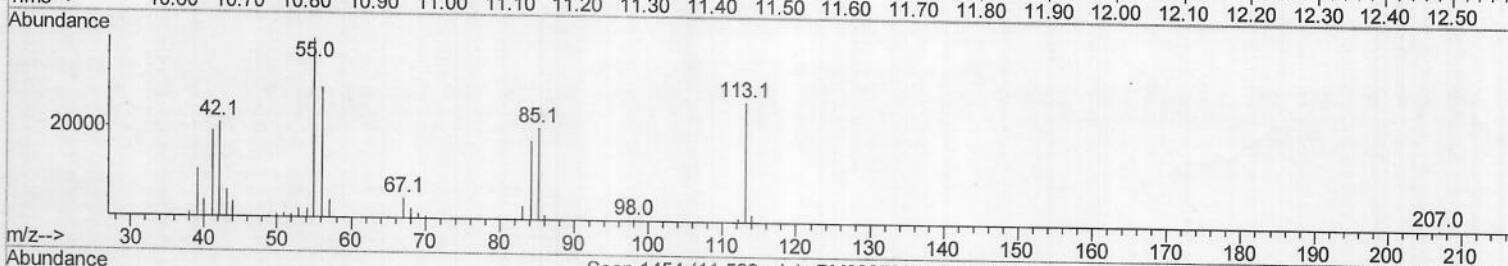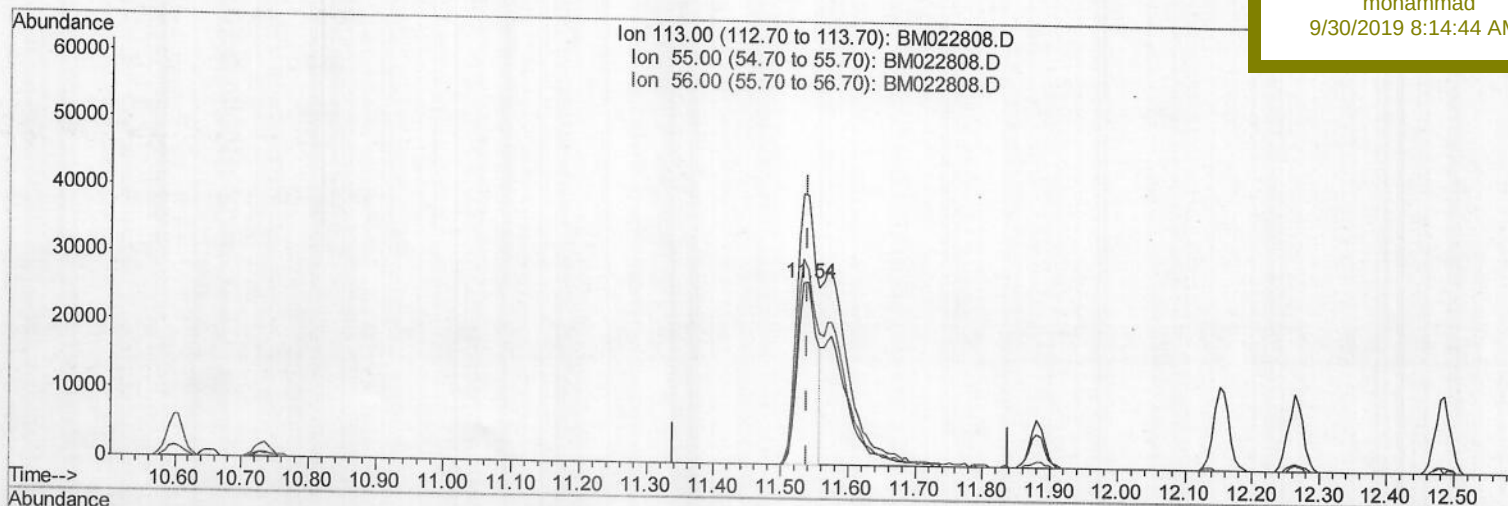

(32) Caprolactam

11.539min (+0.000) 9.39ng/ul

response 53205

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 113.00 | 100    | 100    |
| 55.00  | 150.70 | 148.03 |
| 56.00  | 114.30 | 107.39 |
| 0.00   | 0.00   | 0.00   |



Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092719\

Data File : BM022808.D

Acq On : 28 Sep 2019 04:18

Operator : JU

Sample : SSTDCCC020EC

Misc :

ALS Vial : 11 Sample Multiplier: 1

Quant Time: Sep 28 05:00:51 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM092719MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Sat Sep 28 04:24:28 2019

Response via : Initial Calibration

Instrument :

BNA\_M




LabSampleId :

SSTD02004

Manual Integrations  
APPROVED

mohammad

9/30/2019 8:14:44 AM

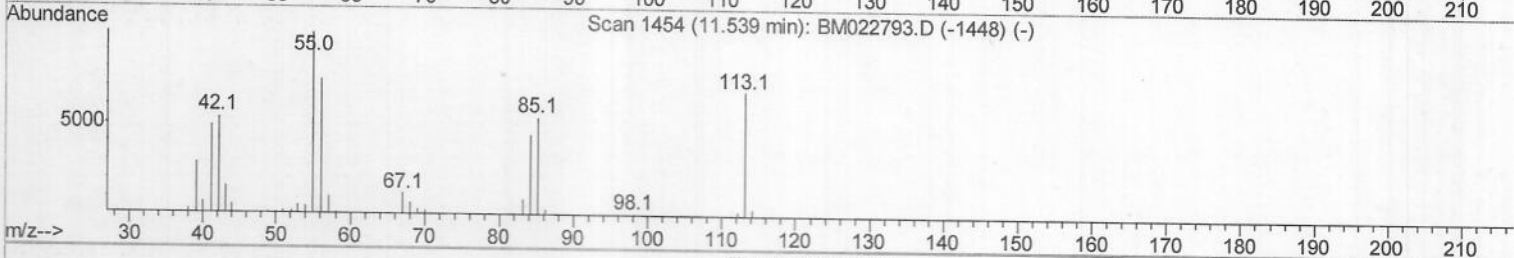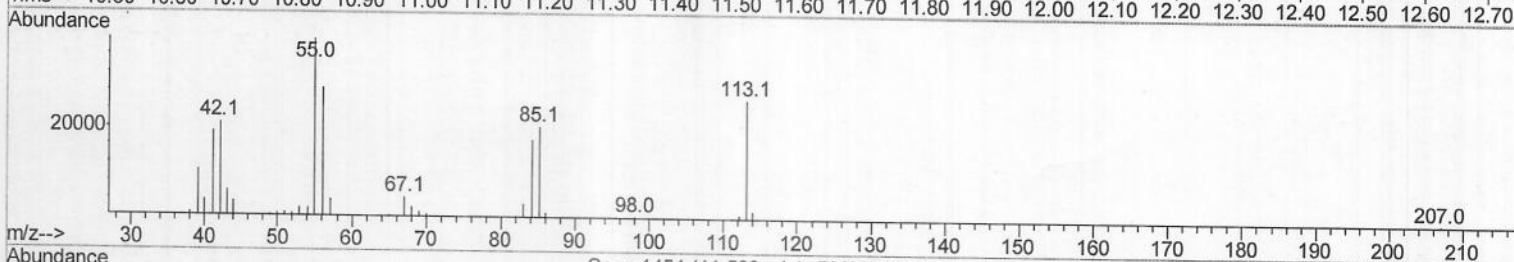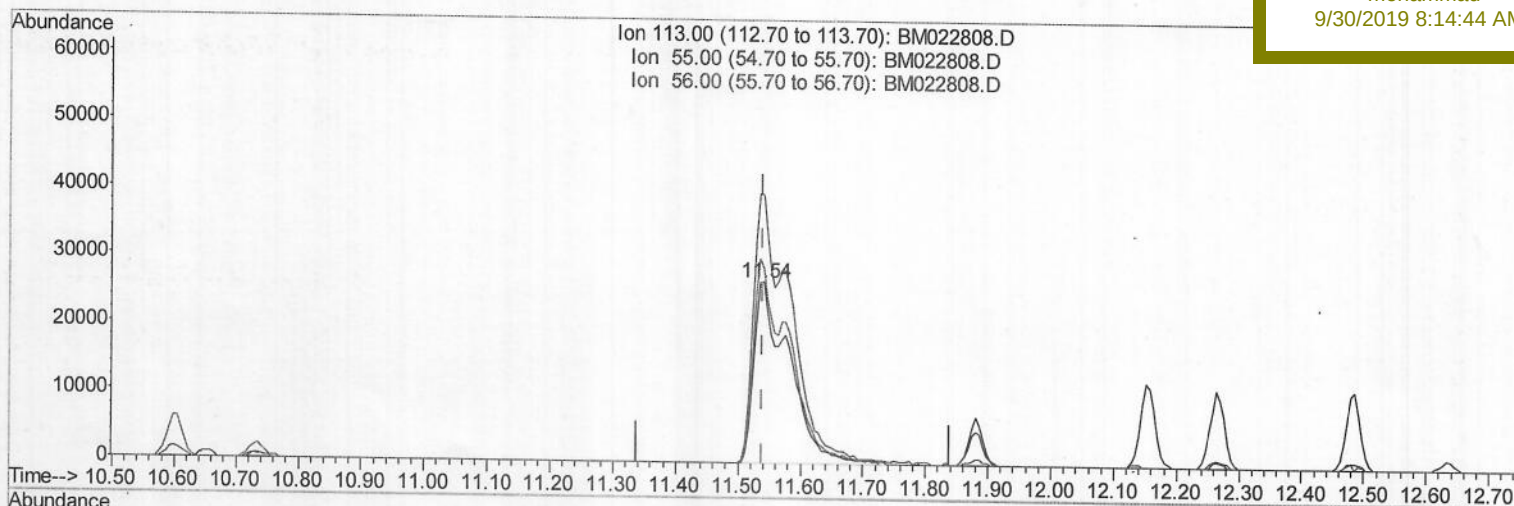

TIC: BM022808.D

(32) Caprolactam

11.539min (+0.000) 18.37ng/ul m y JU 20104129

response 104129

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 113.00 | 100    | 100    |
| 55.00  | 150.70 | 148.03 |
| 56.00  | 114.30 | 107.39 |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092719\  
 Data File : BM022808.D  
 Acq On : 28 Sep 2019 04:18  
 Operator : JU  
 Sample : SSTDCCC020EC  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 LabSampleId :  
 SSTD02004

Quant Time: Sep 28 05:02:38 2019  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM092719MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Sat Sep 28 04:24:28 2019  
 Response via : Initial Calibration

Manual Integrations  
 APPROVED

mohammad  
 9/30/2019 8:14:44 AM

| Internal Standards        | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|---------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 7.81  | 152  | 231268   | 20.00 | ng/ul | 0.00     |
| 18) Naphthalene-d8        | 10.60 | 136  | 1030778  | 20.00 | ng/ul | 0.00     |
| 36) Acenaphthene-d10      | 14.45 | 164  | 665609   | 20.00 | ng/ul | 0.00     |
| 62) Phenanthrene-d10      | 17.19 | 188  | 1395819  | 20.00 | ng/ul | 0.00     |
| 78) Chrysene-d12          | 21.36 | 240  | 1461688  | 20.00 | ng/ul | 0.00     |
| 86) Perylene-d12          | 23.63 | 264  | 1524919  | 20.00 | ng/ul | -0.01    |

## System Monitoring Compounds

|                                |       |     |         |       |       |       |
|--------------------------------|-------|-----|---------|-------|-------|-------|
| 3) 1,4-Dioxane-d8              | 3.27  | 96  | 40656   | 7.60  | ng/uL | 0.00  |
| 5) Phenol-d5                   | 6.97  | 99  | 376220  | 18.41 | ng/ul | 0.00  |
| 7) Bis-(2-Chloroethyl)ether-d  | 7.14  | 67  | 215403  | 19.26 | ng/ul | 0.00  |
| 9) 2-Chlorophenol-d4           | 7.34  | 132 | 308700  | 18.76 | ng/ul | 0.00  |
| 13) 4-Methylphenol-d8          | 8.51  | 113 | 309364  | 18.49 | ng/ul | 0.00  |
| 19) Nitrobenzene-d5            | 8.96  | 128 | 149916  | 18.84 | ng/ul | 0.00  |
| 22) 2-Nitrophenol-d4           | 9.69  | 143 | 160465  | 18.47 | ng/ul | 0.00  |
| 26) 2,4-Dichlorophenol-d3      | 10.22 | 165 | 327697  | 18.95 | ng/ul | 0.00  |
| 29) 4-Chloroaniline-d4         | 10.73 | 131 | 350865  | 16.70 | ng/ul | 0.00  |
| 44) Dimethylphthalate-d6       | 13.86 | 166 | 966019  | 18.70 | ng/ul | 0.00  |
| 47) Acenaphthylene-d8          | 14.14 | 160 | 1137856 | 19.08 | ng/ul | 0.00  |
| 52) 4-Nitrophenol-d4           | 14.63 | 143 | 188783  | 18.50 | ng/ul | 0.00  |
| 58) Fluorene-d10               | 15.43 | 176 | 838138  | 19.04 | ng/ul | 0.00  |
| 63) 4,6-Dinitro-2-methylphenol | 15.55 | 200 | 147997  | 16.29 | ng/ul | 0.00  |
| 71) Anthracene-d10             | 17.28 | 188 | 1300633 | 19.08 | ng/ul | 0.00  |
| 79) Pyrene-d10                 | 19.57 | 212 | 1459501 | 18.55 | ng/ul | 0.00  |
| 90) Benzo(a)pyrene-d12         | 23.48 | 264 | 1472847 | 18.67 | ng/ul | -0.02 |

## Target Compounds

|                                |       |     |         |        |       | Ovalue |
|--------------------------------|-------|-----|---------|--------|-------|--------|
| 2) 1,4-Dioxane                 | 3.30  | 88  | 39171   | 7.405  | ng/uL | 97     |
| 4) Benzaldehyde                | 6.95  | 77  | 137784  | 14.879 | ng/ul | 99     |
| 6) Phenol                      | 7.00  | 94  | 397161  | 18.540 | ng/ul | 99     |
| 8) Bis(2-Chloroethyl)ether     | 7.23  | 93  | 310622  | 19.173 | ng/ul | 99     |
| 10) 2-Chlorophenol             | 7.37  | 128 | 327610  | 18.560 | ng/ul | 99     |
| 11) 2-Methylphenol             | 8.25  | 108 | 306095  | 18.540 | ng/ul | 100    |
| 12) 2,2'-oxybis(1-Chloropropan | 8.34  | 45  | 425746  | 19.875 | ng/ul | 99     |
| 14) Acetophenone               | 8.63  | 105 | 490984  | 19.197 | ng/ul | 99     |
| 15) N-Nitroso-di-n-propylamine | 8.62  | 70  | 250659  | 19.082 | ng/ul | 99     |
| 16) 4-Methylphenol             | 8.57  | 108 | 340262  | 18.639 | ng/ul | 98     |
| 17) Hexachloroethane           | 8.89  | 117 | 127901  | 19.067 | ng/ul | 97     |
| 20) Nitrobenzene               | 9.00  | 77  | 350307  | 18.864 | ng/ul | 99     |
| 21) Isophorone                 | 9.53  | 82  | 700095  | 19.137 | ng/ul | 100    |
| 23) 2-Nitrophenol              | 9.72  | 139 | 184127  | 18.533 | ng/ul | 99     |
| 24) 2,4-Dimethylphenol         | 9.77  | 107 | 366880  | 18.966 | ng/ul | 99     |
| 25) Bis(2-Chloroethoxy)methane | 10.01 | 93  | 447139  | 19.164 | ng/ul | 99     |
| 27) 2,4-Dichlorophenol         | 10.25 | 162 | 329045  | 18.796 | ng/ul | 99     |
| 28) Naphthalene                | 10.65 | 128 | 1063273 | 19.100 | ng/ul | 99     |
| 30) 4-Chloroaniline            | 10.76 | 127 | 375046  | 16.947 | ng/ul | 99     |
| 31) Hexachlorobutadiene        | 10.95 | 225 | 201319  | 19.007 | ng/ul | 100    |
| 32) Caprolactam                | 11.54 | 113 | 104129m | 18.371 | ng/ul | 100    |
| 33) 4-Chloro-3-methylphenol    | 11.88 | 107 | 341402  | 18.943 | ng/ul | 100    |
| 34) 2-Methylnaphthalene        | 12.26 | 142 | 796517  | 19.084 | ng/ul | 99     |

3 TO  
 20/04/19



Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092719\  
 Data File : BM022808.D  
 Acq On : 28 Sep 2019 04:18  
 Operator : JU  
 Sample : SSTDCCC020EC  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 LabSampleId :  
 SSTD02004

Quant Time: Sep 28 05:02:38 2019  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM092719MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Sat Sep 28 04:24:28 2019  
 Response via : Initial Calibration

Manual Integrations  
 APPROVED

mohammad  
 9/30/2019 8:14:44 AM

| Internal Standards             | R.T.  | QIon | Response | Conc   | Units | Dev(Min) |
|--------------------------------|-------|------|----------|--------|-------|----------|
| 35) 1-Methylnaphthalene        | 12.49 | 142  | 762909   | 19.138 | ng/ul | 99       |
| 37) 1,2,4,5-Tetrachlorobenzene | 12.63 | 216  | 412808   | 18.903 | ng/ul | 99       |
| 38) Hexachlorocyclopentadiene  | 12.62 | 237  | 227833   | 16.646 | ng/ul | 98       |
| 39) 2,4,6-Trichlorophenol      | 12.87 | 196  | 272736   | 18.830 | ng/ul | 99       |
| 40) 2,4,5-Trichlorophenol      | 12.95 | 196  | 297005   | 18.802 | ng/ul | 99       |
| 41) 1,1'-Biphenyl              | 13.28 | 154  | 1036488  | 19.018 | ng/ul | 100      |
| 42) 2-Chloronaphthalene        | 13.32 | 162  | 792457   | 19.019 | ng/ul | 99       |
| 43) 2-Nitroaniline             | 13.52 | 65   | 206835   | 19.142 | ng/ul | 99       |
| 45) Dimethylphthalate          | 13.90 | 163  | 1007970  | 18.994 | ng/ul | 99       |
| 46) 2,6-Dinitrotoluene         | 14.02 | 165  | 203306   | 19.214 | ng/ul | 99       |
| 48) Acenaphthylene             | 14.17 | 152  | 1237780  | 19.224 | ng/ul | 99       |
| 49) 3-Nitroaniline             | 14.34 | 138  | 179955   | 17.533 | ng/ul | 98       |
| 50) Acenaphthene               | 14.51 | 153  | 851625   | 18.987 | ng/ul | 100      |
| 51) 2,4-Dinitrophenol          | 14.55 | 184  | 100677   | 14.909 | ng/ul | 97       |
| 53) 4-Nitrophenol              | 14.65 | 109  | 140124   | 18.784 | ng/ul | 98       |
| 54) Dibenzofuran               | 14.85 | 168  | 1210327  | 18.894 | ng/ul | 99       |
| 55) 2,4-Dinitrotoluene         | 14.80 | 165  | 294227   | 18.847 | ng/ul | 100      |
| 56) 2,3,4,6-Tetrachlorophenol  | 15.07 | 232  | 259205   | 18.650 | ng/ul | 96       |
| 57) Diethylphthalate           | 15.27 | 149  | 1022960  | 19.201 | ng/ul | 100      |
| 59) Fluorene                   | 15.49 | 166  | 990599   | 19.136 | ng/ul | 100      |
| 60) 4-Chlorophenyl-phenylether | 15.49 | 204  | 502442   | 19.148 | ng/ul | 98       |
| 61) 4-Nitroaniline             | 15.50 | 138  | 212604   | 18.337 | ng/ul | 99       |
| 64) 4,6-Dinitro-2-methylphenol | 15.57 | 198  | 169809   | 16.716 | ng/ul | 95       |
| 65) N-Nitrosodiphenylamine     | 15.70 | 169  | 869372   | 18.949 | ng/ul | 100      |
| 66) 4-Bromophenyl-phenylether  | 16.38 | 248  | 317125   | 18.833 | ng/ul | 98       |
| 67) Hexachlorobenzene          | 16.50 | 284  | 353868   | 18.848 | ng/ul | 98       |
| 68) Atrazine                   | 16.65 | 200  | 314448   | 18.747 | ng/ul | 99       |
| 69) Pentachlorophenol          | 16.83 | 266  | 212874   | 17.478 | ng/ul | 99       |
| 70) Phenanthrene               | 17.23 | 178  | 1581178  | 18.981 | ng/ul | 100      |
| 72) Anthracene                 | 17.32 | 178  | 1626331  | 19.160 | ng/ul | 99       |
| 73) 1,2,3,4-Tetrachlorobenzene | 13.25 | 216  | 409375   | 18.793 | ng/uL | 98       |
| 74) Pentachlorobenzene         | 14.77 | 250  | 411630   | 18.931 | ng/uL | 99       |
| 75) Carbazole                  | 17.58 | 167  | 1471171  | 19.501 | ng/ul | 100      |
| 76) Di-n-butylphthalate        | 18.15 | 149  | 1755458  | 19.736 | ng/ul | 100      |
| 77) Fluoranthene               | 19.24 | 202  | 1877267  | 20.037 | ng/ul | 99       |
| 80) Pvrene                     | 19.60 | 202  | 1959268  | 18.909 | ng/ul | 99       |
| 81) Butylbenzylphthalate       | 20.50 | 149  | 825854   | 19.380 | ng/ul | 96       |
| 82) 3,3'-Dichlorobenzidine     | 21.27 | 252  | 603505   | 18.125 | ng/ul | 99       |
| 83) Benzo(a)anthracene         | 21.34 | 228  | 1996331  | 19.023 | ng/ul | 100      |
| 84) Bis(2-ethylhexyl)phthalate | 21.28 | 149  | 1257539  | 20.769 | ng/ul | 100      |
| 85) Chrysene                   | 21.40 | 228  | 1847889  | 19.099 | ng/ul | 99       |
| 87) Di-n-octyl phthalate       | 22.16 | 149  | 2122080  | 20.462 | ng/ul | 100      |
| 88) Benzo(b)fluoranthene       | 22.94 | 252  | 1964409  | 19.412 | ng/ul | 99       |
| 89) Benzo(k)fluoranthene       | 22.99 | 252  | 1797758  | 18.569 | ng/ul | 100      |
| 91) Benzo(a)pyrene             | 23.53 | 252  | 1771470  | 18.659 | ng/ul | 99       |
| 92) Indeno(1,2,3-cd)pyrene     | 25.93 | 276  | 1877922  | 18.622 | ng/ul | 99       |
| 93) Dibenzo(a,h)anthracene     | 25.94 | 278  | 1590099  | 18.849 | ng/ul | 100      |
| 94) Benzo(a,h,i)perylene       | 26.63 | 276  | 1505000  | 18.499 | ng/ul | 99       |

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092719\  
Data File : BM022808.D  
Acq On : 28 Sep 2019 04:18  
Operator : JU  
Sample : SSTDCCC020EC  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Sep 28 05:02:38 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM092719MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Sat Sep 28 04:24:28 2019  
Response via : Initial Calibration

Instrument :  
BNA\_M  
LabSampleId :  
SSTD02004

Manual Integrations  
APPROVED

mohammad  
9/30/2019 8:14:44 AM

| Internal Standards                                                         | R.T. | QIon | Response | Conc | Units | Dev(Min) |
|----------------------------------------------------------------------------|------|------|----------|------|-------|----------|
| -----                                                                      |      |      |          |      |       |          |
| (#) = qualifier out of range (m) = manual integration (+) = signals summed |      |      |          |      |       |          |