

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092719\
 Data File : BM022806.D
 Acq On : 28 Sep 2019 03:05
 Operator : JU
 Sample : PB123342BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK42

Quant Time: Sep 28 04:52:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 28 04:24:28 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	253949	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	1121558	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.44	164	733843	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.18	188	1551078	20.00	ng/ul	0.00
78) Chrysene-d12	21.36	240	1625151	20.00	ng/ul	-0.01
86) Perylene-d12	23.63	264	1777721	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.28	96	15509	2.64	ng/uL	0.00
5) Phenol-d5	6.97	99	270140	12.04	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.14	67	415052	33.80	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	514726	28.49	ng/ul	0.00
13) 4-Methylphenol-d8	8.51	113	376308	20.48	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	300445	34.71	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	330238	34.94	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	569747	30.28	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	204319	8.94	ng/ul	0.00
44) Dimethylphthalate-d6	13.86	166	2034319	35.72	ng/ul	0.00
47) Acenaphthylene-d8	14.14	160	2287549	34.79	ng/ul	0.00
52) 4-Nitrophenol-d4	14.63	143	120549	10.71	ng/ul	-0.01
58) Fluorene-d10	15.44	176	1707110	35.17	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.55	200	279843	27.72	ng/ul	0.00
71) Anthracene-d10	17.28	188	2728422	36.02	ng/ul	0.00
79) Pyrene-d10	19.57	212	3182474	36.38	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.49	264	3402652	37.00	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.90	163	129056	2.206	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092719\
Data File : BM022806.D
Acq On : 28 Sep 2019 03:05
Operator : JU
Sample : PB123342BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK42

Quant Time: Sep 28 04:52:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM092719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 28 04:24:28 2019
Response via : Initial Calibration

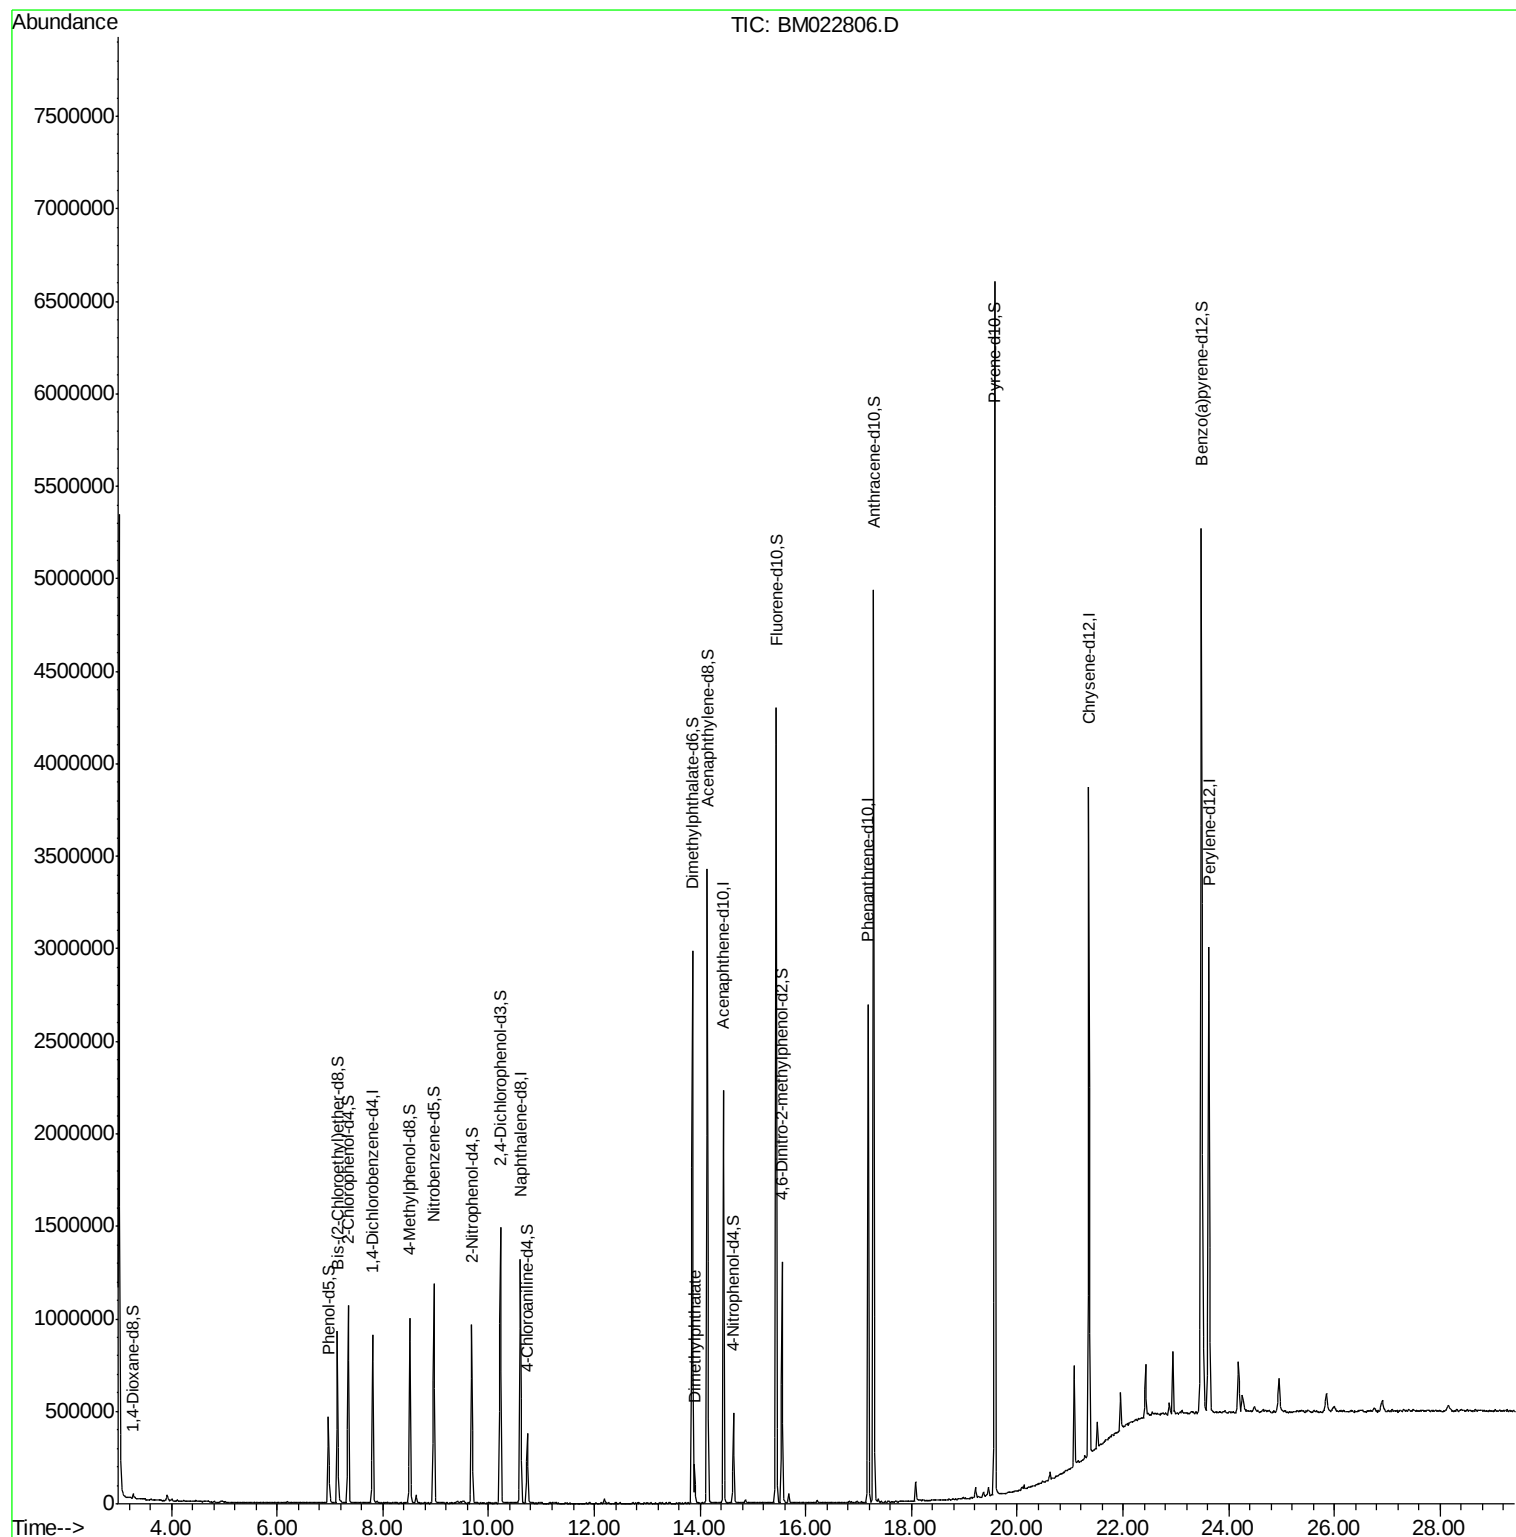

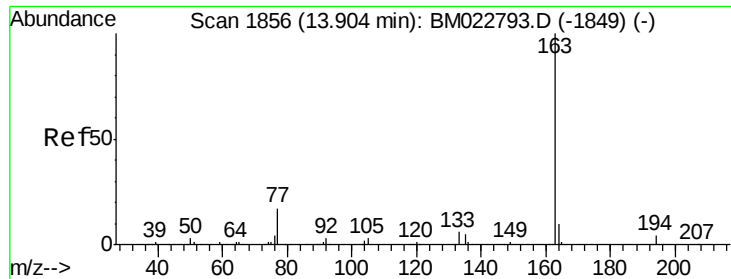

#45

Dimethylphthalate

Concen: 2.206 ng/ul

RT: 13.90 min Scan# 1855

Delta R.T. -0.01 min

Lab File: BM022806.D

Acq: 28 Sep 2019 03:05

Instrument :

BNA_M

ClientSampleId :

SBLK42


Tot Ion:163 Resp: 129056

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.0

164 10.1 8.1 12.1

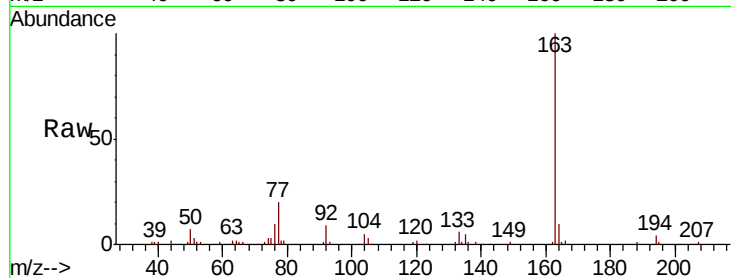

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

