

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092721\
 Data File : BM032207.D
 Acq On : 27 Sep 2021 16:22
 Operator : CG/JU
 Sample : M3919-10DL 2X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB6Y9DL

Quant Time: Sep 27 16:52:33 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 27 13:37:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.664	152	9083	0.400	ng/ul	0.00
4) Naphthalene-d8	10.456	136	29918	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.308	164	15759	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.033	188	30106	0.400	ng/ul	0.00
17) Chrysene-d12	21.196	240	19723	0.400	ng/ul	0.00
23) Perylene-d12	23.361	264	16218	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.993	96	25418	2.603	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.044	152	6422	0.161	ng/ul	0.00
18) Fluoranthene-d10	19.053	212	11333	0.212	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.027	88	16250	1.618	ng/ul	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092721\
Data File : BM032207.D
Acq On : 27 Sep 2021 16:22
Operator : CG/JU
Sample : M3919-10DL 2X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB6Y9DL

Quant Time: Sep 27 16:52:33 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 27 13:37:22 2021
Response via : Initial Calibration

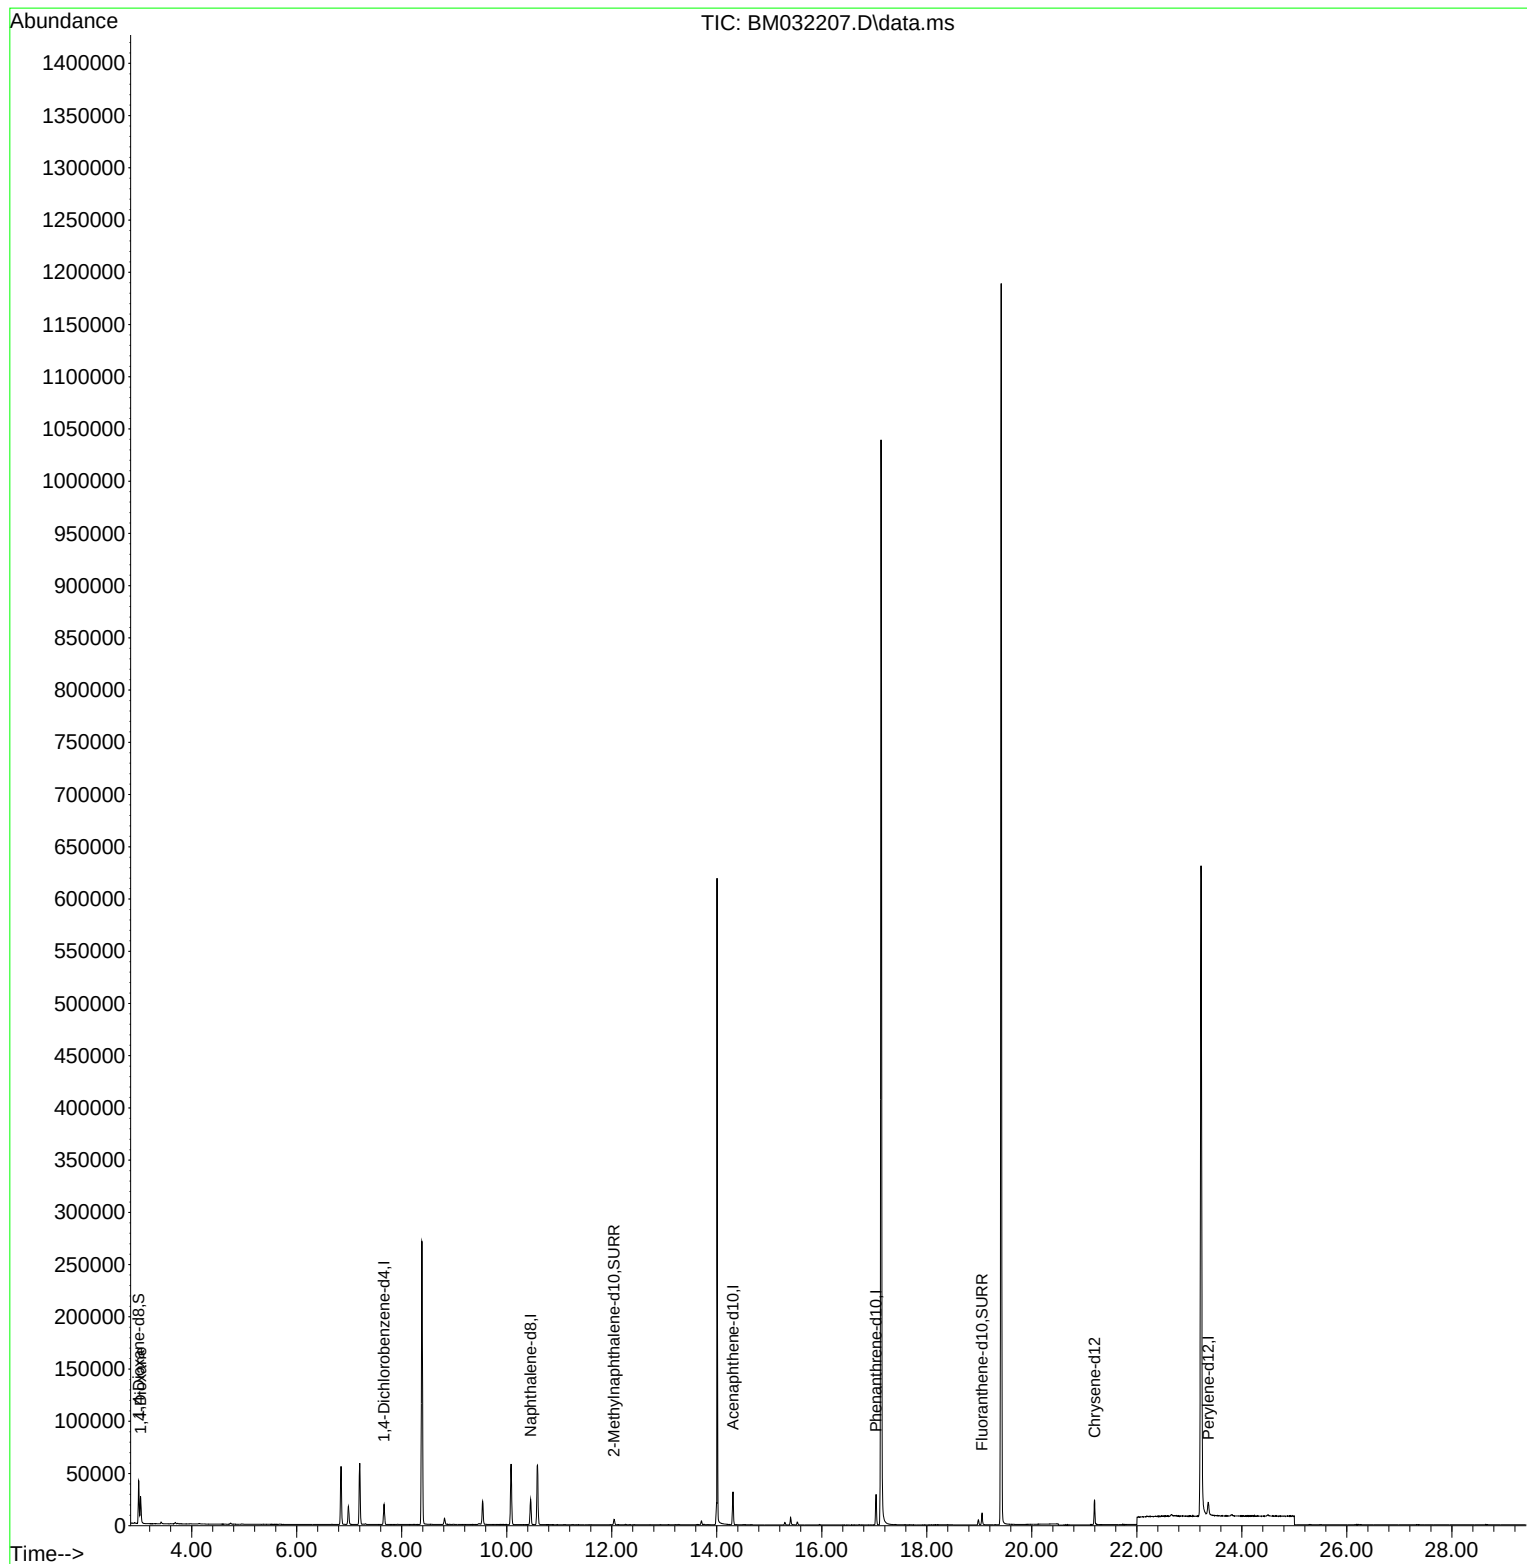

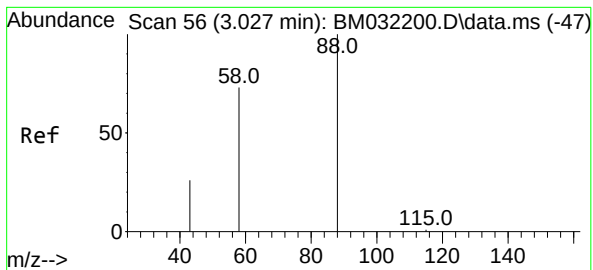

#2
 1,4-Dioxane
 Concen: 1.618 ng/ul
 RT: 3.027 min Scan# 56
 Delta R.T. 0.000 min
 Lab File: BM032207.D
 Acq: 27 Sep 2021 16:22

Instrument :
 BNA_M
 ClientSampleId :
 GB6Y9DL

Tgt Ion: 88 Resp: 16250

Ion	Ratio	Lower	Upper
88	100		
43	28.6	26.1	39.1
58	70.9	50.2	75.2

