

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092721\
 Data File : BM032212.D
 Acq On : 27 Sep 2021 19:29
 Operator : CG/JU
 Sample : M3919-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB6Y7

Quant Time: Sep 28 02:29:42 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 27 13:37:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.664	152	8081	0.400	ng/ul	0.00
4) Naphthalene-d8	10.456	136	24489	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.308	164	11808	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.033	188	20469	0.400	ng/ul	0.00
17) Chrysene-d12	21.193	240	13761	0.400	ng/ul	0.00
23) Perylene-d12	23.361	264	12952	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.989	96	41038	4.724	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.044	152	9029	0.277	ng/ul	0.00
18) Fluoranthene-d10	19.053	212	16909	0.452	ng/ul	0.00
Target Compounds						
15) Phenanthrene	17.075	178	3400	0.051	ng/ul#	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092721\
Data File : BM032212.D
Acq On : 27 Sep 2021 19:29
Operator : CG/JU
Sample : M3919-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB6Y7


Quant Time: Sep 28 02:29:42 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 27 13:37:22 2021
Response via : Initial Calibration

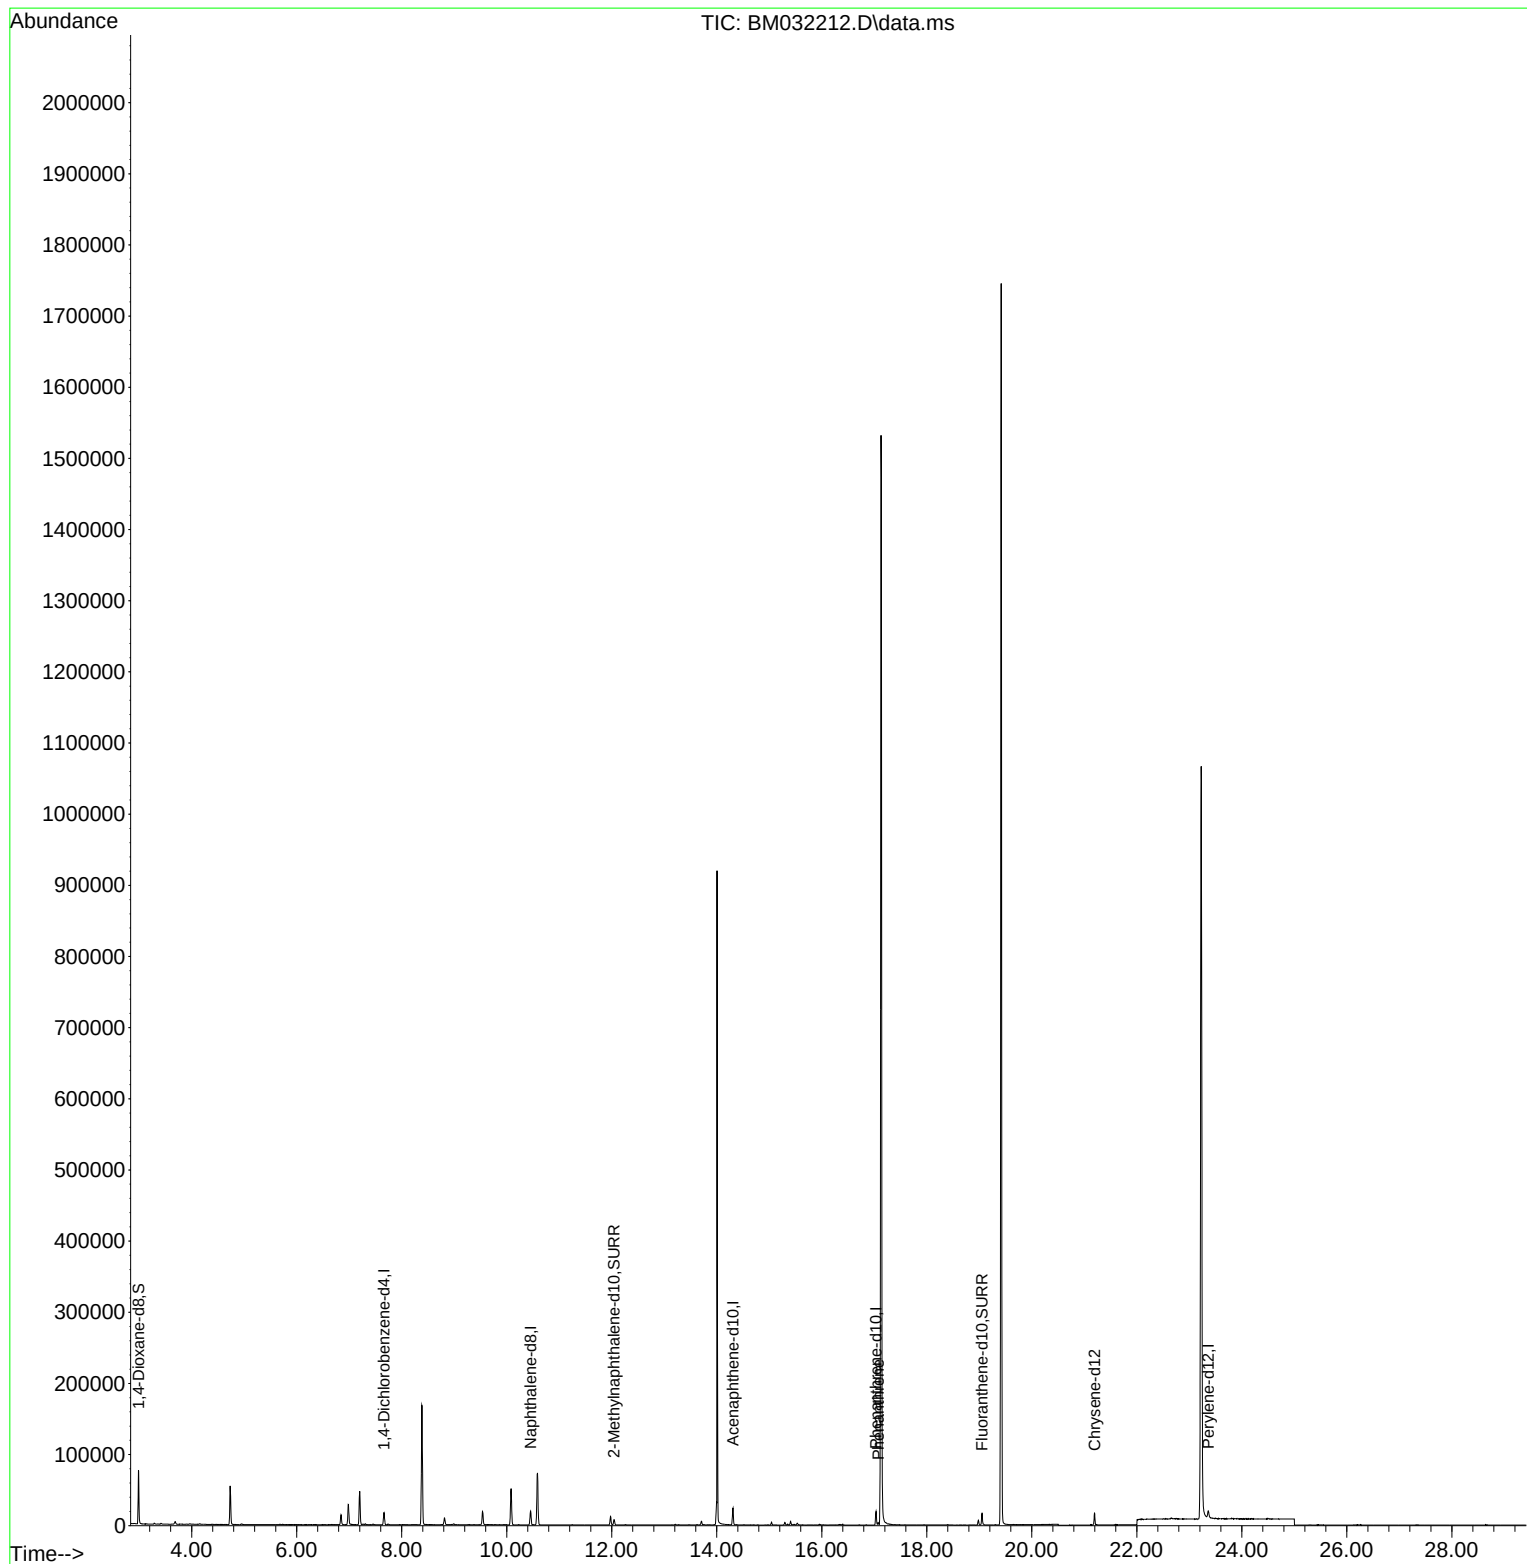

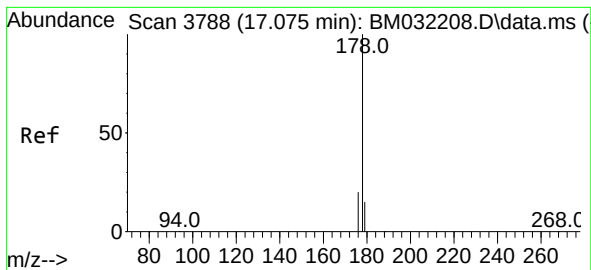

#15
Phenanthrene
Concen: 0.051 ng/ul
RT: 17.075 min Scan# 3788
Delta R.T. 0.000 min
Lab File: BM032212.D
Acq: 27 Sep 2021 19:29

Instrument :
BNA_M
ClientSampleId :
GB6Y7

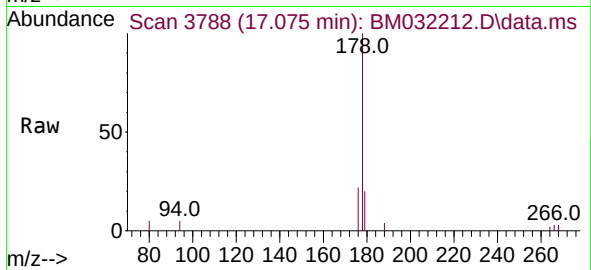

Tgt Ion:178 Resp: 3400
Ion Ratio Lower Upper
178 100
179 20.1 12.6 18.8#
176 21.6 15.8 23.6

