

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092721\
 Data File : BM032213.D
 Acq On : 27 Sep 2021 20:05
 Operator : CG/JU
 Sample : M3919-12
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB6Z1

Quant Time: Sep 28 02:29:51 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 27 13:37:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.664	152	7248	0.400	ng/ul	0.00
4) Naphthalene-d8	10.456	136	22307	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.308	164	11287	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.033	188	20291	0.400	ng/ul	0.00
17) Chrysene-d12	21.193	240	14939	0.400	ng/ul	0.00
23) Perylene-d12	23.358	264	14635	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.989	96	40729	5.227	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.044	152	10976	0.370	ng/ul	0.00
18) Fluoranthene-d10	19.050	212	20416	0.503	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.027	88	7843	0.978	ng/ul	94
15) Phenanthrene	17.075	178	2184	0.033	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092721\
Data File : BM032213.D
Acq On : 27 Sep 2021 20:05
Operator : CG/JU
Sample : M3919-12
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB6Z1

Quant Time: Sep 28 02:29:51 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 27 13:37:22 2021
Response via : Initial Calibration




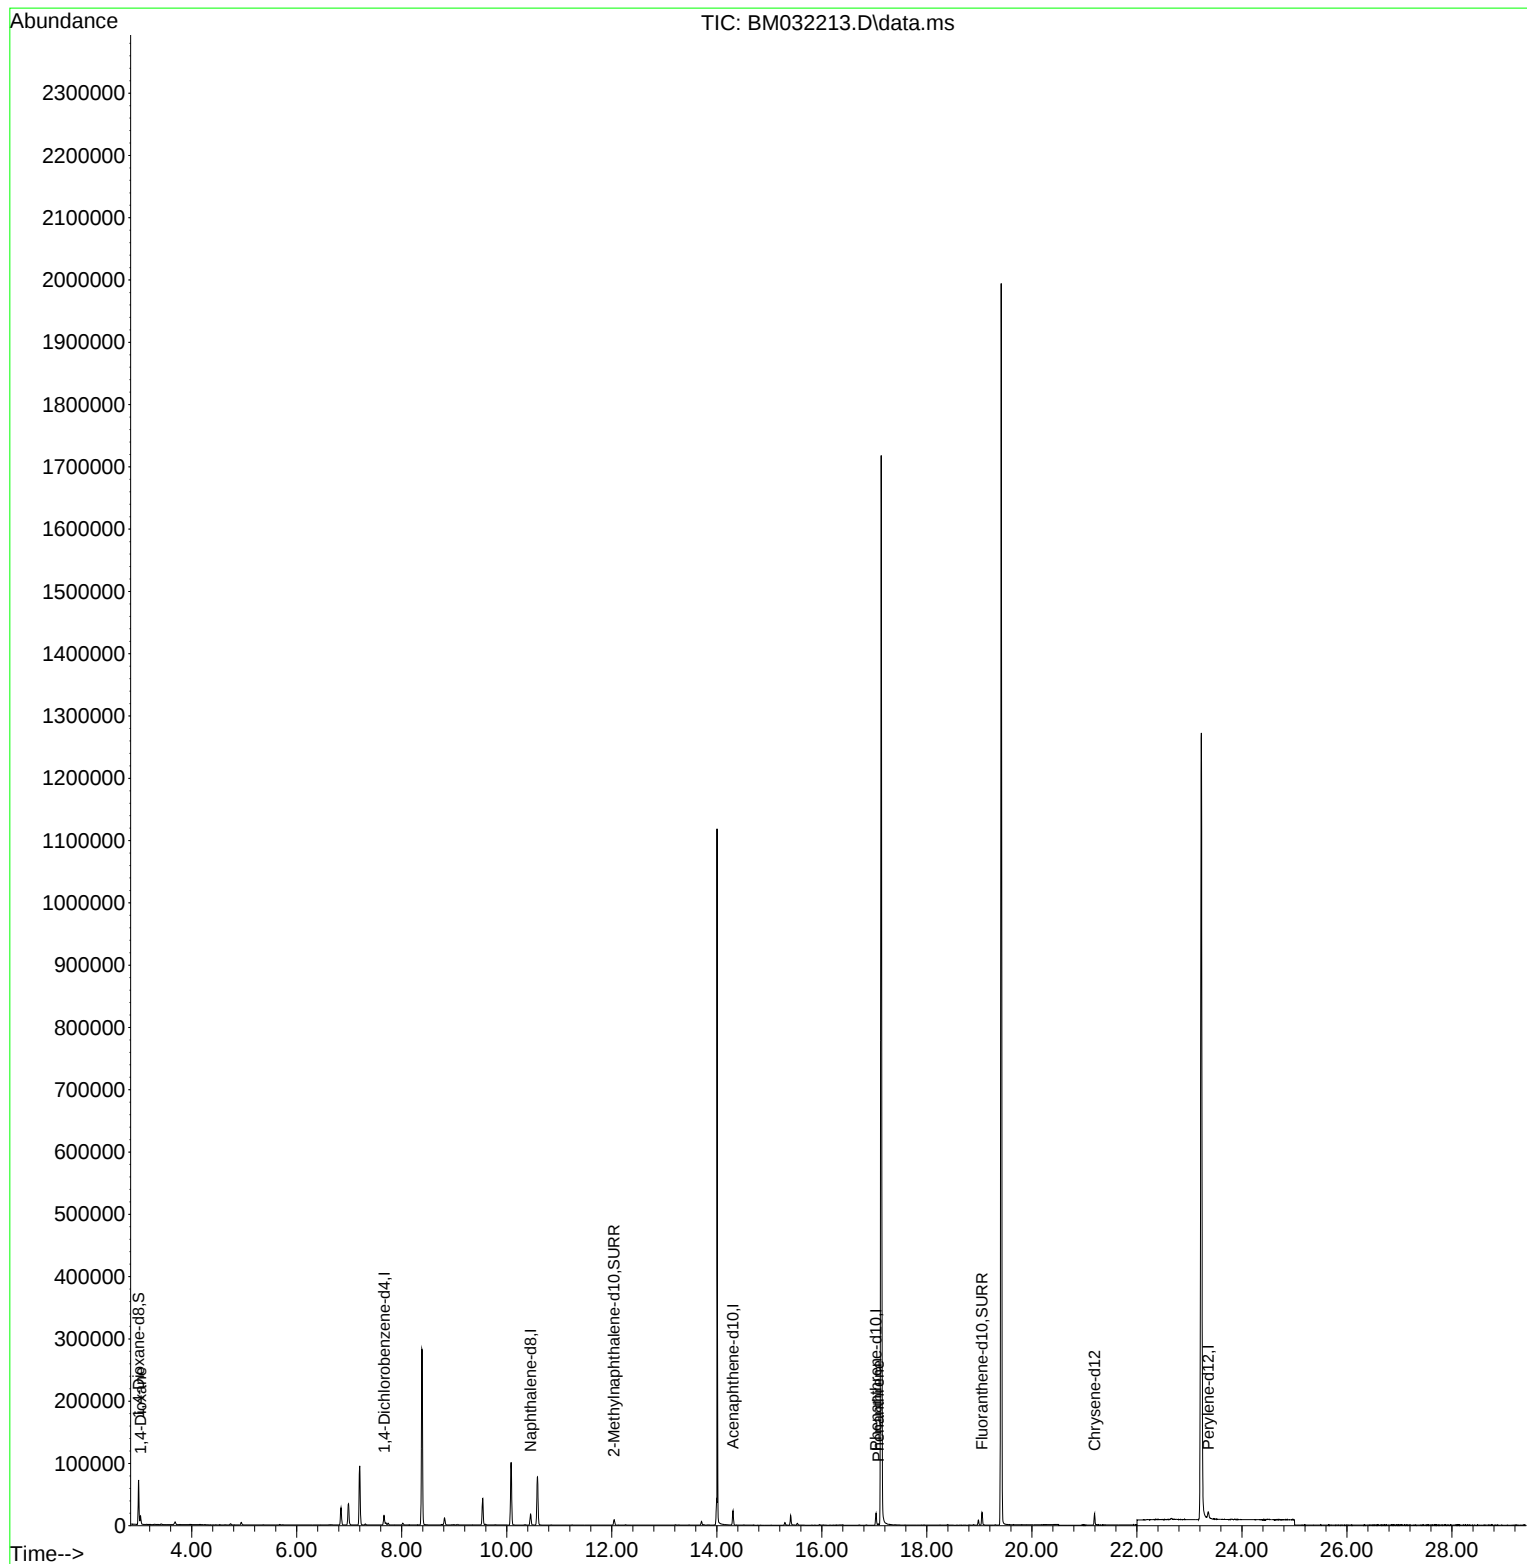


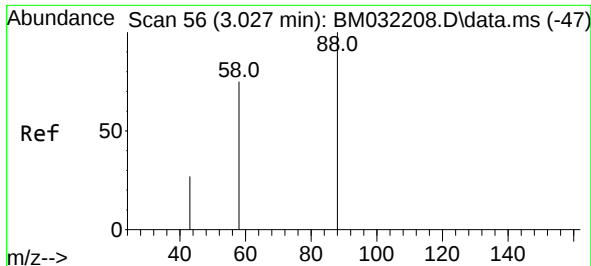

#2
1,4-Dioxane
Concen: 0.978 ng/ul
RT: 3.027 min Scan# 56
Delta R.T. 0.000 min
Lab File: BM032213.D
Acq: 27 Sep 2021 20:05

Instrument :
BNA_M
ClientSampled :
GB6Z1

Tgt Ion: 88 Resp: 7843
Ion Ratio Lower Upper
88 100
43 30.6 26.1 39.1
58 67.8 50.2 75.2

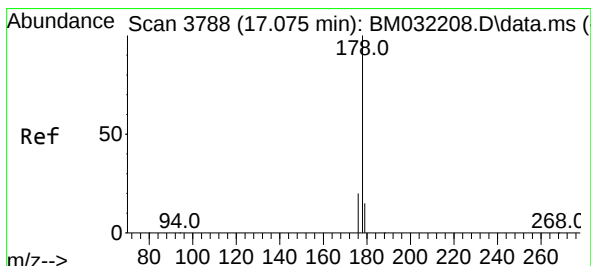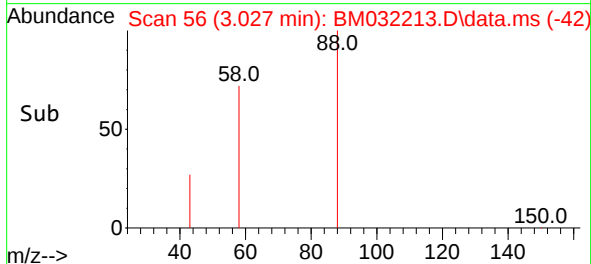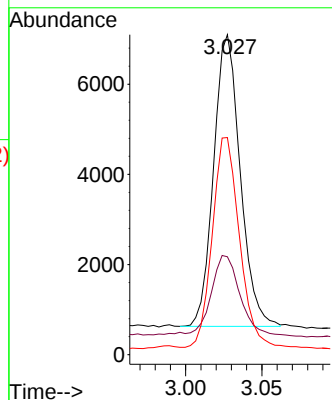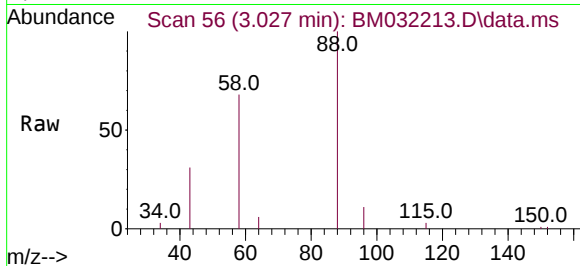

#15
Phenanthrene
Concen: 0.033 ng/ul
RT: 17.075 min Scan# 3788
Delta R.T. 0.000 min
Lab File: BM032213.D
Acq: 27 Sep 2021 20:05

Tgt Ion: 178 Resp: 2184
Ion Ratio Lower Upper
178 100
179 22.1 12.6 18.8#
176 24.0 15.8 23.6#

