

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092721\
 Data File : BM032214.D
 Acq On : 27 Sep 2021 20:42
 Operator : CG/JU
 Sample : M3919-19
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB6Z8

Quant Time: Sep 28 02:29:59 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 27 13:37:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.664	152	8480	0.400	ng/ul	0.00
4) Naphthalene-d8	10.456	136	28412	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.308	164	15855	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.033	188	31080	0.400	ng/ul	0.00
17) Chrysene-d12	21.193	240	21201	0.400	ng/ul	0.00
23) Perylene-d12	23.358	264	18009	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.989	96	47958	5.261	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.044	152	14348	0.379	ng/ul	0.00
18) Fluoranthene-d10	19.049	212	32091	0.557	ng/ul	0.00
Target Compounds						
15) Phenanthrene	17.074	178	13753	0.136	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092721\
Data File : BM032214.D
Acq On : 27 Sep 2021 20:42
Operator : CG/JU
Sample : M3919-19
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB6Z8


Quant Time: Sep 28 02:29:59 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 27 13:37:22 2021
Response via : Initial Calibration

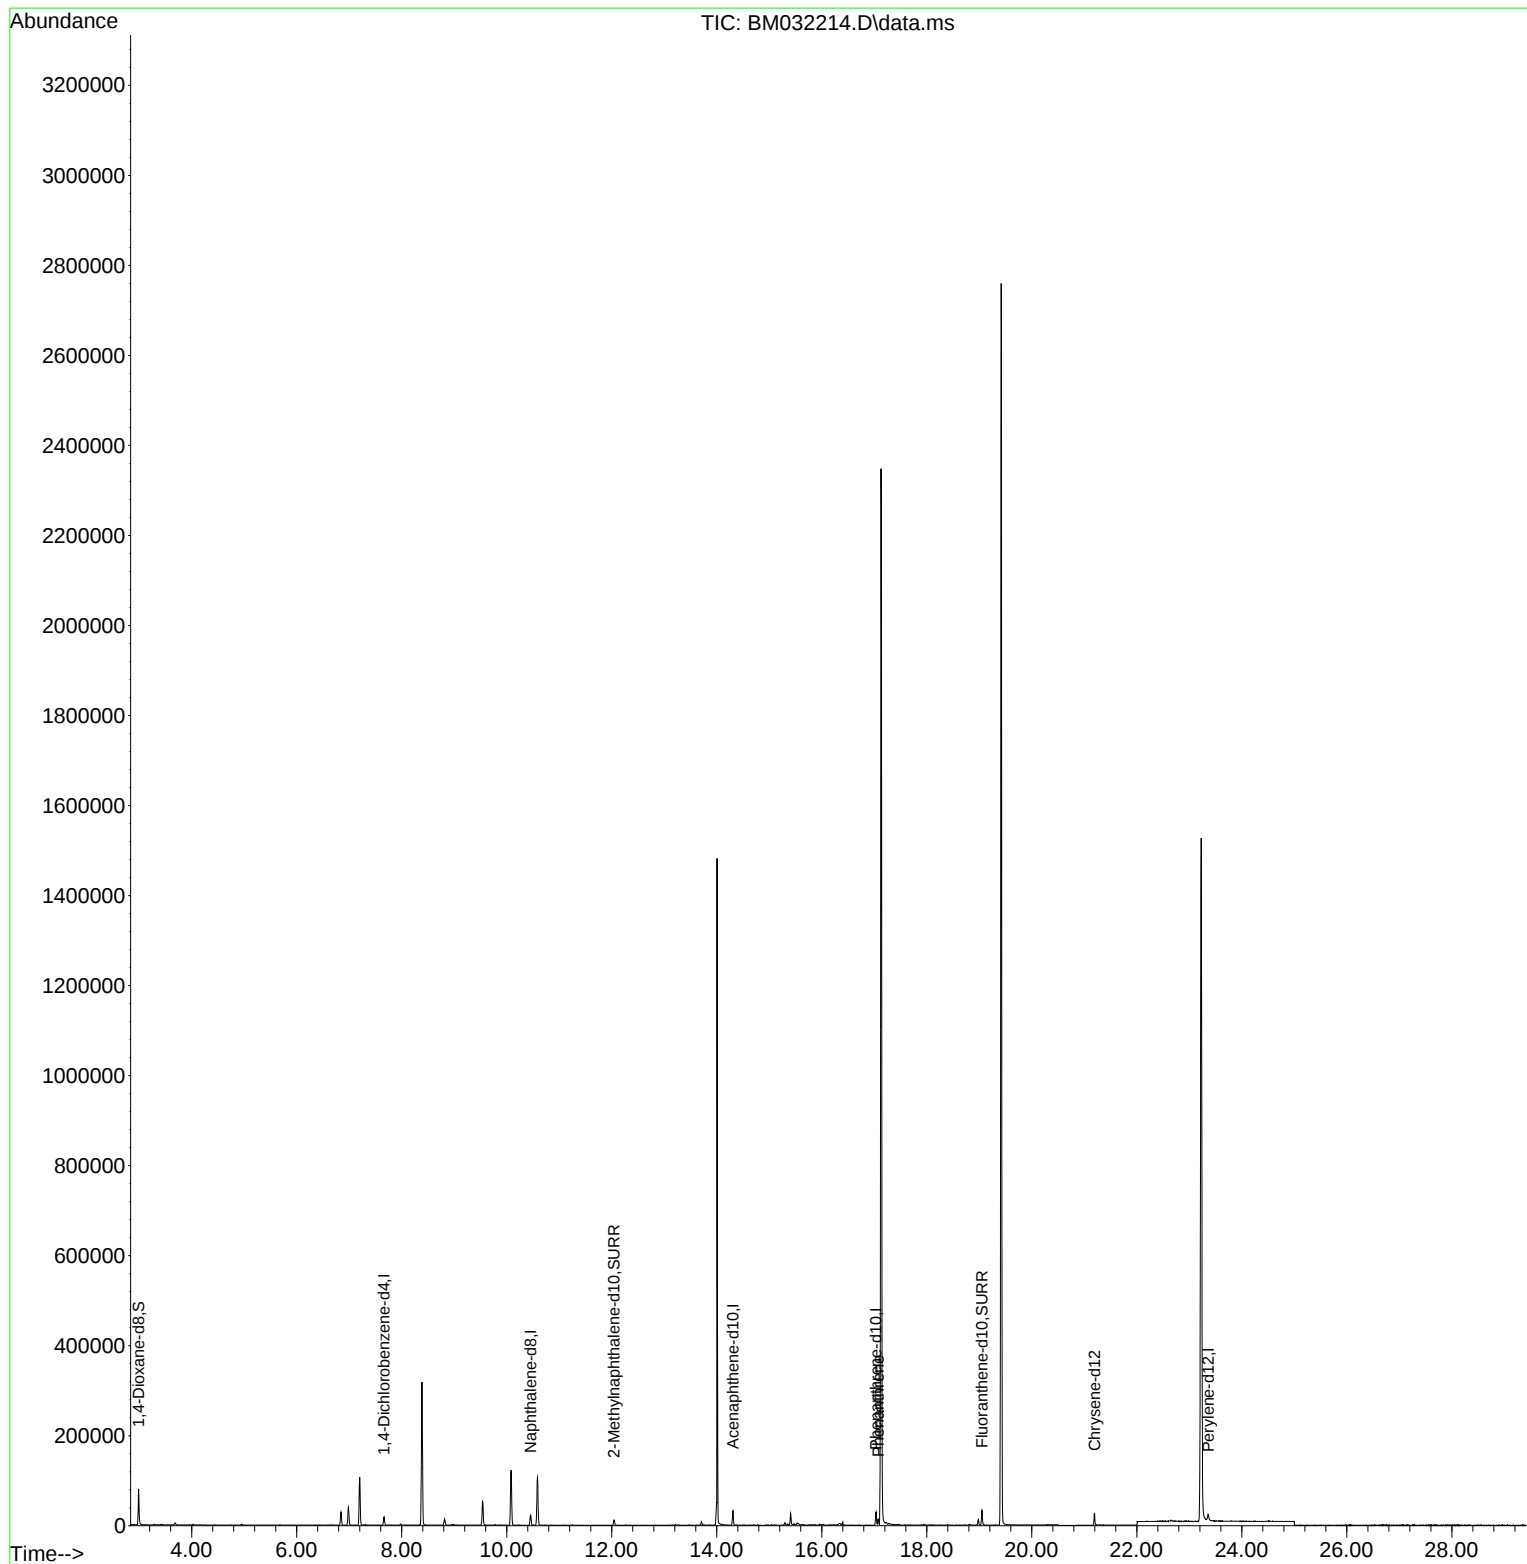

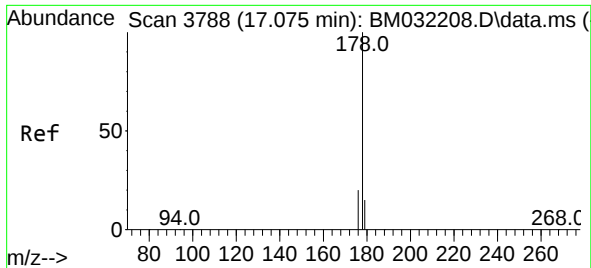

#15
 Phenanthrene
 Concen: 0.136 ng/ul
 RT: 17.074 min Scan# 3788
 Delta R.T. -0.000 min
 Lab File: BM032214.D
 Acq: 27 Sep 2021 20:42

Instrument :
 BNA_M
 ClientSampleId :
 GB6Z8

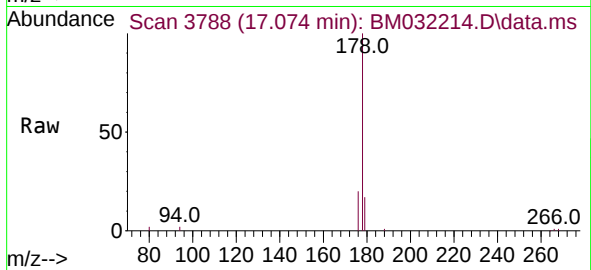

Tgt Ion:	178	Resp:	13753
Ion	Ratio	Lower	Upper
178	100		
179	17.5	12.6	18.8
176	20.0	15.8	23.6

