

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092721\
 Data File : BM032215.D
 Acq On : 27 Sep 2021 21:19
 Operator : CG/JU
 Sample : M3919-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB6Z5

Quant Time: Sep 28 02:30:07 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 27 13:37:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.664	152	7342	0.400	ng/ul	0.00
4) Naphthalene-d8	10.456	136	23115	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.308	164	12169	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.033	188	22366	0.400	ng/ul	0.00
17) Chrysene-d12	21.193	240	16729	0.400	ng/ul	0.00
23) Perylene-d12	23.356	264	16517	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.989	96	50172	6.357	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.044	152	12280	0.399	ng/ul	0.00
18) Fluoranthene-d10	19.050	212	24041	0.529	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.024	88	185124	22.797	ng/ul	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092721\
Data File : BM032215.D
Acq On : 27 Sep 2021 21:19
Operator : CG/JU
Sample : M3919-16
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB6Z5


Quant Time: Sep 28 02:30:07 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 27 13:37:22 2021
Response via : Initial Calibration

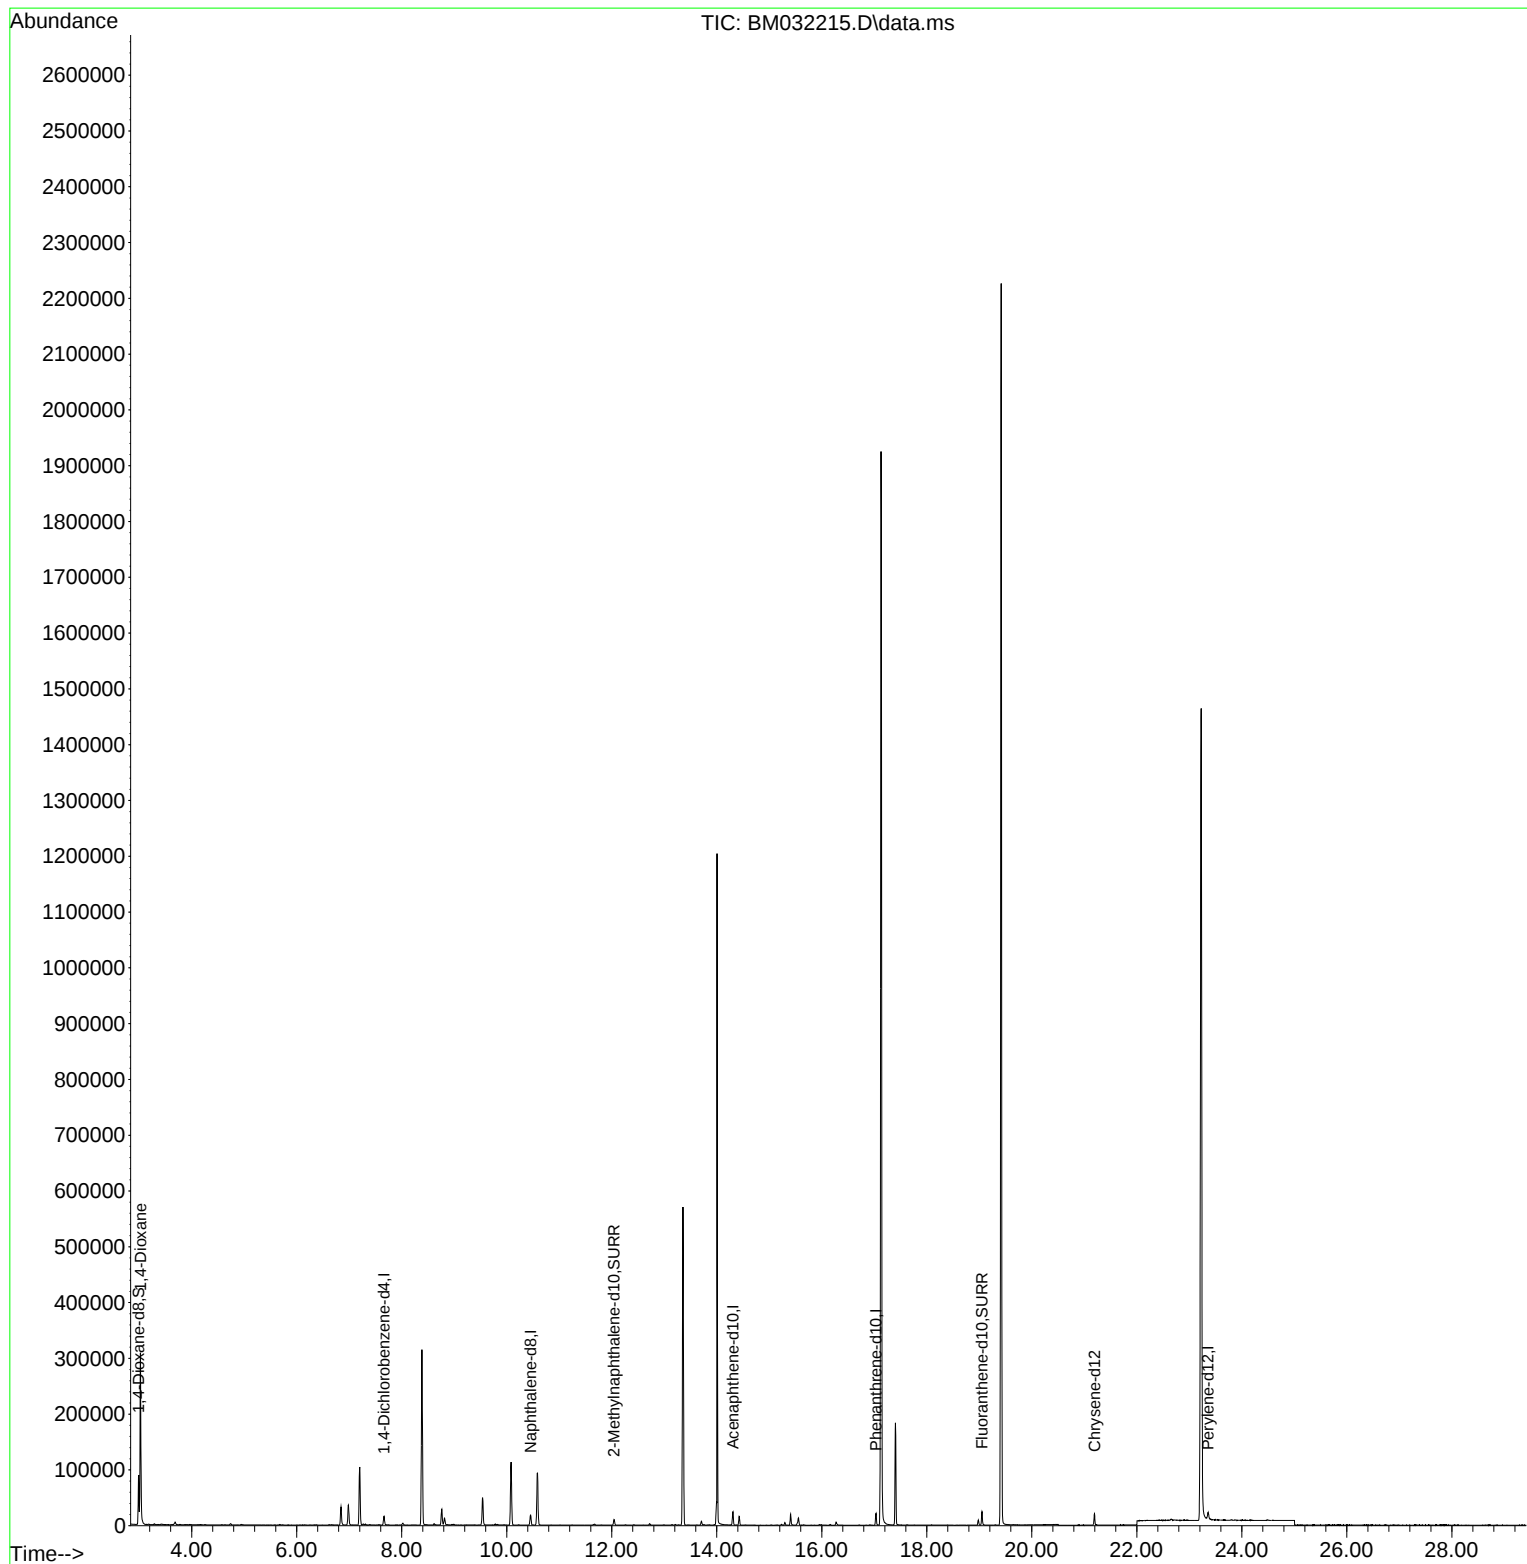

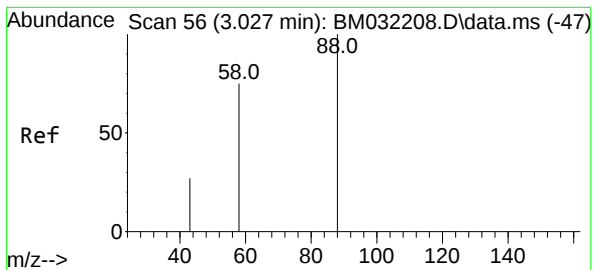

#2
 1,4-Dioxane
 Concen: 22.797 ng/ul
 RT: 3.024 min Scan# 55
 Delta R.T. -0.003 min
 Lab File: BM032215.D
 Acq: 27 Sep 2021 21:19

Instrument :
 BNA_M
 ClientSampleId :
 GB6Z5

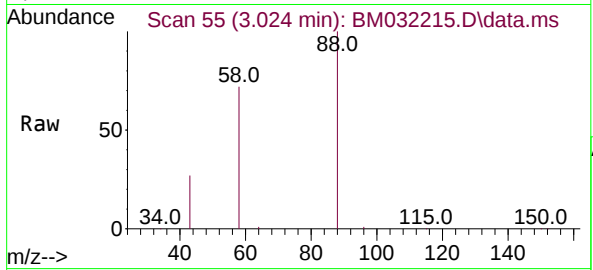

Tgt Ion:	88	Resp:	185124
Ion	Ratio	Lower	Upper
88	100		
43	26.8	26.1	39.1
58	72.4	50.2	75.2

