

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092721\
 Data File : BM032224.D
 Acq On : 28 Sep 2021 02:46
 Operator : CG/JU
 Sample : M3919-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB6Y5

Quant Time: Sep 28 03:55:59 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 27 13:37:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.660	152	8188	0.400	ng/ul	0.00
4) Naphthalene-d8	10.452	136	24838	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.304	164	12203	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.029	188	22047	0.400	ng/ul	0.00
17) Chrysene-d12	21.191	240	16705	0.400	ng/ul	0.00
23) Perylene-d12	23.356	264	16629	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.989	96	46353	5.266	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.044	152	10533	0.319	ng/ul	0.00
18) Fluoranthene-d10	19.050	212	20000	0.441	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.027	88	5593	0.618	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092721\
Data File : BM032224.D
Acq On : 28 Sep 2021 02:46
Operator : CG/JU
Sample : M3919-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB6Y5


Quant Time: Sep 28 03:55:59 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 27 13:37:22 2021
Response via : Initial Calibration

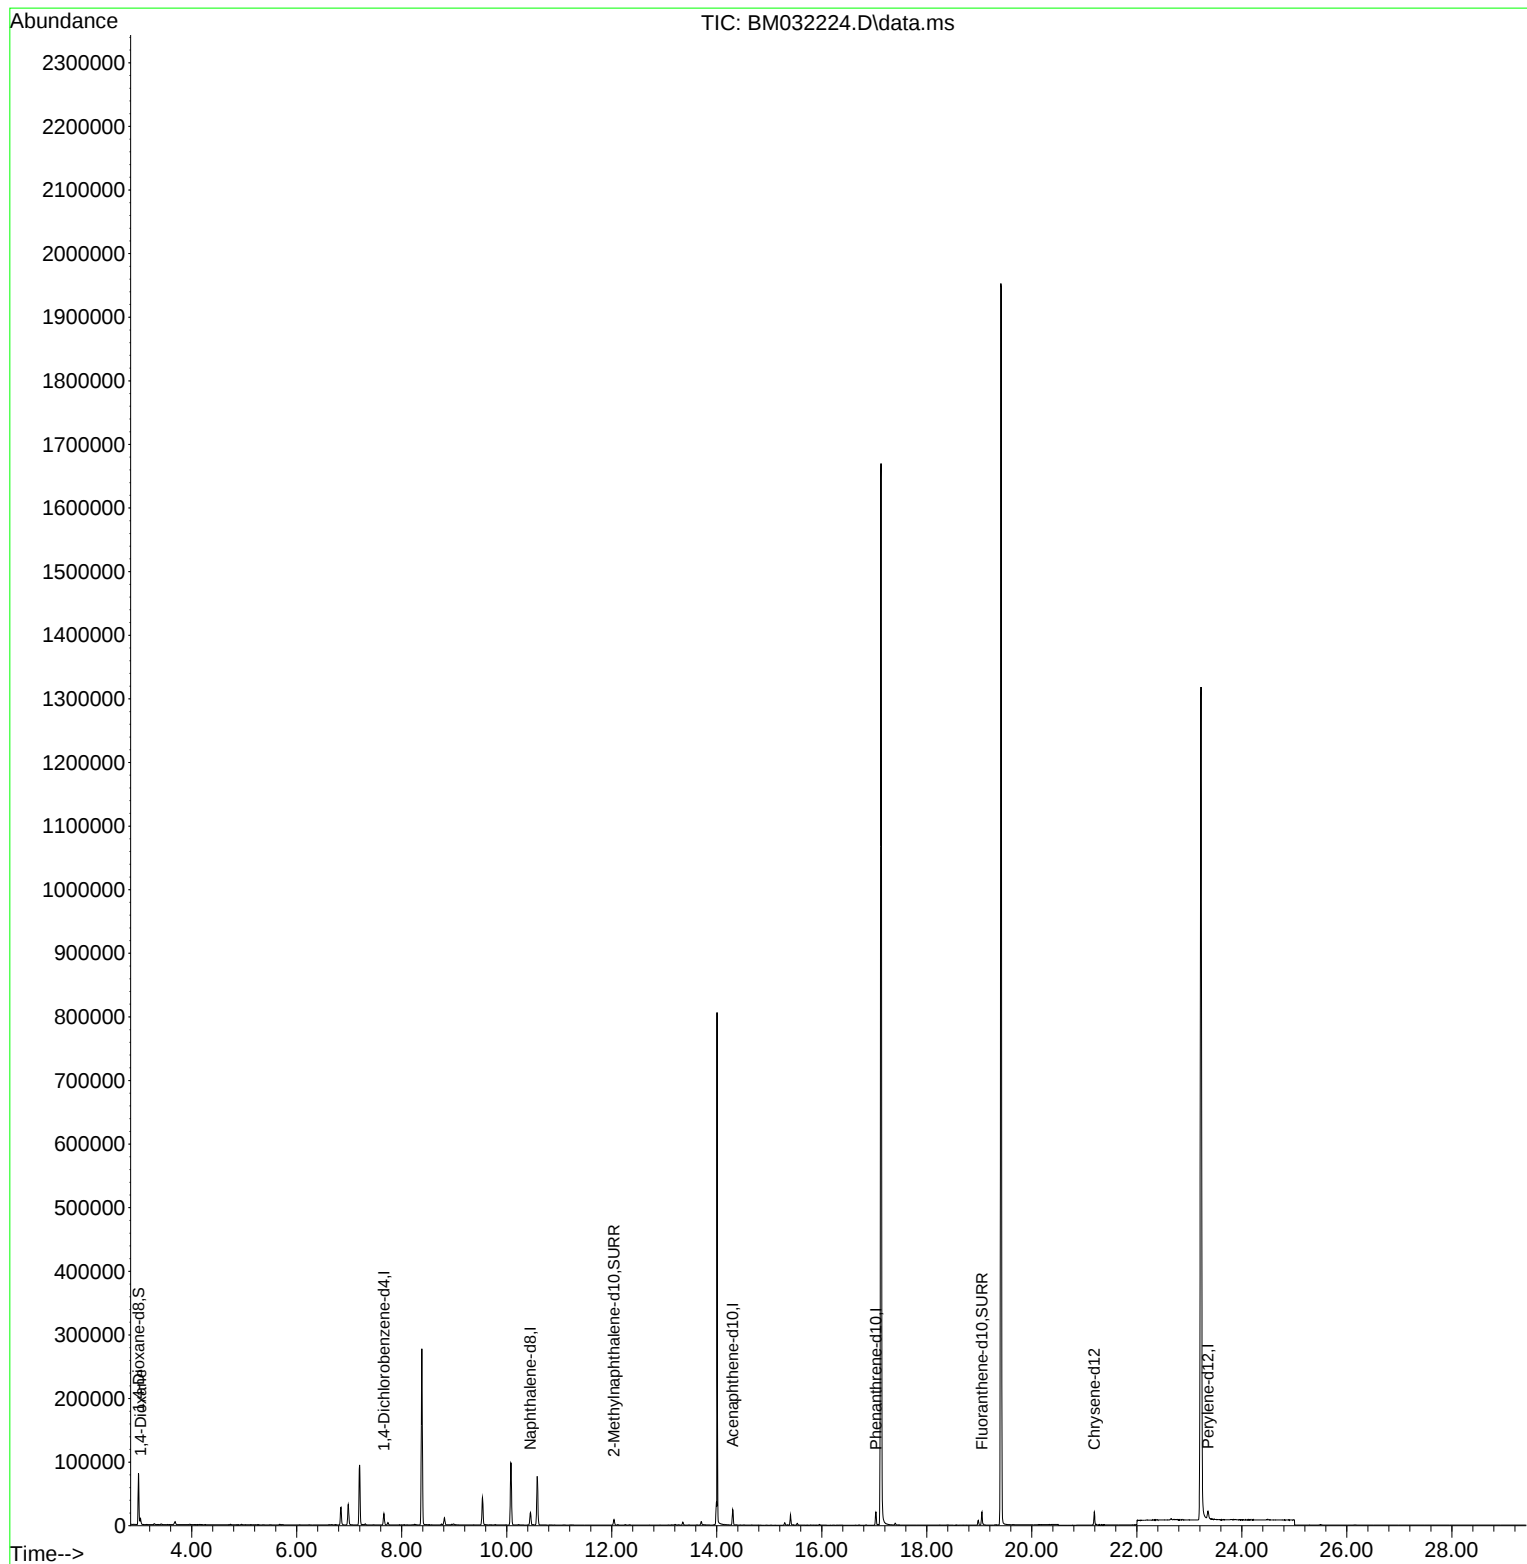

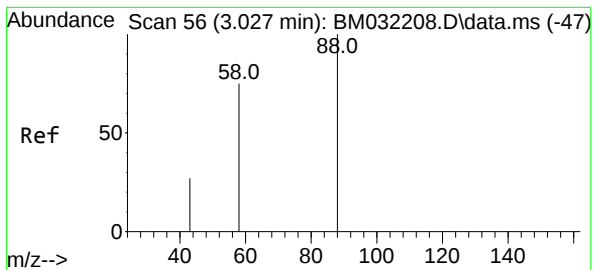

#2
 1,4-Dioxane
 Concen: 0.618 ng/ul
 RT: 3.027 min Scan# 56
 Delta R.T. 0.000 min
 Lab File: BM032224.D
 Acq: 28 Sep 2021 02:46

Instrument :
 BNA_M
 ClientSampleId :
 GB6Y5

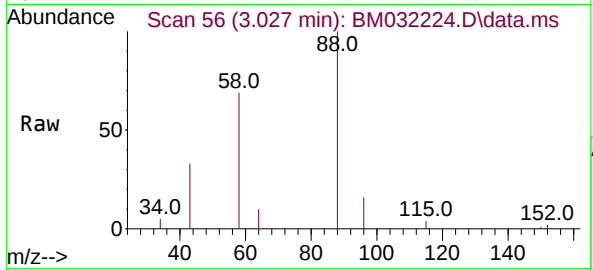

Tgt Ion:	88	Resp:	5593
Ion	Ratio	Lower	Upper
88	100		
43	32.9	26.1	39.1
58	69.1	50.2	75.2

