

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092721\
 Data File : BM032230.D
 Acq On : 28 Sep 2021 06:58
 Operator : CG/JU
 Sample : M3919-15
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB6Z4

Quant Time: Sep 28 08:17:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 27 13:37:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.660	152	7123	0.400	ng/ul	0.00
4) Naphthalene-d8	10.451	136	21486	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.304	164	10838	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.029	188	20058	0.400	ng/ul	0.00
17) Chrysene-d12	21.188	240	14964	0.400	ng/ul	0.00
23) Perylene-d12	23.353	264	14667	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.986	96	49774	6.500	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.039	152	10898	0.381	ng/ul	0.00
18) Fluoranthene-d10	19.050	212	20354	0.501	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.020	88	200771	25.484	ng/ul	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092721\
Data File : BM032230.D
Acq On : 28 Sep 2021 06:58
Operator : CG/JU
Sample : M3919-15
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB6Z4


Quant Time: Sep 28 08:17:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 27 13:37:22 2021
Response via : Initial Calibration

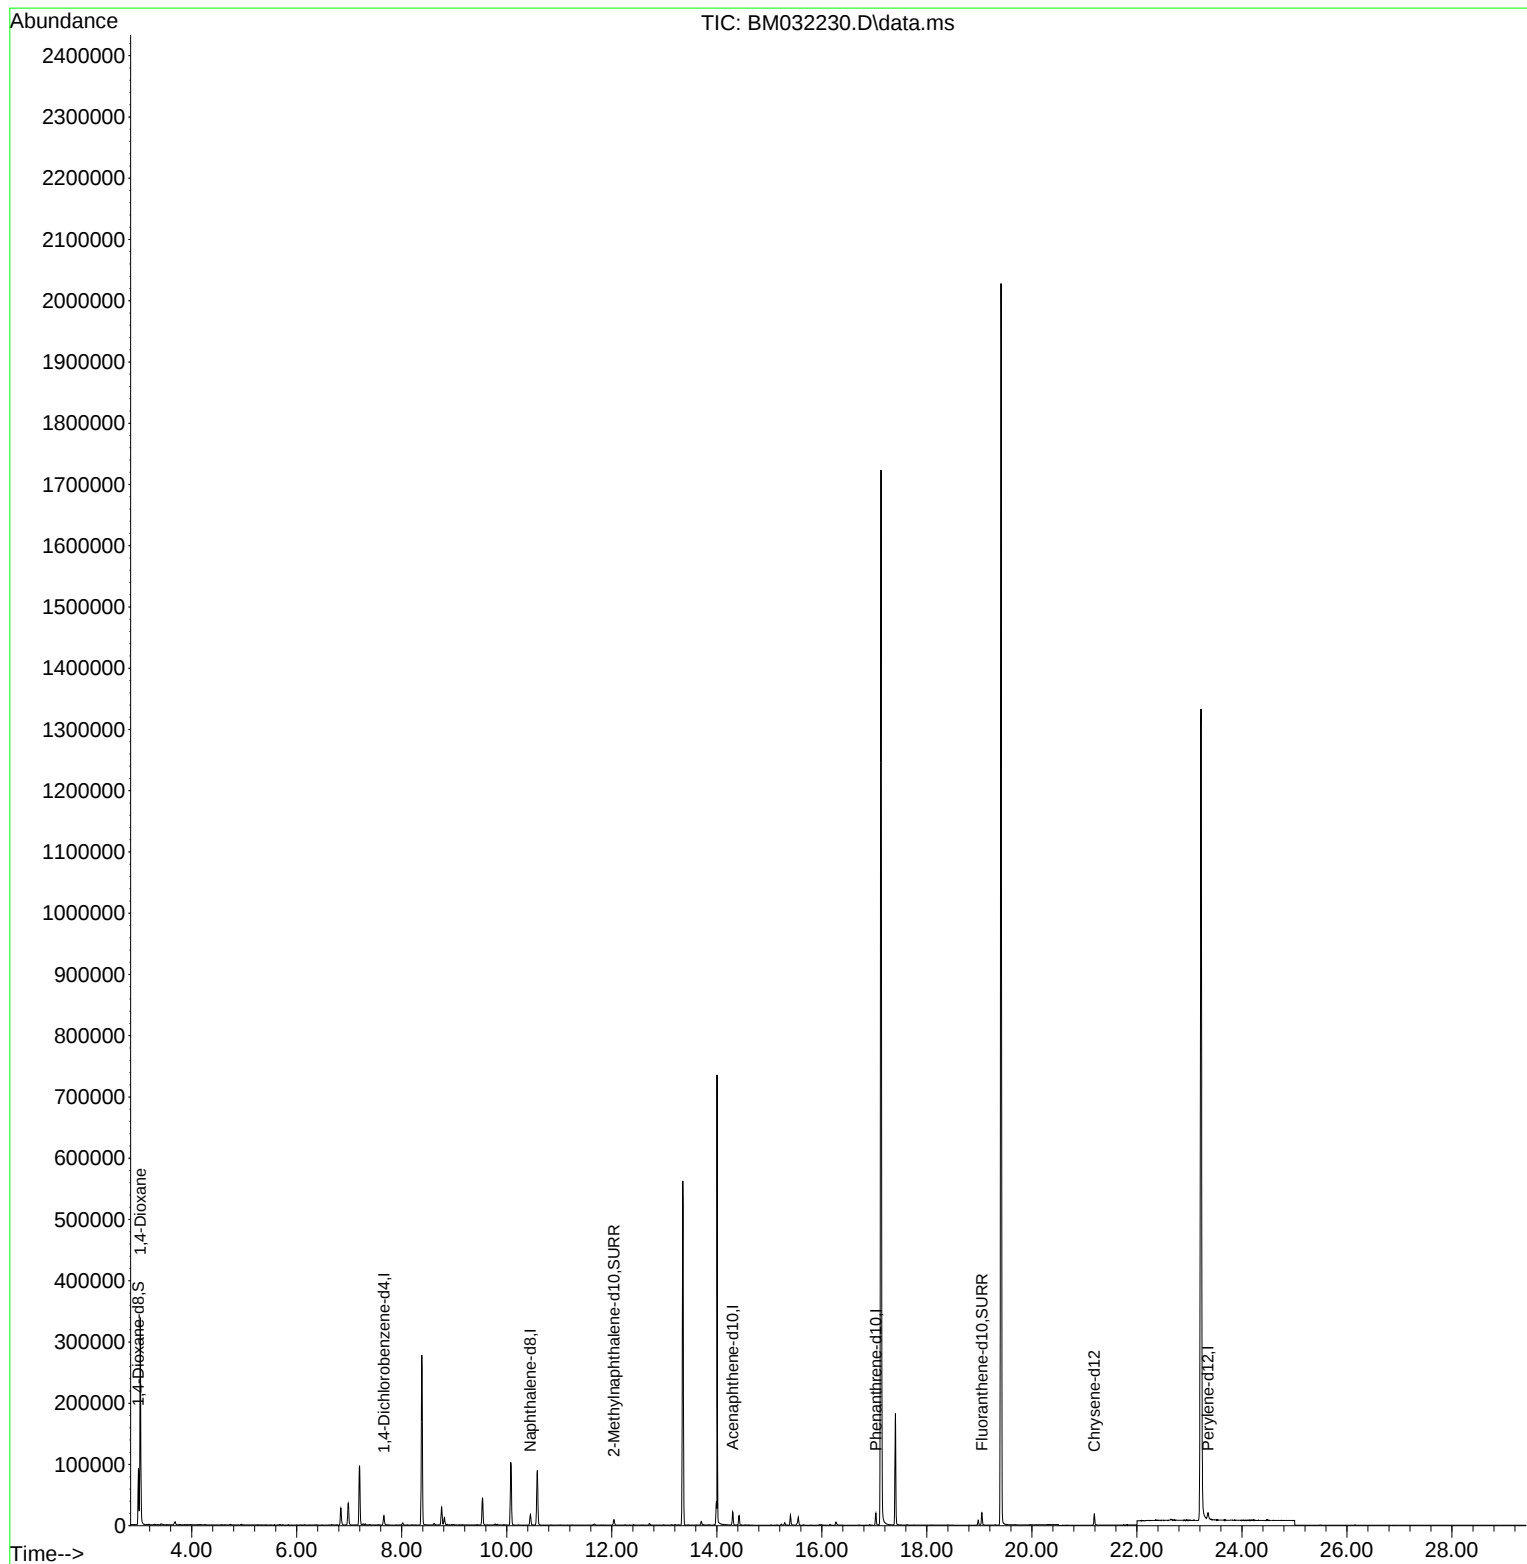

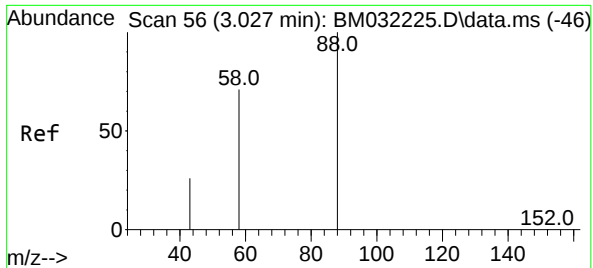

#2
 1,4-Dioxane
 Concen: 25.484 ng/ul
 RT: 3.020 min Scan# 54
 Delta R.T. -0.007 min
 Lab File: BM032230.D
 Acq: 28 Sep 2021 06:58

Instrument :
 BNA_M
 ClientSampleId :
 GB6Z4

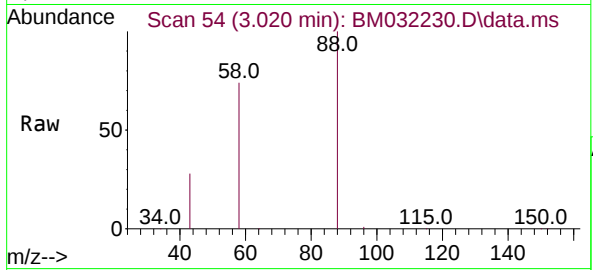

Tgt Ion: 88 Resp: 200771

Ion	Ratio	Lower	Upper
88	100		
43	27.6	26.1	39.1
58	74.0	50.2	75.2

