

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092721\
 Data File : BM032232.D
 Acq On : 28 Sep 2021 08:09
 Operator : CG/JU
 Sample : M3919-13
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB6Z2

Quant Time: Sep 28 08:43:06 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 27 13:37:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.660	152	8074	0.400	ng/ul	0.00
4) Naphthalene-d8	10.452	136	24589	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.304	164	12591	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.029	188	23239	0.400	ng/ul	0.00
17) Chrysene-d12	21.191	240	17637	0.400	ng/ul	0.00
23) Perylene-d12	23.356	264	16916	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.986	96	49445	5.696	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.039	152	11335	0.346	ng/ul	0.00
18) Fluoranthene-d10	19.046	212	22611	0.472	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.024	88	156845	17.564	ng/ul	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092721\
Data File : BM032232.D
Acq On : 28 Sep 2021 08:09
Operator : CG/JU
Sample : M3919-13
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB6Z2

Quant Time: Sep 28 08:43:06 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 27 13:37:22 2021
Response via : Initial Calibration

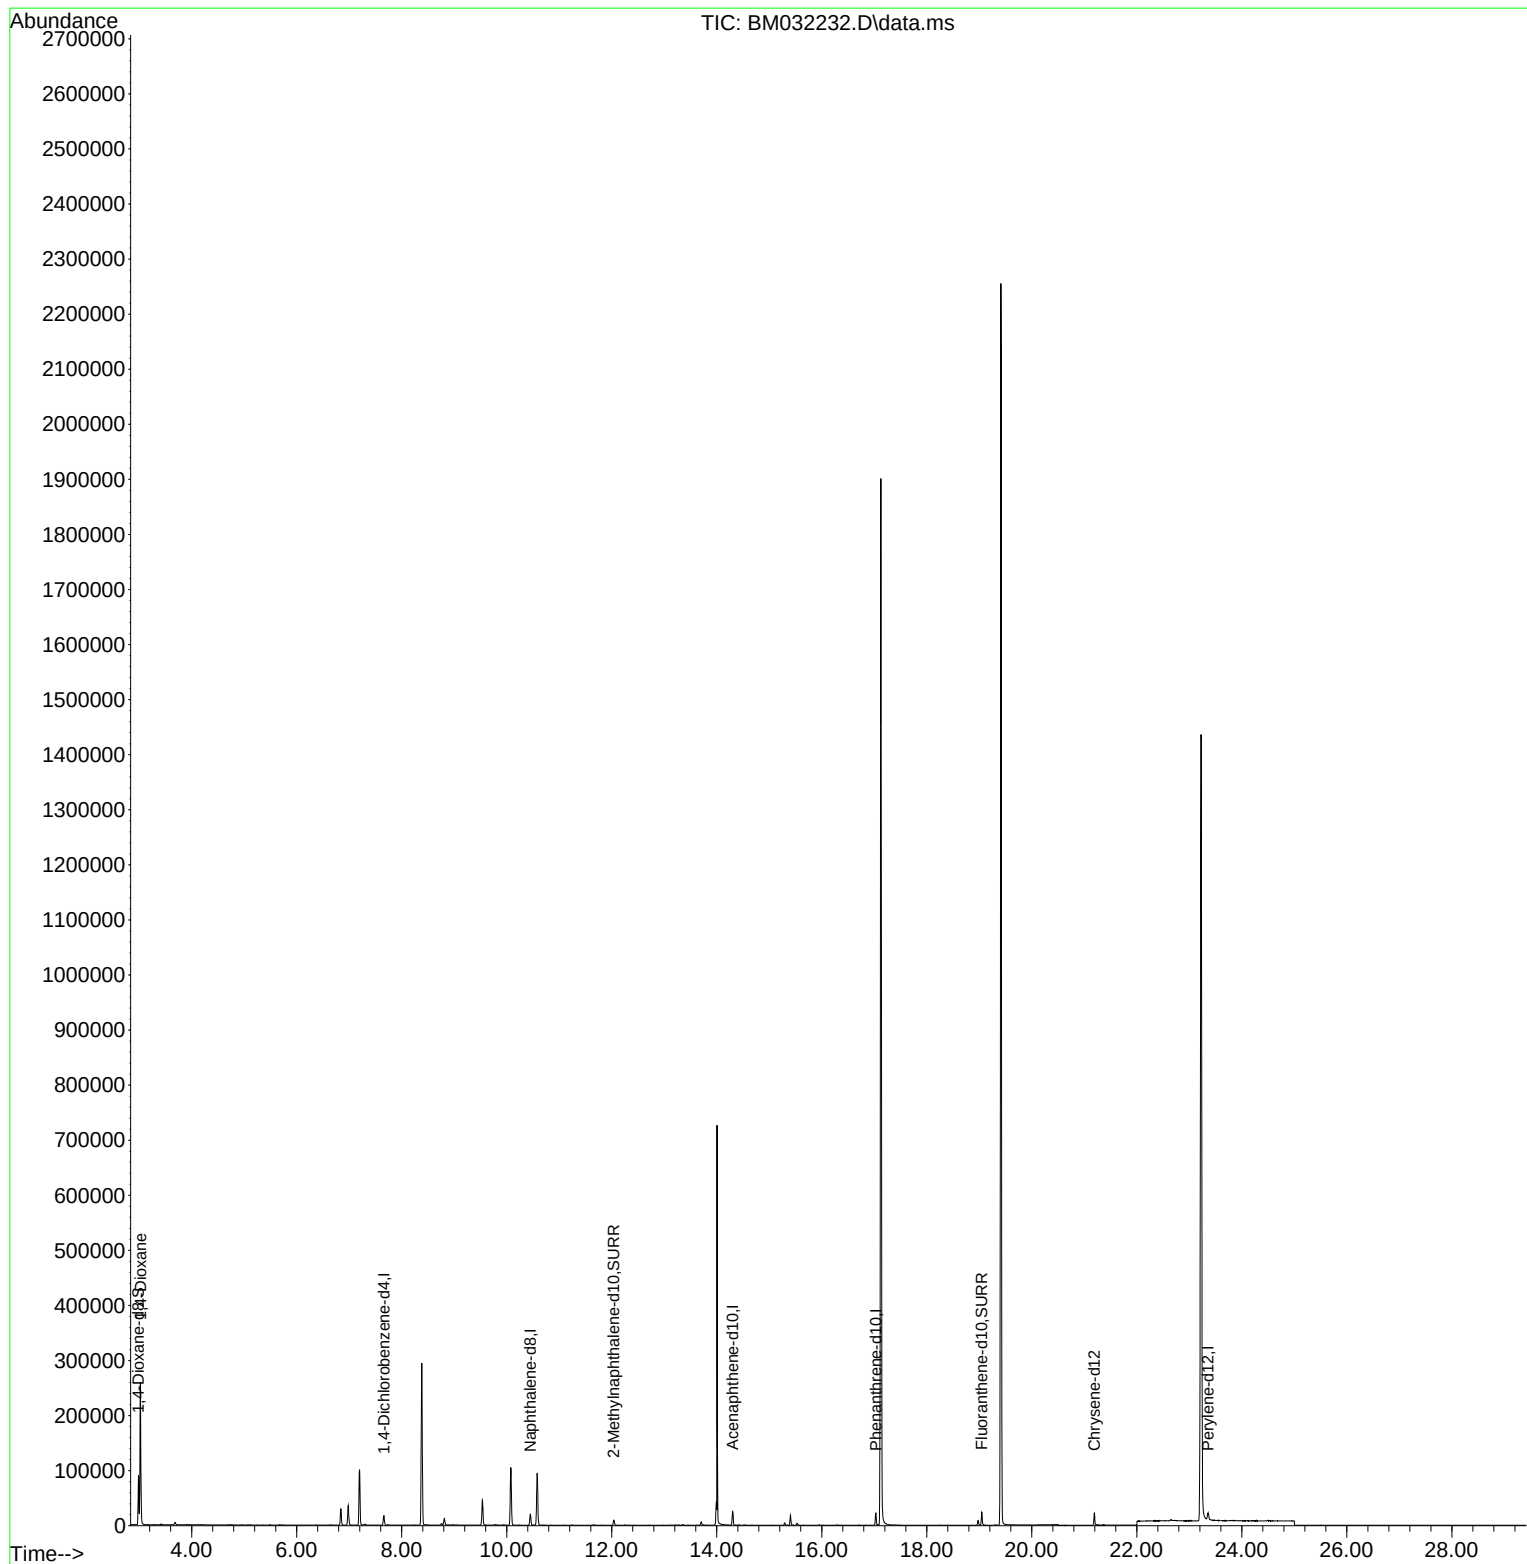

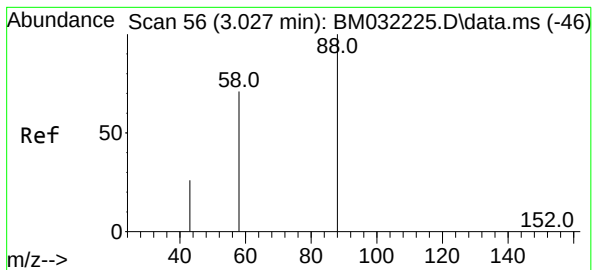

#2
 1,4-Dioxane
 Concen: 17.564 ng/ul
 RT: 3.024 min Scan# 55
 Delta R.T. -0.003 min
 Lab File: BM032232.D
 Acq: 28 Sep 2021 08:09

Instrument :
 BNA_M
 ClientSampleId :
 GB6Z2

Tgt Ion: 88 Resp: 156845

Ion	Ratio	Lower	Upper
88	100		
43	26.4	26.1	39.1
58	71.8	50.2	75.2

