

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092721\
 Data File : BM032236.D
 Acq On : 28 Sep 2021 11:24
 Operator : CG/JU
 Sample : M3919-19
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB6Z8

Quant Time: Sep 28 11:59:00 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 27 13:37:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.660	152	7098	0.400	ng/ul	0.00
4) Naphthalene-d8	10.447	136	21683	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.304	164	10621	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.029	188	19966	0.400	ng/ul	0.00
17) Chrysene-d12	21.191	240	14906	0.400	ng/ul	0.00
23) Perylene-d12	23.356	264	14365	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.986	96	32399	4.246	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.039	152	8003	0.277	ng/ul	0.00
18) Fluoranthene-d10	19.049	212	15677	0.387	ng/ul	0.00
Target Compounds						
15) Phenanthrene	17.071	178	6805	0.105	ng/ul	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092721\
Data File : BM032236.D
Acq On : 28 Sep 2021 11:24
Operator : CG/JU
Sample : M3919-19
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB6Z8


Quant Time: Sep 28 11:59:00 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 27 13:37:22 2021
Response via : Initial Calibration

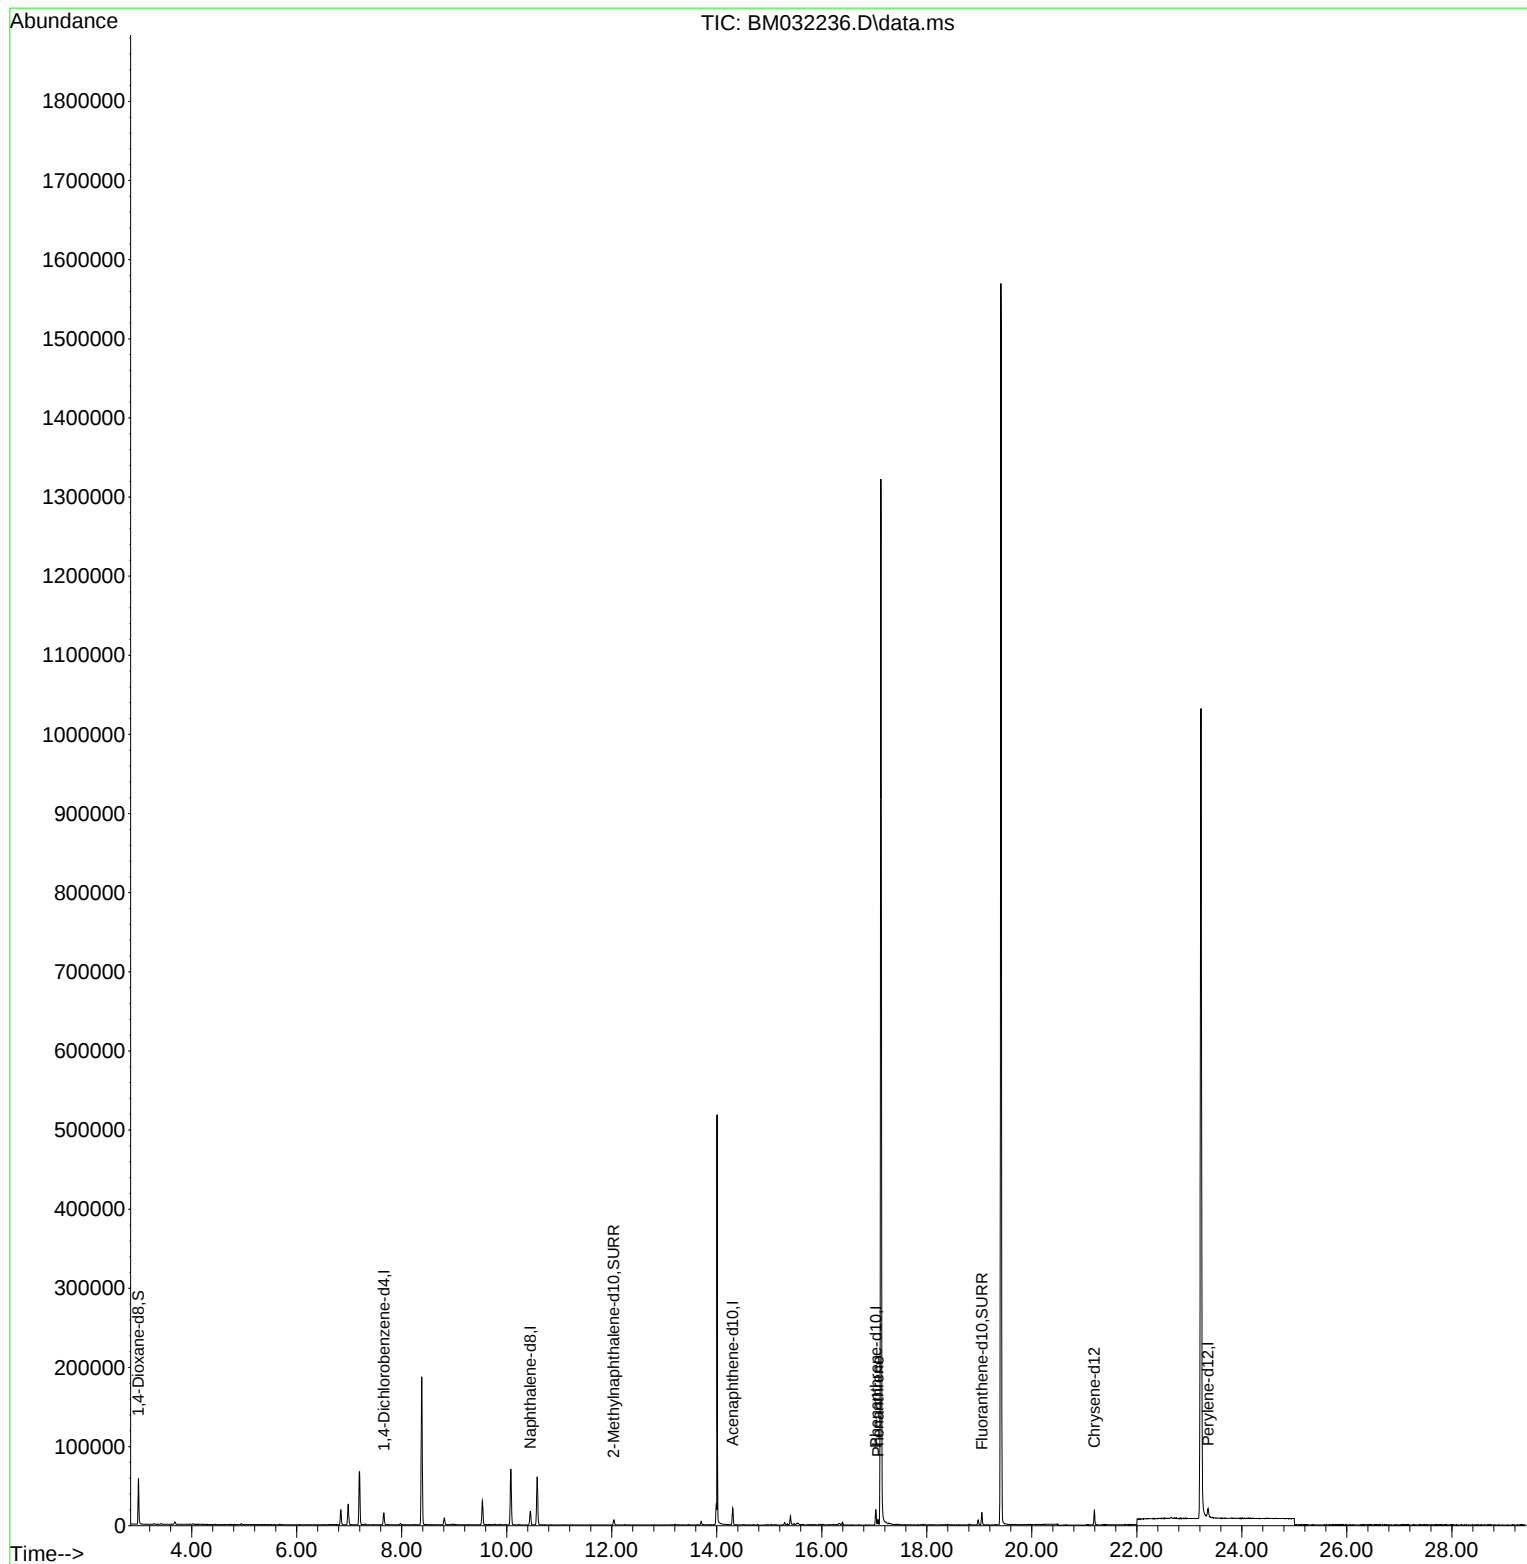

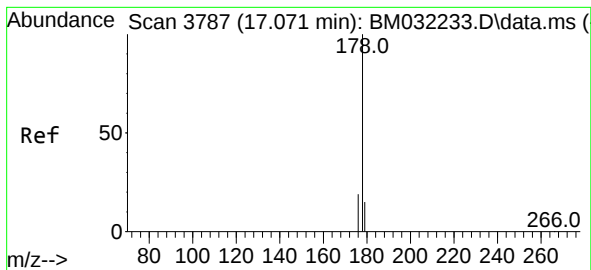

#15
 Phenanthrene
 Concen: 0.105 ng/ul
 RT: 17.071 min Scan# 3787
 Delta R.T. -0.004 min
 Lab File: BM032236.D
 Acq: 28 Sep 2021 11:24

Instrument :
 BNA_M
 ClientSampleId :
 GB6Z8

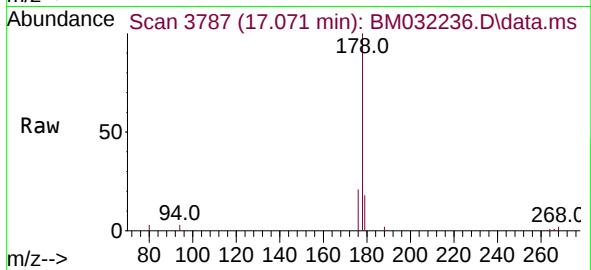

Tgt Ion:	178	Resp:	6805
Ion	Ratio	Lower	Upper
178	100		
179	18.3	12.6	18.8
176	20.7	15.8	23.6

