

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092721\
 Data File : BM032243.D
 Acq On : 28 Sep 2021 16:47
 Operator : CG/JU
 Sample : M3739-08
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK1

Quant Time: Sep 28 17:30:24 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 27 13:37:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.660	152	6618	0.400	ng/ul	0.00
4) Naphthalene-d8	10.451	136	20982	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.303	164	10952	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.028	188	19912	0.400	ng/ul	0.00
17) Chrysene-d12	21.190	240	14947	0.400	ng/ul	0.00
23) Perylene-d12	23.352	264	15988	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.986	96	52286	7.349	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.038	152	10003	0.358	ng/ul	0.00
18) Fluoranthene-d10	19.045	212	20677	0.509	ng/ul	0.00
Target Compounds						
7) 2-Methylnaphthalene	12.115	142	806	0.020	ng/ul	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092721\
Data File : BM032243.D
Acq On : 28 Sep 2021 16:47
Operator : CG/JU
Sample : M3739-08
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK1

Quant Time: Sep 28 17:30:24 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 27 13:37:22 2021
Response via : Initial Calibration

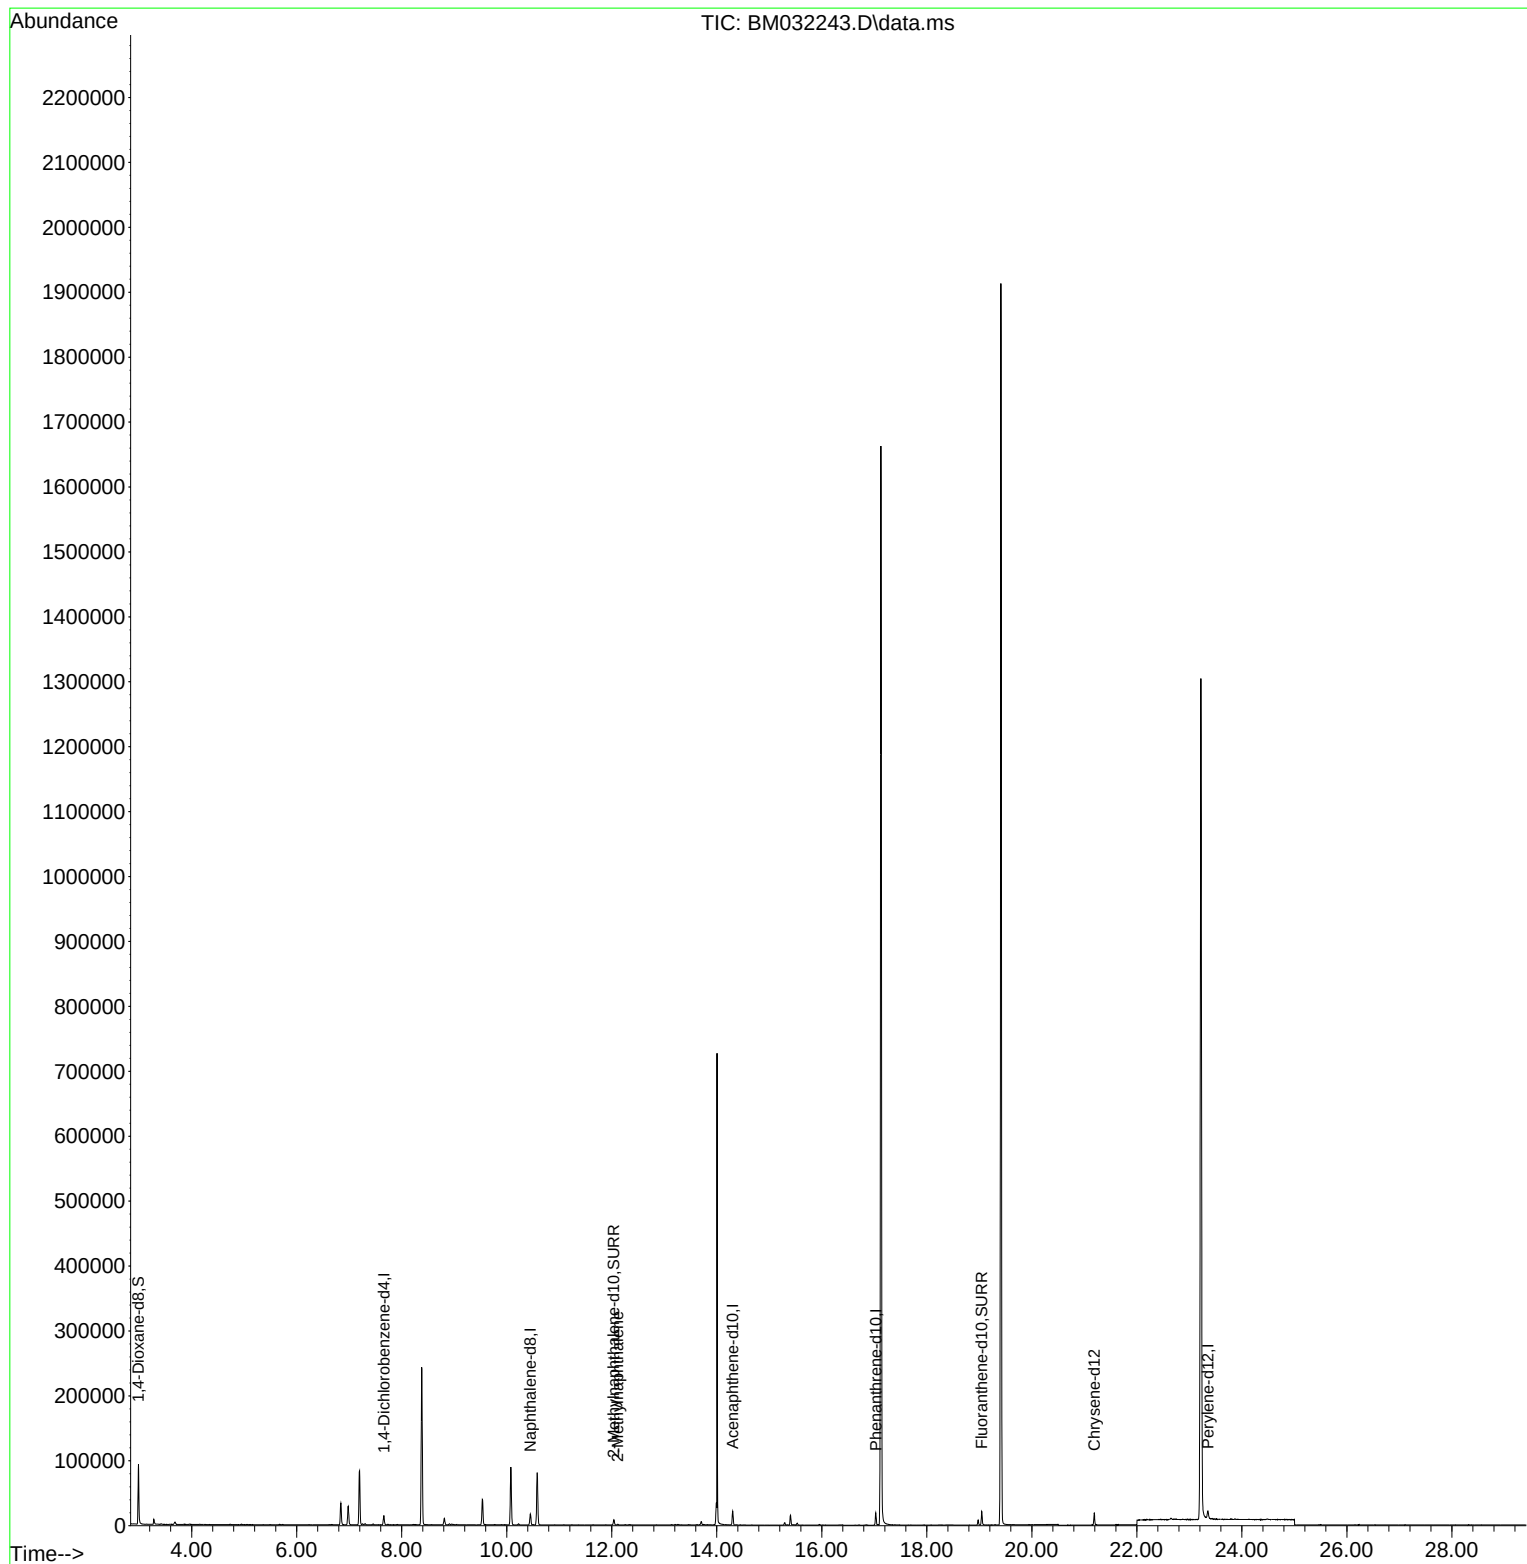

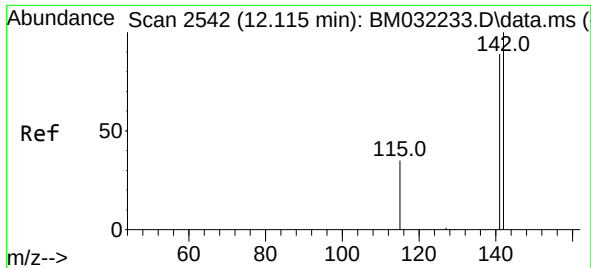

#7
 2-Methylnaphthalene
 Concen: 0.020 ng/ul
 RT: 12.115 min Scan# 2542
 Delta R.T. -0.005 min
 Lab File: BM032243.D
 Acq: 28 Sep 2021 16:47

Instrument :
 BNA_M
 ClientSampleId :
 C0AK1

Tgt Ion:142 Resp: 806
 Ion Ratio Lower Upper
 142 100
 141 89.5 71.2 106.8

