

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092721\
 Data File : BM032280.D
 Acq On : 29 Sep 2021 20:02
 Operator : CG/JU
 Sample : M3777-16
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF4

Quant Time: Sep 30 01:04:50 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 27 13:37:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.653	152	6328	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.443	136	19031	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.300	164	8982	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.023	188	16437	0.400	ng/ul	-0.01
17) Chrysene-d12	21.186	240	13717	0.400	ng/ul	0.00
23) Perylene-d12	23.349	264	14512	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.986	96	29649	4.358	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.035	152	7368	0.291	ng/ul	-0.01
18) Fluoranthene-d10	19.042	212	15582	0.418	ng/ul	-0.01
Target Compounds						
					Qvalue	
20) Pyrene	19.435	202	4009	0.070	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092721\
Data File : BM032280.D
Acq On : 29 Sep 2021 20:02
Operator : CG/JU
Sample : M3777-16
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF4

Quant Time: Sep 30 01:04:50 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM092721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 27 13:37:22 2021
Response via : Initial Calibration

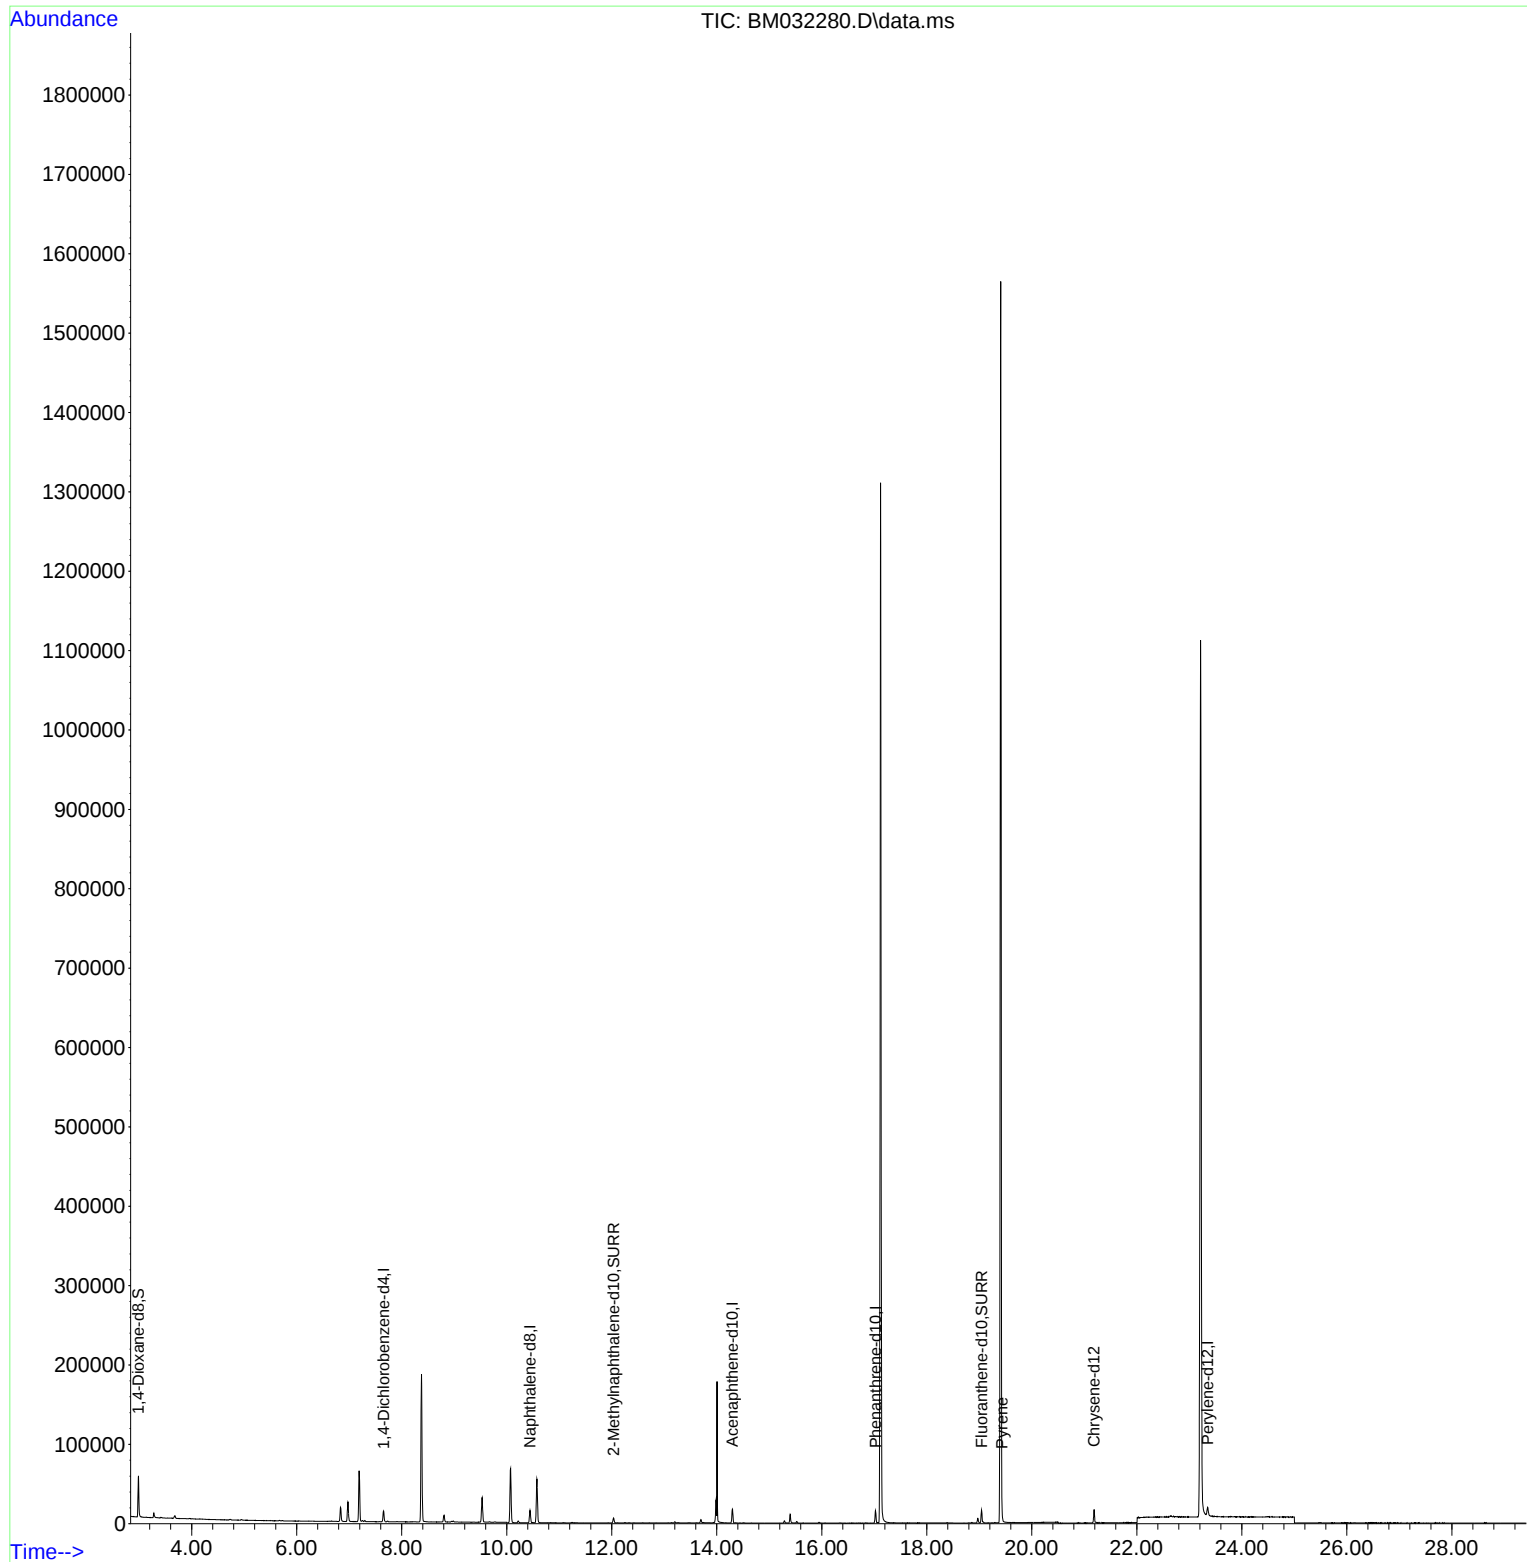

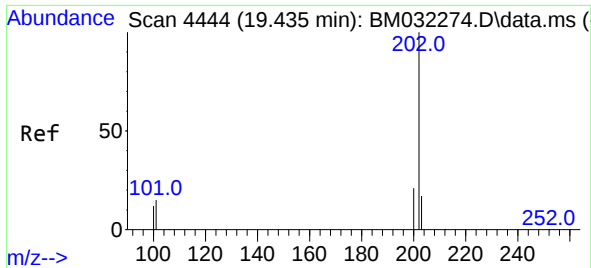

#20
Pyrene
Concen: 0.070 ng/ul
RT: 19.435 min Scan# 4444
Delta R.T. -0.008 min
Lab File: BM032280.D
Acq: 29 Sep 2021 20:02

Instrument :
BNA_M
ClientSampleId :
C0AF4

Tgt Ion:	202	Resp:	4009
Ion	Ratio	Lower	Upper
202	100		
101	17.8	12.1	18.1
100	16.3	9.8	14.6#

