

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092723\
 Data File : BM042082.D
 Acq On : 27 Sep 2023 13:23
 Operator : MA/JU
 Sample : 04385-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EZYP3

Quant Time: Sep 27 15:09:05 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 13:50:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	3972	0.400	ng/ul	0.00
4) Naphthalene-d8	10.757	136	10545	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.587	164	4812	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.341	188	9987	0.400	ng/ul	-0.01
17) Chrysene-d12	21.518	240	4828	0.400	ng/ul	0.00
23) Perylene-d12	23.921	264	5732	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	19416	3.587	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.341	152	3846	0.291	ng/ul	-0.01
18) Fluoranthene-d10	19.362	212	6794	0.342	ng/ul	-0.01
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.402	88	950	0.167	ng/ul#	75
5) Naphthalene	10.807	128	1161	0.033	ng/ul#	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092723\
Data File : BM042082.D
Acq On : 27 Sep 2023 13:23
Operator : MA/JU
Sample : 04385-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EZYP3

Quant Time: Sep 27 15:09:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 13:50:58 2023
Response via : Initial Calibration




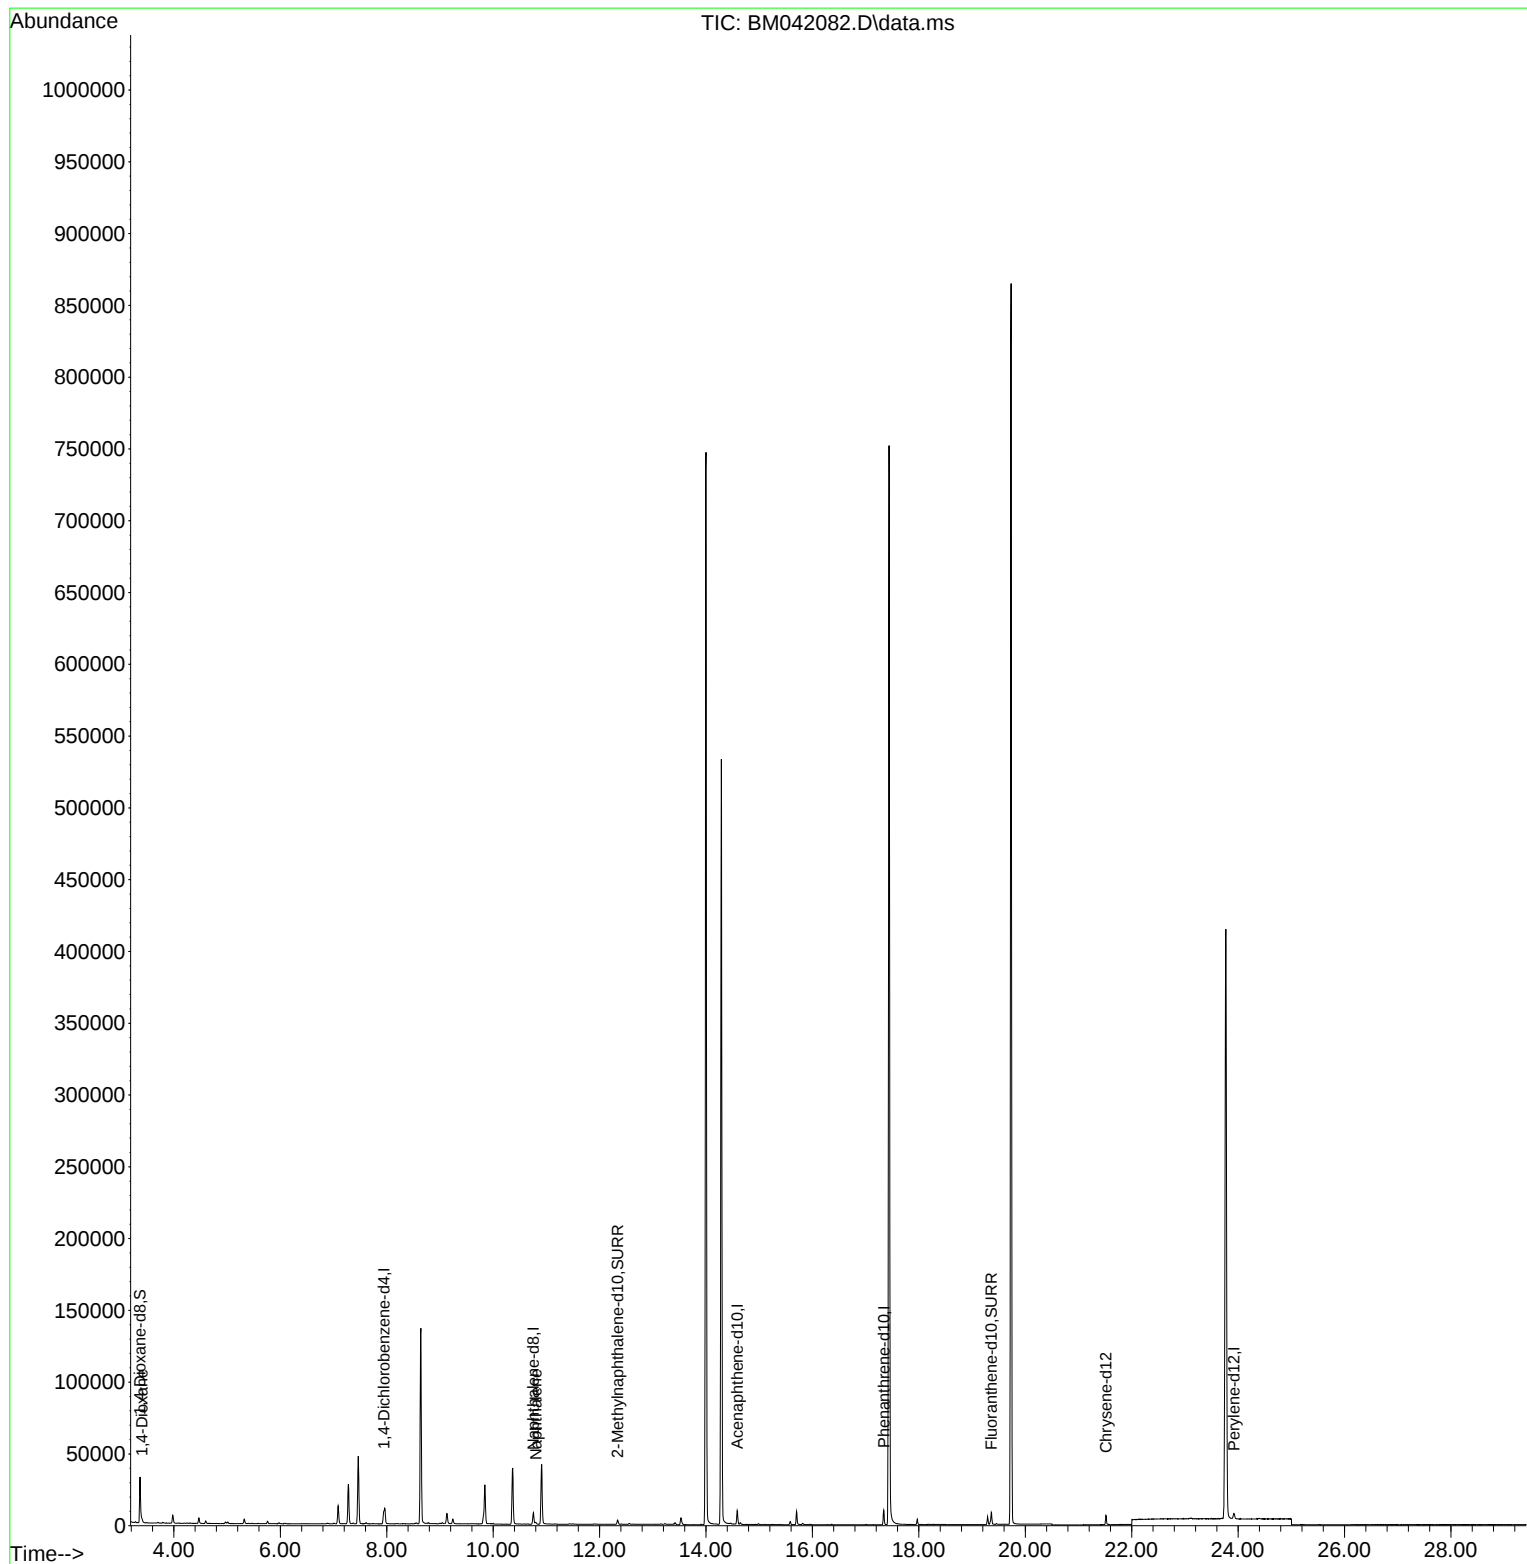


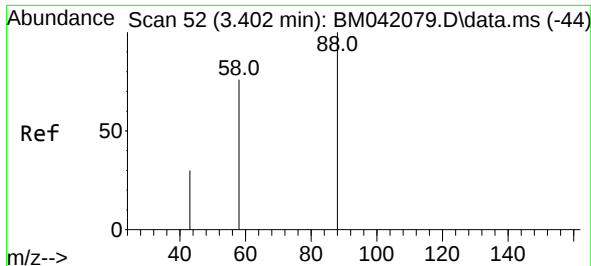

#2
1,4-Dioxane
Concen: 0.167 ng/ul
RT: 3.402 min Scan# 51
Delta R.T. -0.008 min
Lab File: BM042082.D
Acq: 27 Sep 2023 13:23

Instrument :
BNA_M
ClientSampleId :
EZYP3

Tgt Ion: 88 Resp: 950
Ion Ratio Lower Upper
88 100
43 81.2 42.9 64.3#
58 58.9 56.4 84.6

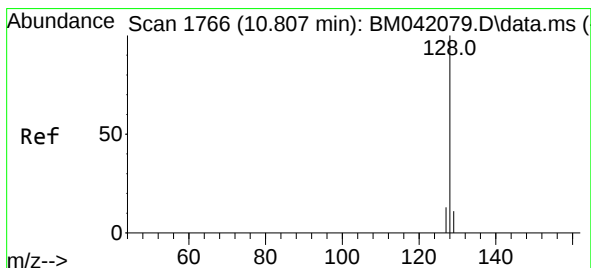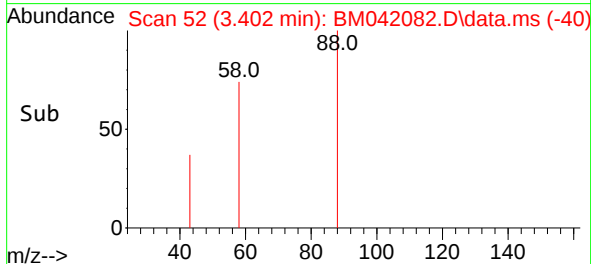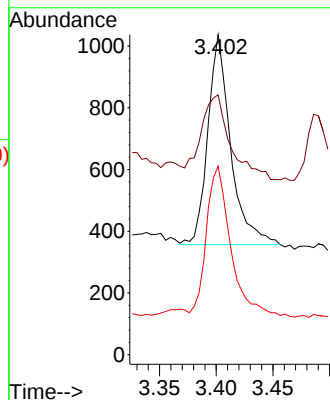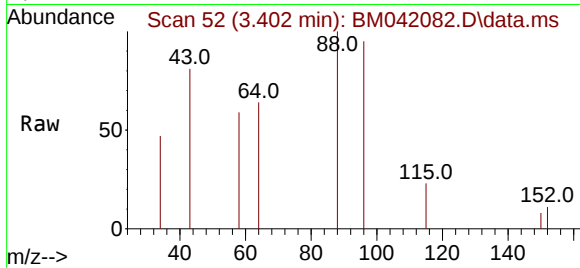

#5
Naphthalene
Concen: 0.033 ng/ul
RT: 10.807 min Scan# 1766
Delta R.T. -0.011 min
Lab File: BM042082.D
Acq: 27 Sep 2023 13:23

Tgt Ion: 128 Resp: 1161
Ion Ratio Lower Upper
128 100
129 20.9 9.2 13.8#
127 20.3 10.8 16.2#

