

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092723\
 Data File : BM042083.D
 Acq On : 27 Sep 2023 13:59
 Operator : MA/JU
 Sample : 04450-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJ65

Quant Time: Sep 27 15:09:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 13:50:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.942	152	4229	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.757	136	11129	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.588	164	5087	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.341	188	10960	0.400	ng/ul	-0.01
17) Chrysene-d12	21.516	240	5526	0.400	ng/ul	0.00
23) Perylene-d12	23.921	264	6571	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	22461	3.898	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.341	152	4276	0.307	ng/ul	-0.01
18) Fluoranthene-d10	19.366	212	8087	0.355	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.402	88	1517	0.250	ng/ul#	88
5) Naphthalene	10.807	128	1037	0.028	ng/ul#	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092723\
Data File : BM042083.D
Acq On : 27 Sep 2023 13:59
Operator : MA/JU
Sample : 04450-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJ65

Quant Time: Sep 27 15:09:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 13:50:58 2023
Response via : Initial Calibration




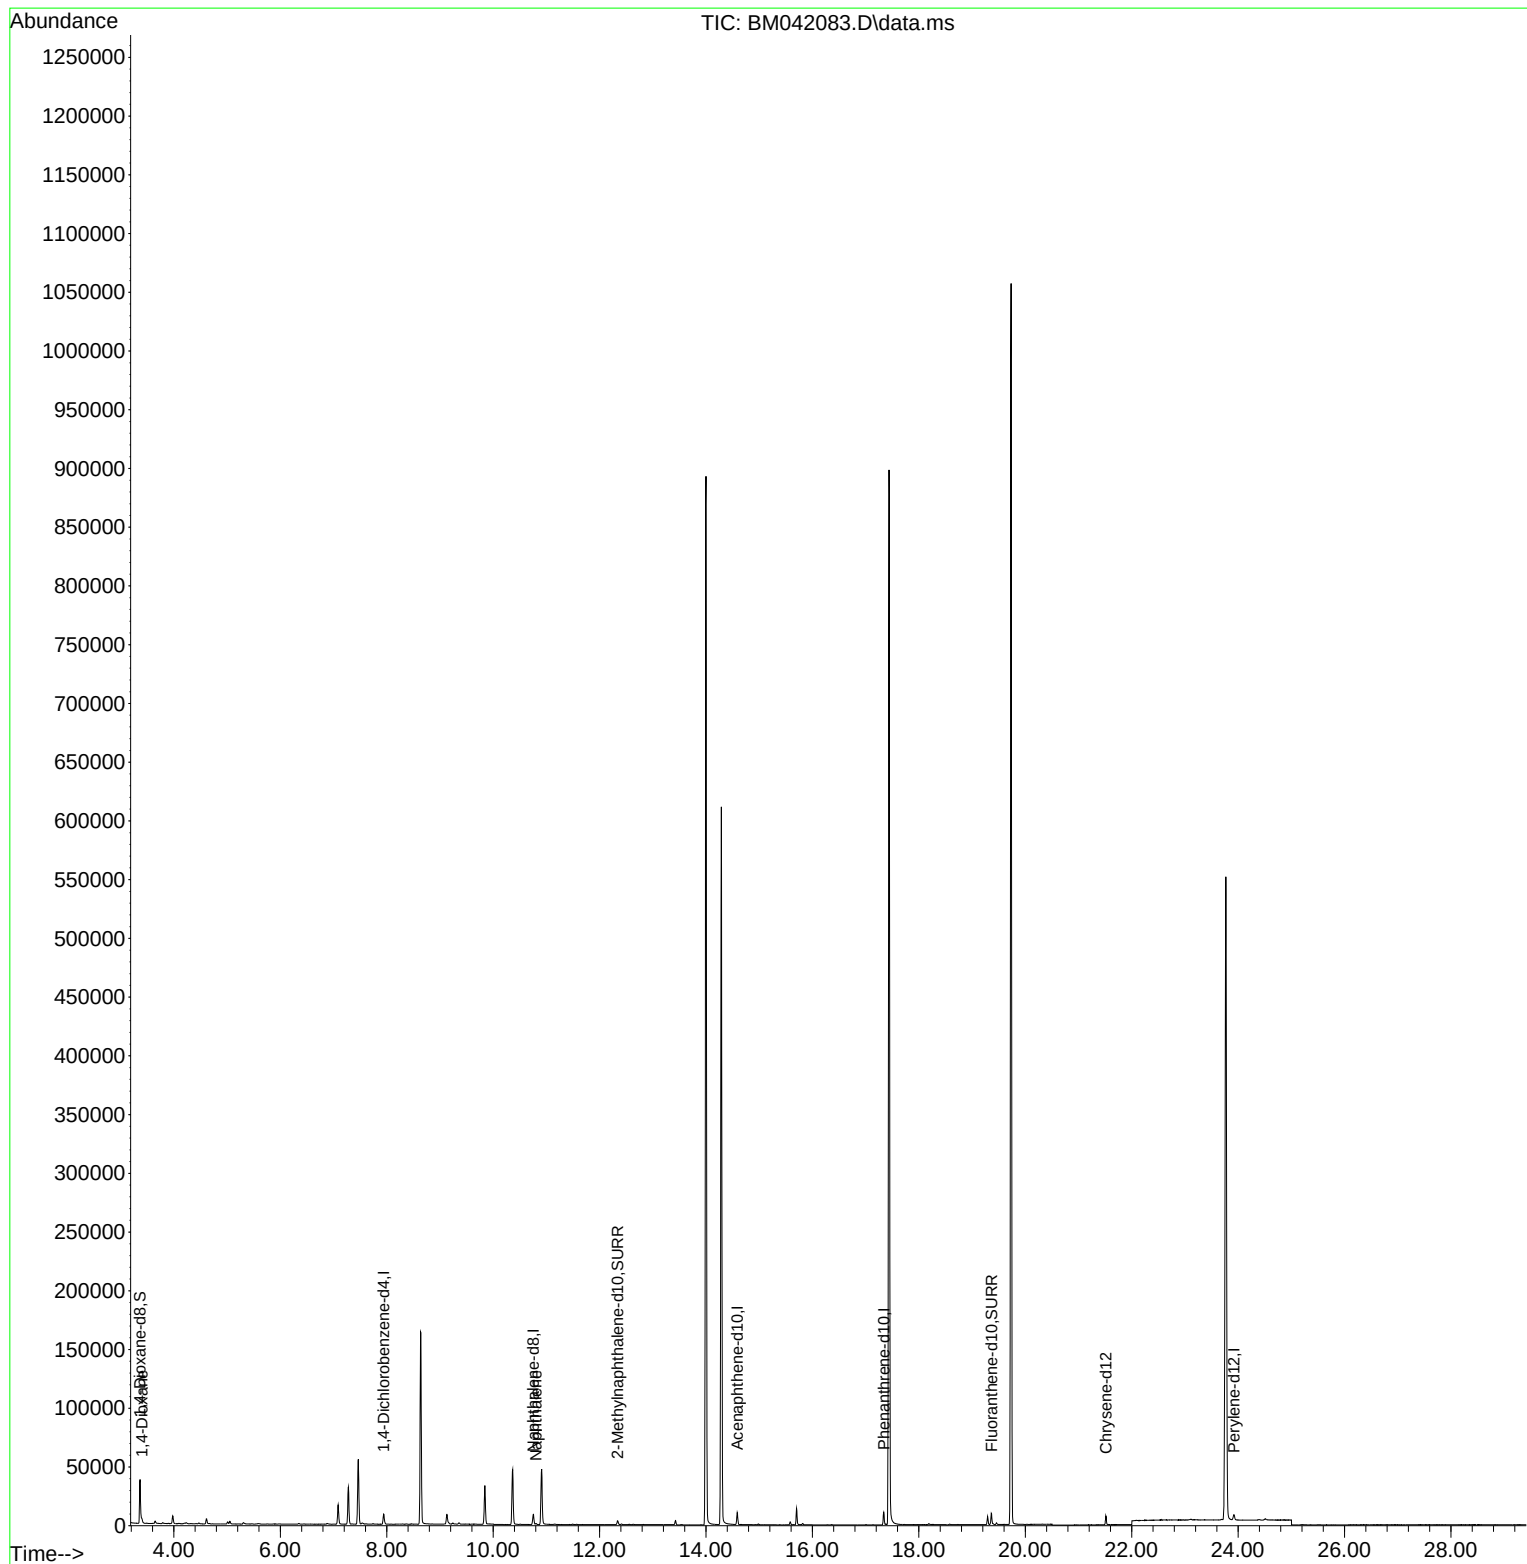


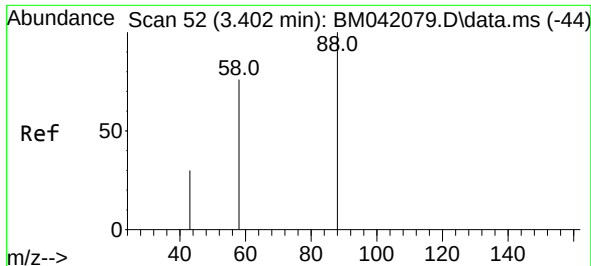

#2
 1,4-Dioxane
 Concen: 0.250 ng/ul
 RT: 3.402 min Scan# 51
 Delta R.T. -0.008 min
 Lab File: BM042083.D
 Acq: 27 Sep 2023 13:59

Instrument :
 BNA_M
 ClientSampleId :
 BBJ65

Tgt Ion: 88 Resp: 1517
 Ion Ratio Lower Upper
 88 100
 43 67.0 42.9 64.3#
 58 65.2 56.4 84.6

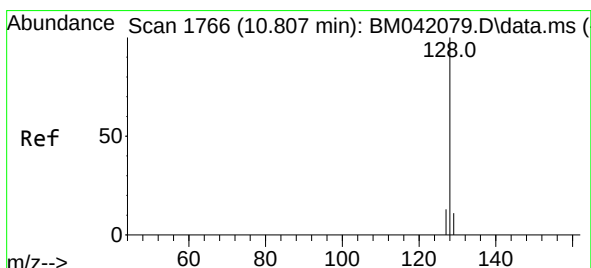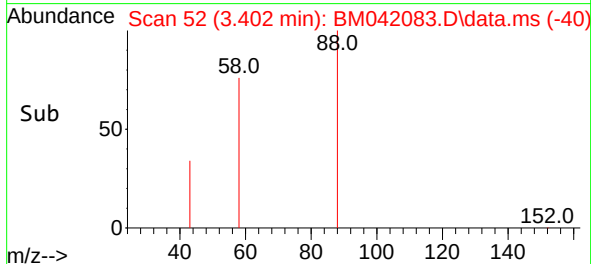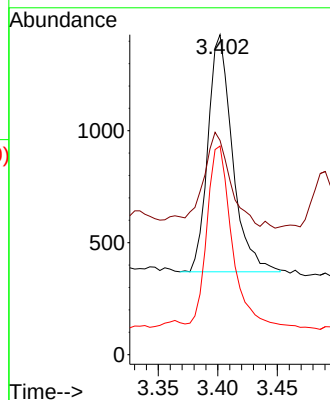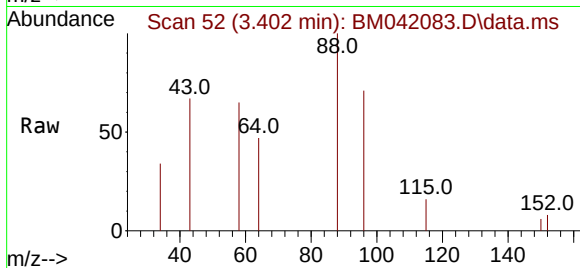

#5
 Naphthalene
 Concen: 0.028 ng/ul
 RT: 10.807 min Scan# 1766
 Delta R.T. -0.011 min
 Lab File: BM042083.D
 Acq: 27 Sep 2023 13:59

Tgt Ion: 128 Resp: 1037
 Ion Ratio Lower Upper
 128 100
 129 23.0 9.2 13.8#
 127 21.0 10.8 16.2#

