

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092723\
 Data File : BM042091.D
 Acq On : 27 Sep 2023 19:36
 Operator : MA/JU
 Sample : 04450-17
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBHR2

Quant Time: Sep 28 01:03:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 13:50:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.942	152	3732	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.757	136	10171	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.588	164	5091	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.341	188	11409	0.400	ng/ul	-0.01
17) Chrysene-d12	21.516	240	6101	0.400	ng/ul	0.00
23) Perylene-d12	23.921	264	6897	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	24128	4.744	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.335	152	5341	0.419	ng/ul	-0.02
18) Fluoranthene-d10	19.362	212	10963	0.436	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.398	88	1108	0.207	ng/ul#	32


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092723\
Data File : BM042091.D
Acq On : 27 Sep 2023 19:36
Operator : MA/JU
Sample : 04450-17
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBHR2


Quant Time: Sep 28 01:03:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 13:50:58 2023
Response via : Initial Calibration

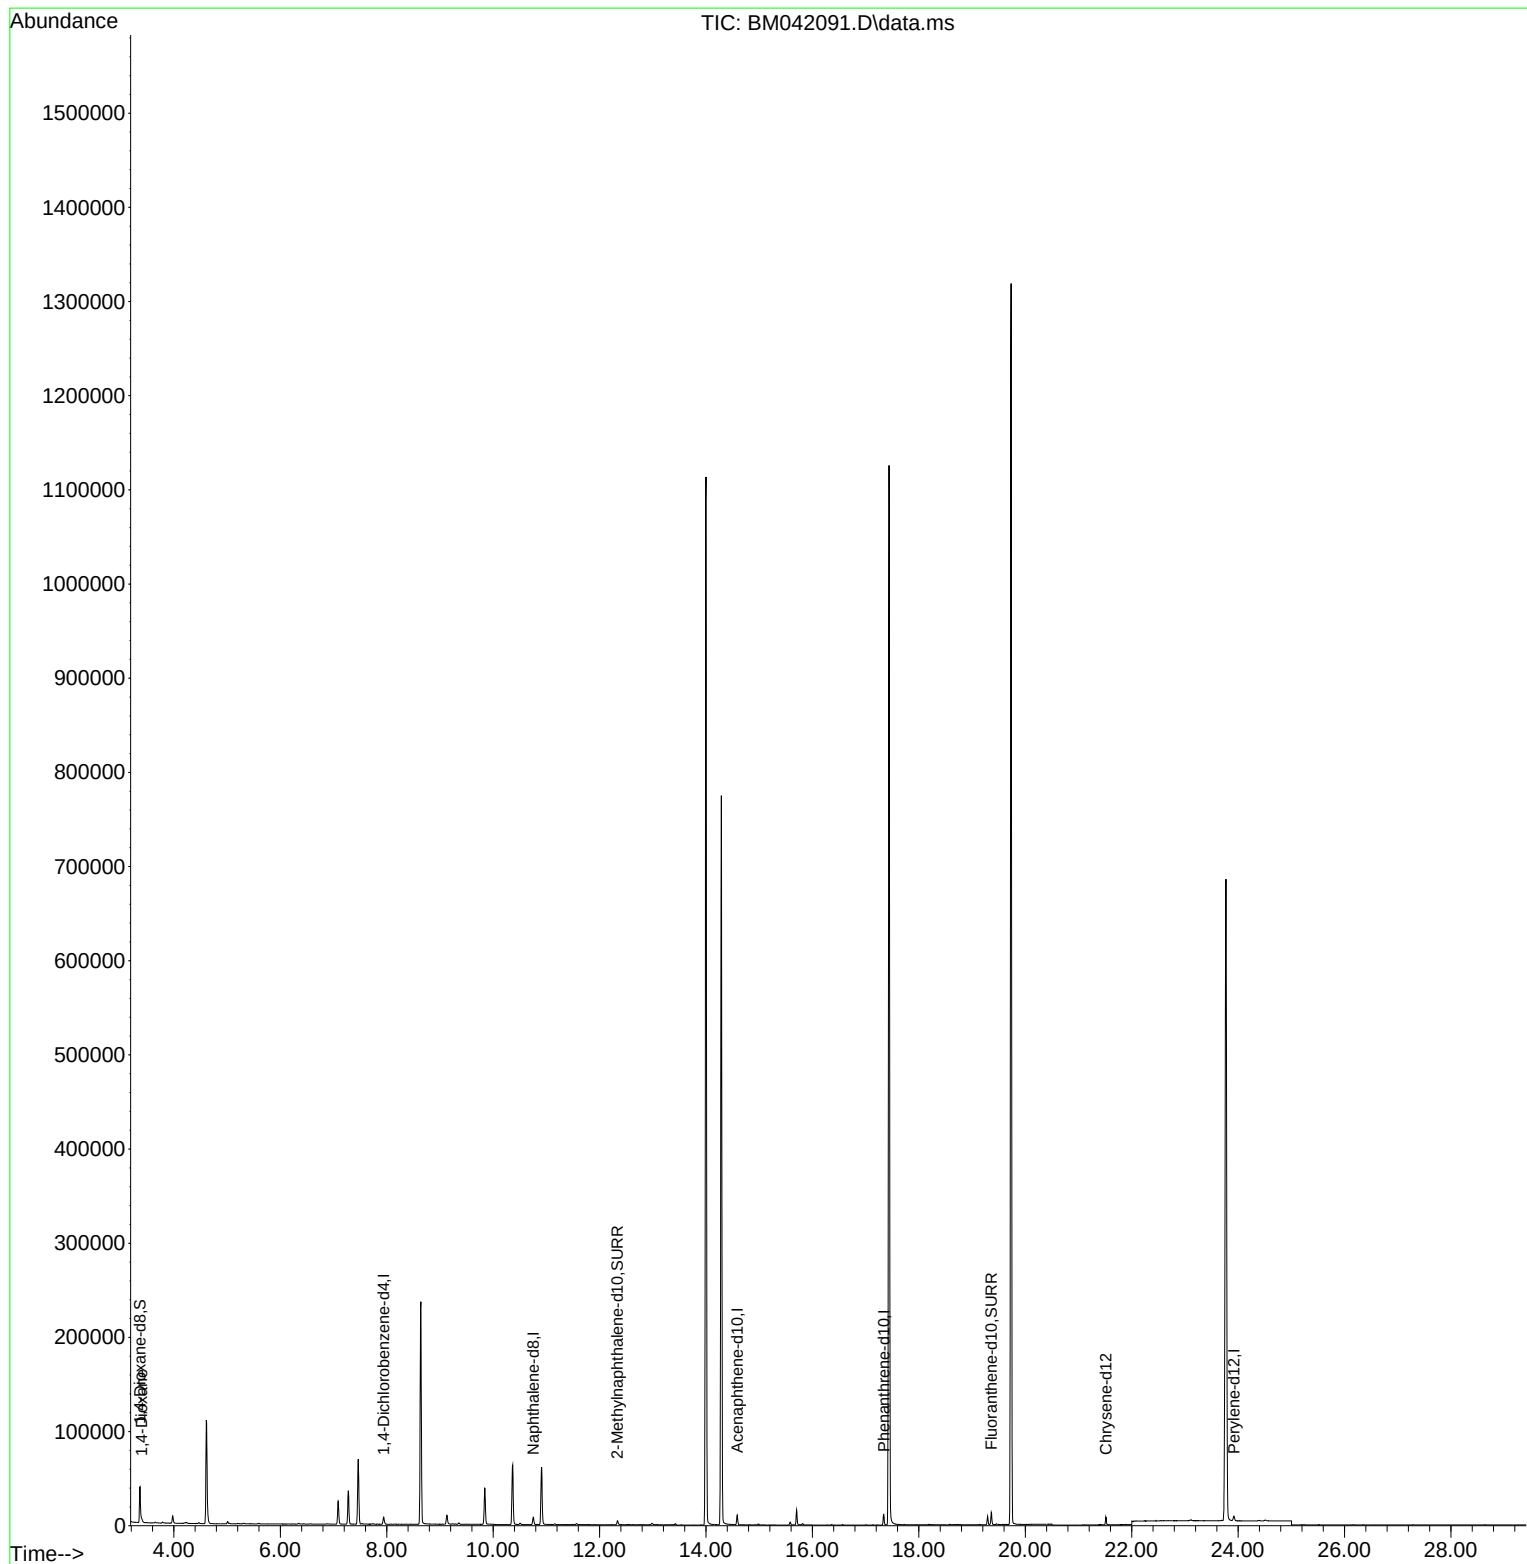

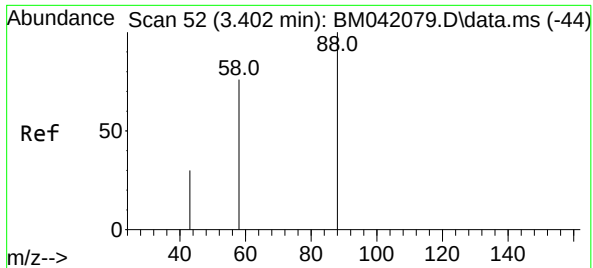

#2
 1,4-Dioxane
 Concen: 0.207 ng/ul
 RT: 3.398 min Scan# 51
 Delta R.T. -0.012 min
 Lab File: BM042091.D
 Acq: 27 Sep 2023 19:36

Instrument :
 BNA_M
 ClientSampleId :
 BBHR2

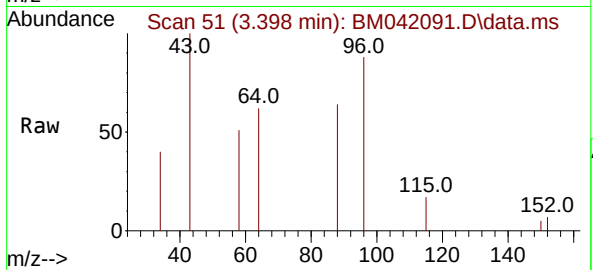

Tgt Ion: 88	Resp: 1108		
Ion Ratio	Lower	Upper	
88 100			
43 156.4	42.9	64.3#	
58 79.1	56.4	84.6	

