

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092723\
 Data File : BM042098.D
 Acq On : 27 Sep 2023 23:49
 Operator : MA/JU
 Sample : 04450-22
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJC9

Quant Time: Sep 28 01:04:37 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 13:50:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.941	152	3259	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.751	136	8451	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.587	164	4370	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.337	188	9155	0.400	ng/ul	-0.02
17) Chrysene-d12	21.512	240	4787	0.400	ng/ul	-0.01
23) Perylene-d12	23.915	264	5469	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	28242	6.359	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.335	152	4258	0.402	ng/ul	-0.02
18) Fluoranthene-d10	19.361	212	8406	0.426	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.397	88	2325	0.498	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092723\
Data File : BM042098.D
Acq On : 27 Sep 2023 23:49
Operator : MA/JU
Sample : 04450-22
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJC9

Quant Time: Sep 28 01:04:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 13:50:58 2023
Response via : Initial Calibration

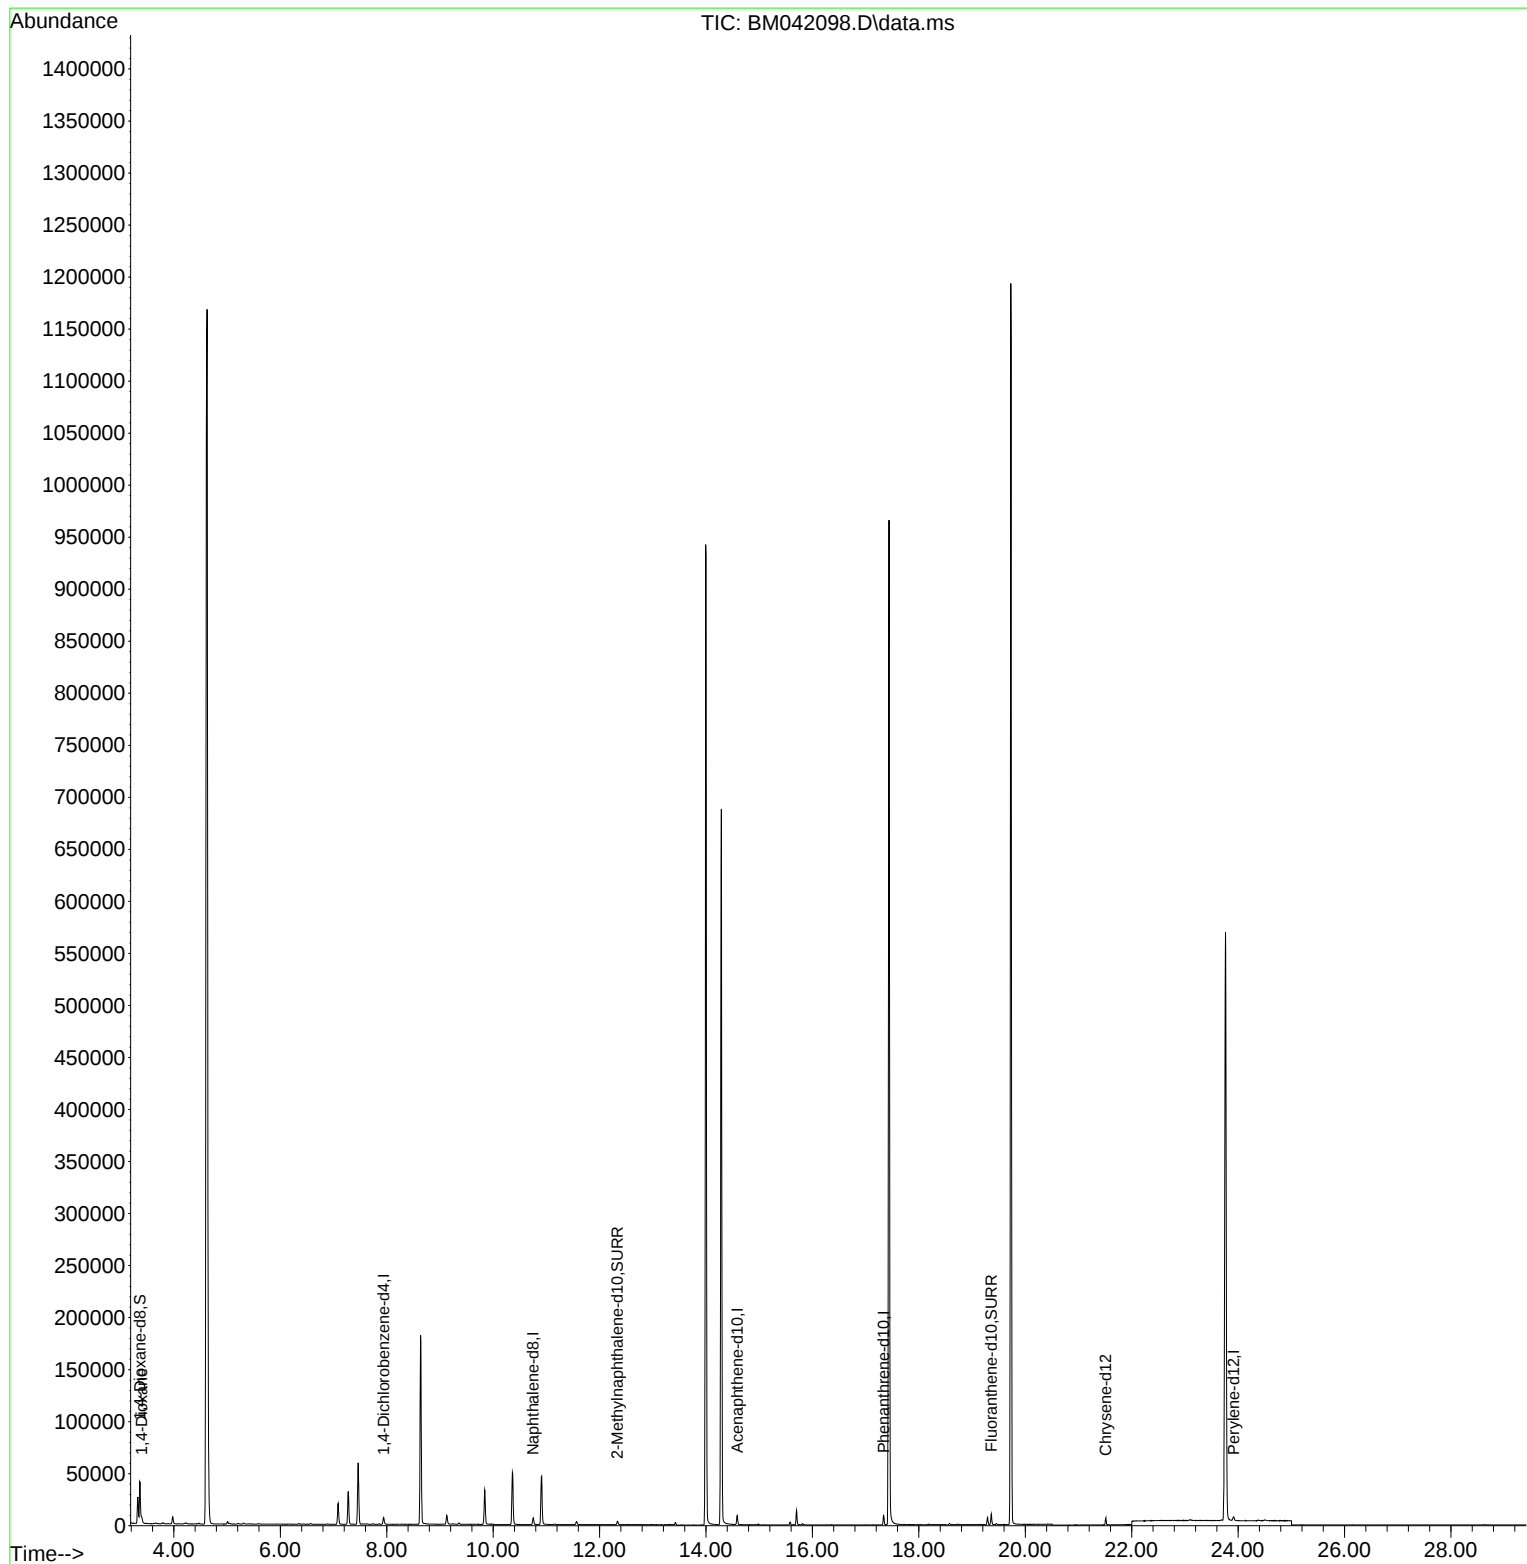

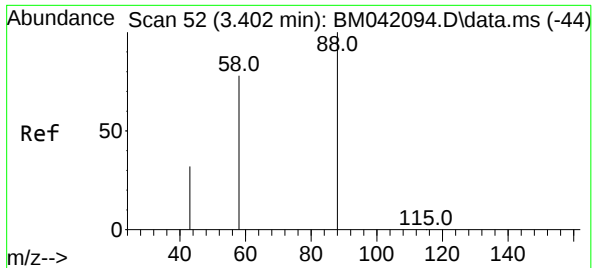

#2
 1,4-Dioxane
 Concen: 0.498 ng/ul
 RT: 3.397 min Scan# 51
 Delta R.T. -0.013 min
 Lab File: BM042098.D
 Acq: 27 Sep 2023 23:49

Instrument :
 BNA_M
 ClientSampleId :
 BBJC9

Tgt Ion:	88	Resp:	2325
Ion	Ratio	Lower	Upper
88	100		
43	64.5	42.9	64.3#
58	72.0	56.4	84.6

