

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092724\
 Data File : BM047680.D
 Acq On : 27 Sep 2024 18:55
 Operator : RC/JU
 Sample : SSTD01037
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD010021

Quant Time: Sep 28 02:05:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 28 01:59:50 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	135931	20.000	ng/u1	0.00
20) Naphthalene-d8	10.610	136	520217	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.451	164	298179	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.186	188	572030	20.000	ng/u1	0.00
79) Chrysene-d12	21.409	240	532729	20.000	ng/u1	0.00
88) Perylene-d12	24.415	264	579497	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	17769	5.272	ng/uL	0.00
4) Pyridine-d5	3.675	84	126248	11.724	ng/u1	0.00
7) Phenol-d5	6.975	99	119388	9.370	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.146	67	92860	11.708	ng/u1	0.00
11) 2-Chlorophenol-d4	7.346	132	92936	9.577	ng/u1	0.00
15) 4-Methylphenol-d8	8.516	113	86771	8.664	ng/u1	0.00
21) Nitrobenzene-d5	8.963	128	41883	10.425	ng/u1	0.00
24) 2-Nitrophenol-d4	9.692	143	37654	9.921	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	80248	10.399	ng/u1	0.00
31) 4-Chloroaniline-d4	10.739	131	118529	9.385	ng/u1	0.00
46) Dimethylphthalate-d6	13.857	166	223652	10.205	ng/u1	0.00
49) Acenaphthylene-d8	14.139	160	263137	9.950	ng/u1	0.00
54) 4-Nitrophenol-d4	14.633	143	35424	8.158	ng/u1	0.00
60) Fluorene-d10	15.439	176	192284	10.153	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.551	200	26397	8.729	ng/u1	0.00
73) Anthracene-d10	17.280	188	286901	10.416	ng/u1	0.00
81) Pyrene-d10	19.568	212	309241	9.960	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.209	264	308271	10.011	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.293	88	19680	5.410	ng/uL	91
5) Pyridine	3.693	79	134961	12.139	ng/u1	97
6) Benzaldehyde	6.951	77	78392	11.624	ng/u1	95
8) Phenol	7.004	94	128862	9.824	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.234	93	108523	10.462	ng/u1	95
12) 2-Chlorophenol	7.381	128	99815	9.931	ng/u1	99
13) 2-Methylphenol	8.251	108	88050	8.918	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.334	45	210689	13.860	ng/u1	99
16) Acetophenone	8.634	105	157966	9.801	ng/u1	97
17) N-Nitroso-di-n-propyla...	8.616	70	85608	10.009	ng/u1	99
18) 4-Methylphenol	8.581	108	101541	9.419	ng/u1	98
19) Hexachloroethane	8.898	117	45639	10.568	ng/u1	99
22) Nitrobenzene	9.010	77	121607	12.113	ng/u1	98
23) Isophorone	9.539	82	214621	10.720	ng/u1	98
25) 2-Nitrophenol	9.722	139	44561	10.155	ng/u1	96
26) 2,4-Dimethylphenol	9.781	107	98685	10.456	ng/u1	95
27) Bis(2-Chloroethoxy)met...	10.016	93	134781	11.126	ng/u1	96
29) 2,4-Dichlorophenol	10.251	162	83104	10.622	ng/u1	96
30) Naphthalene	10.657	128	315178	10.997	ng/u1	99
32) 4-Chloroaniline	10.763	127	117279	9.438	ng/u1	100
33) Hexachlorobutadiene	10.951	225	57751	12.376	ng/u1	99
34) Caprolactam	11.528	113	22209	7.370	ng/u1	96
35) 4-Chloro-3-methylphenol	11.886	107	81866	9.292	ng/u1	97
36) 2-Methylnaphthalene	12.269	142	194343	9.864	ng/u1	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092724\
 Data File : BM047680.D
 Acq On : 27 Sep 2024 18:55
 Operator : RC/JU
 Sample : SSTD01037
 Misc :
 ALS Vial : 3 Sample Multiplier: 1


Instrument :
 BNA_M
 ClientSampleId :
 SSTD010021


Quant Time: Sep 28 02:05:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 28 01:59:50 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.492	142	198075	9.951	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	12.639	216	102731	11.605	ng/ul	96
40) Hexachlorocyclopentadiene	12.628	237	57969	9.525	ng/ul	97
41) 2,4,6-Trichlorophenol	12.880	196	56833	10.463	ng/ul	98
42) 2,4,5-Trichlorophenol	12.945	196	63252	10.714	ng/ul	99
43) 1,1'-Biphenyl	13.280	154	253847	10.800	ng/ul	99
44) 2-Chloronaphthalene	13.322	162	195309	10.836	ng/ul	98
45) 2-Nitroaniline	13.522	65	54914	10.472	ng/ul	99
47) Dimethylphthalate	13.904	163	227910	10.238	ng/ul	99
48) 2,6-Dinitrotoluene	14.016	165	35961	8.852	ng/ul	92
50) Acenaphthylene	14.169	152	300647	10.517	ng/ul	99
51) 3-Nitroaniline	14.339	138	39491	8.327	ng/ul	95
52) Acenaphthene	14.510	153	214670	10.570	ng/ul	97
53) 2,4-Dinitrophenol	14.551	184	16134	7.218	ng/ul	90
55) 4-Nitrophenol	14.645	109	32033	8.762	ng/ul	97
56) Dibenzofuran	14.845	168	288883	10.943	ng/ul	99
57) 2,4-Dinitrotoluene	14.798	165	55498	9.487	ng/ul	94
58) 2,3,4,6-Tetrachlorophenol	15.069	232	47534	10.463	ng/ul#	97
59) Diethylphthalate	15.269	149	226794	9.629	ng/ul	100
61) Fluorene	15.492	166	238429	10.349	ng/ul	98
62) 4-Chlorophenyl-phenyle...	15.486	204	112360	10.532	ng/ul	99
63) 4-Nitroaniline	15.498	138	40031	8.530	ng/ul	98
66) 4,6-Dinitro-2-methylph...	15.563	198	30489	8.920	ng/ul	95
67) N-Nitrosodiphenylamine	15.698	169	184753	10.390	ng/ul	99
68) 4-Bromophenyl-phenylether	16.380	248	61106	10.325	ng/ul	93
69) Hexachlorobenzene	16.498	284	71033	10.504	ng/ul	98
70) Atrazine	16.645	200	59285	9.490	ng/ul	97
71) Pentachlorophenol	16.839	266	37139	8.727	ng/ul	96
72) Phenanthrene	17.227	178	348365	10.675	ng/ul	99
74) Anthracene	17.315	178	353719	10.705	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.245	216	101551	12.208	ng/uL	98
76) Pentachlorobenzene	14.769	250	96922	11.797	ng/uL	98
77) Carbazole	17.580	167	308595	10.215	ng/ul	99
78) Di-n-butylphthalate	18.151	149	337453	8.664	ng/ul	100
80) Fluoranthene	19.239	202	366070	10.004	ng/ul	98
82) Pyrene	19.598	202	412264	10.570	ng/ul	99
83) Butylbenzylphthalate	20.498	149	132134	7.421	ng/ul	94
84) 3,3'-Dichlorobenzidine	21.315	252	104025	8.259	ng/ul	98
85) Benzo(a)anthracene	21.392	228	387095	10.172	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.321	149	198810	7.364	ng/ul	98
87) Chrysene	21.450	228	380840	10.847	ng/ul	98
89) Di-n-octyl phthalate	22.456	149	301643	6.516	ng/ul	100
90) Benzo(b)fluoranthene	23.462	252	374805	10.076	ng/ul	98
91) Benzo(k)fluoranthene	23.527	252	383812	10.505	ng/ul	98
93) Benzo(a)pyrene	24.274	252	353798	10.353	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	27.803	276	457650	10.920	ng/ul	99
95) Dibenzo(a,h)anthracene	27.868	278	370445	10.856	ng/ul	98
96) Benzo(g,h,i)perylene	28.856	276	358270	11.191	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Sep 28 02:05:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 28 01:59:50 2024
Response via : Initial Calibration




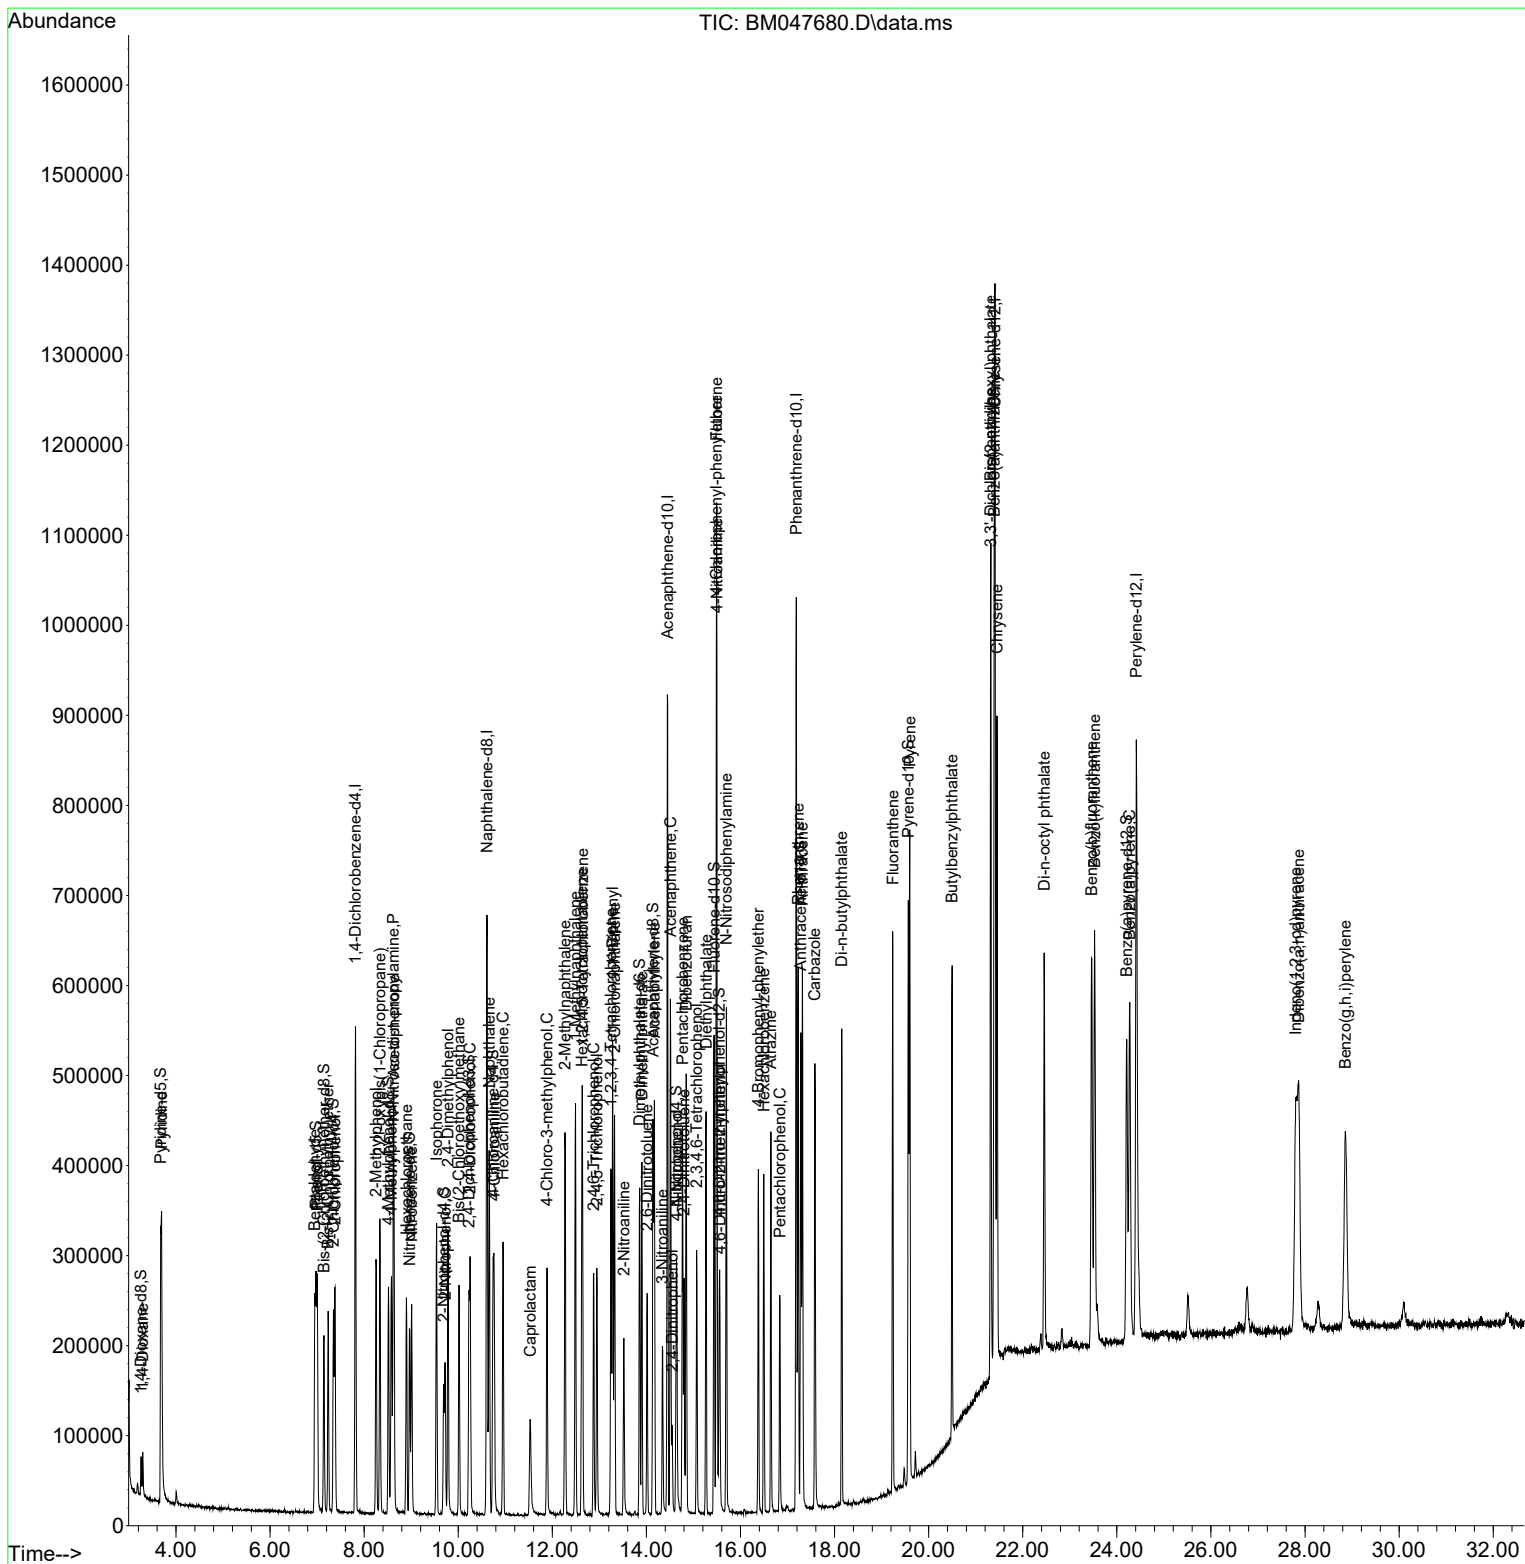




#2
1,4-Dioxane
Concen: 5.410 ng/uL
RT: 3.293 min Scan# 51
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55




Instrument :
BNA_M
ClientSampleId :
SSTD010021


Tgt Ion: 88 Resp: 19680
Ion Ratio Lower Upper
88 100
43 41.4 29.1 43.7
58 93.1 67.7 101.5

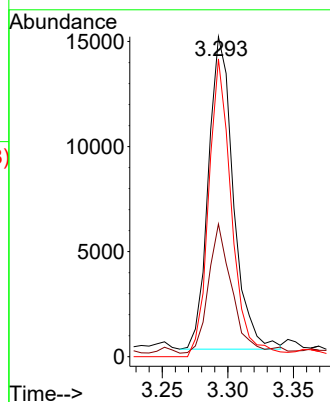

#5
Pyridine
Concen: 12.139 ng/uL
RT: 3.693 min Scan# 120
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55

Tgt Ion: 79 Resp: 134961
Ion Ratio Lower Upper
79 100
52 90.0 69.4 104.2
51 42.8 32.6 49.0



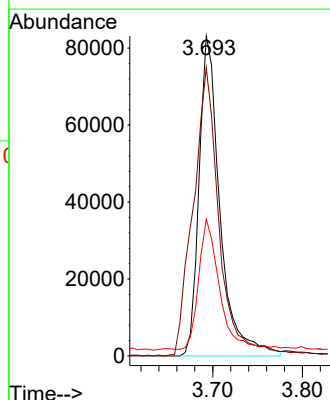
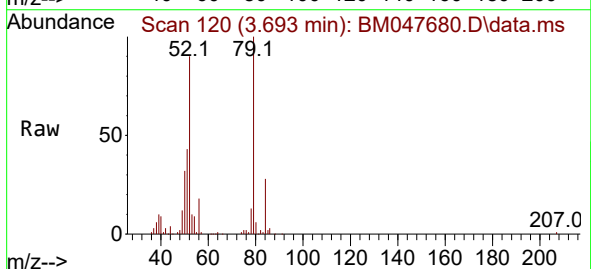




#6
Benzaldehyde
Concen: 11.624 ng/ul
RT: 6.951 min Scan# 674
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55




Instrument :
BNA_M
ClientSampleId :
SSTD010021


Tgt Ion: 77 Resp: 78392
Ion Ratio Lower Upper
77 100
105 87.0 72.2 108.2
106 82.3 70.7 106.1



#8
Phenol
Concen: 9.824 ng/ul
RT: 7.004 min Scan# 683
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55

Tgt Ion: 94 Resp: 128862
Ion Ratio Lower Upper
94 100
65 32.3 26.3 39.5
66 39.7 30.5 45.7

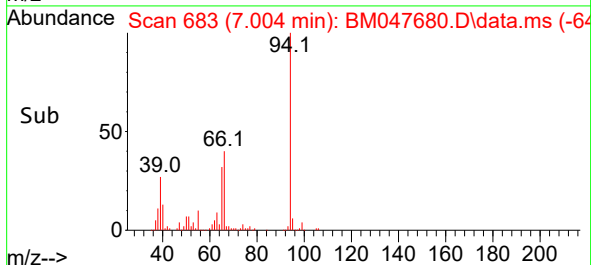







#10
 Bis(2-Chloroethyl)ether
 Concen: 10.462 ng/ul
 RT: 7.234 min Scan# 710
 Delta R.T. -0.000 min
 Lab File: BM047680.D
 Acq: 27 Sep 2024 18:55

Instrument :
 BNA_M
 ClientSampleId :
 SSTD010021

Tgt Ion: 93 Resp: 108523




Ion	Ratio	Lower	Upper
93	100		
63	92.5	69.4	104.2
95	33.0	25.0	37.6

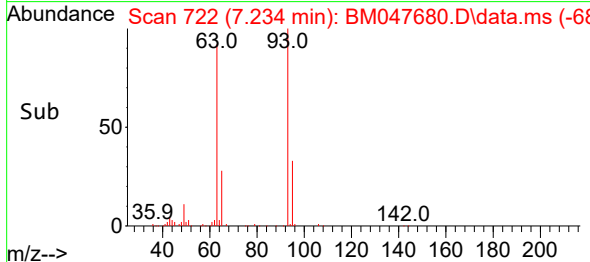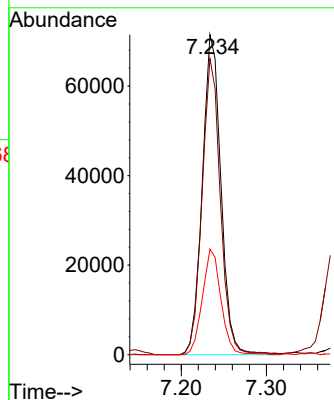


#12
 2-Chlorophenol
 Concen: 9.931 ng/ul
 RT: 7.381 min Scan# 747
 Delta R.T. -0.000 min
 Lab File: BM047680.D
 Acq: 27 Sep 2024 18:55

Tgt Ion:128 Resp: 99815

Ion	Ratio	Lower	Upper
128	100		
64	53.4	42.7	64.1
130	33.7	26.0	39.0

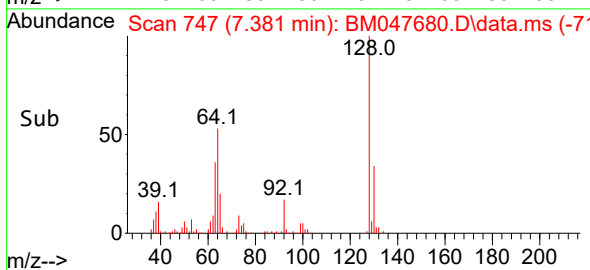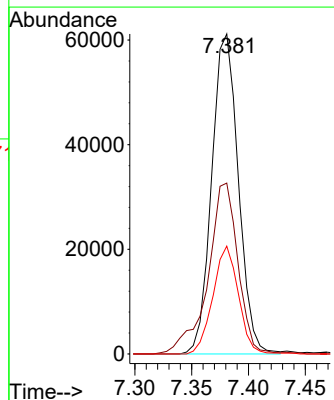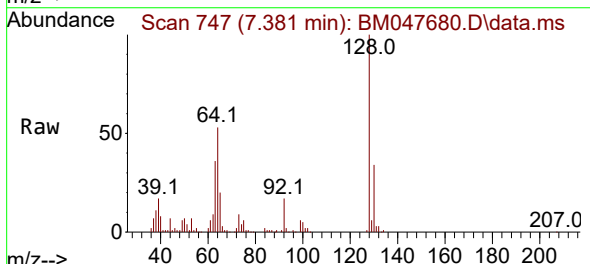



#13

2-Methylphenol

Concen: 8.918 ng/ul

RT: 8.251 min Scan# 896

Delta R.T. -0.006 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55

Instrument :

BNA_M

ClientSampleId :





SSTD010021

Tgt Ion:108 Resp: 88050

Ion Ratio Lower Upper

108 100

107 87.2 69.3 103.9



#14

2,2'-oxybis(1-Chloropropane)

Concen: 13.860 ng/ul

RT: 8.334 min Scan# 909

Delta R.T. -0.000 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55




Tgt Ion: 45 Resp: 210689


Ion Ratio Lower Upper

45 100

77 11.6 9.0 13.6

79 8.3 6.5 9.7









#16
Acetophenone
Concen: 9.801 ng/ul
RT: 8.634 min Scan# 916
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55




Instrument :
BNA_M
ClientSampleId :
SSTD010021


Tgt Ion:105 Resp: 157966
Ion Ratio Lower Upper
105 100
77 79.8 66.6 100.0
51 32.3 27.0 40.4



#17
N-Nitroso-di-n-propylamine
Concen: 10.009 ng/ul
RT: 8.616 min Scan# 957
Delta R.T. -0.006 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55

Tgt Ion: 70 Resp: 85608
Ion Ratio Lower Upper
70 100
42 69.7 55.3 82.9
101 7.4 6.8 10.2
130 17.2 13.7 20.5









#18
4-Methylphenol
Concen: 9.419 ng/ul
RT: 8.581 min Scan# 91
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55




Instrument :
BNA_M
ClientSampleId :
SSTD010021


Tgt Ion:108 Resp: 101541
Ion Ratio Lower Upper
108 100
107 108.8 88.4 132.6

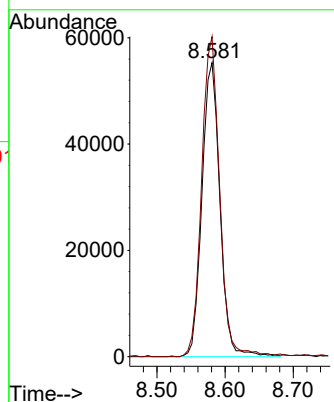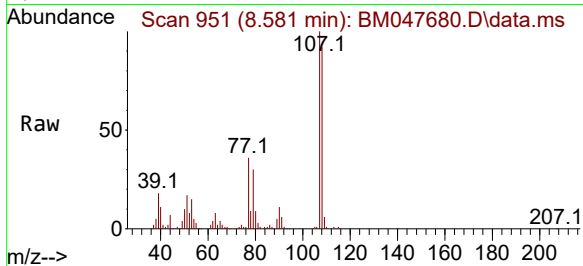

#19
Hexachloroethane
Concen: 10.568 ng/ul
RT: 8.898 min Scan# 1005
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55

Tgt Ion:117 Resp: 45639
Ion Ratio Lower Upper
117 100
201 89.9 71.0 106.6
199 55.7 44.2 66.4



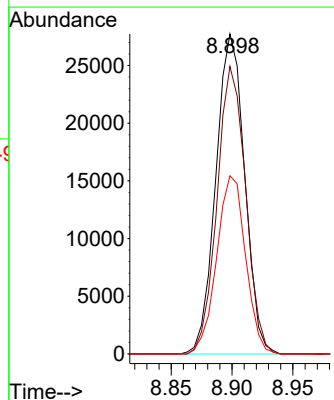
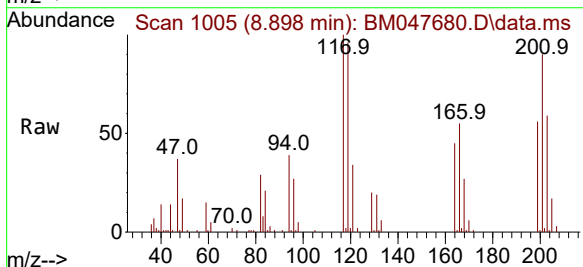




#22
Nitrobenzene
Concen: 12.113 ng/ul
RT: 9.010 min Scan# 1024
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55




Instrument :
BNA_M
ClientSampleId :
SSTD010021


Tgt Ion: 77 Resp: 121607
Ion Ratio Lower Upper
77 100
123 40.8 31.7 47.5
65 13.6 11.1 16.7

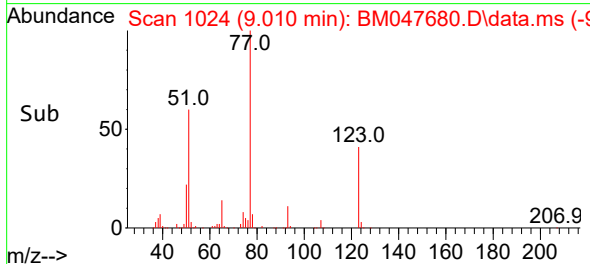

#23
Isophorone
Concen: 10.720 ng/ul
RT: 9.539 min Scan# 1114
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55

Tgt Ion: 82 Resp: 214621
Ion Ratio Lower Upper
82 100
95 6.4 4.9 7.3
138 15.7 12.0 18.0


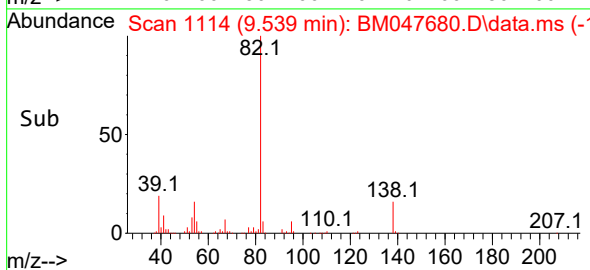

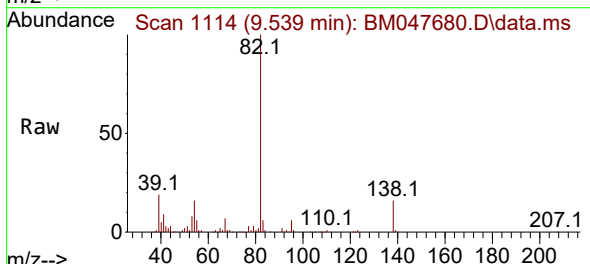




#25
2-Nitrophenol
Concen: 10.155 ng/ul
RT: 9.722 min Scan# 1145
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55




Instrument :
BNA_M
ClientSampleId :
SSTD010021


Tgt Ion:	139	Resp:	44561
Ion Ratio	Lower	Upper	
139	100		
65	57.6	49.6	74.4
109	30.1	23.4	35.2

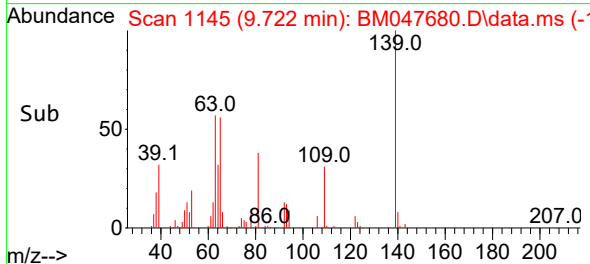

#26
2,4-Dimethylphenol
Concen: 10.456 ng/ul
RT: 9.781 min Scan# 1155
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55

Tgt Ion:	107	Resp:	98685
Ion Ratio	Lower	Upper	
107	100		
121	48.4	37.8	56.8
122	88.2	65.4	98.0

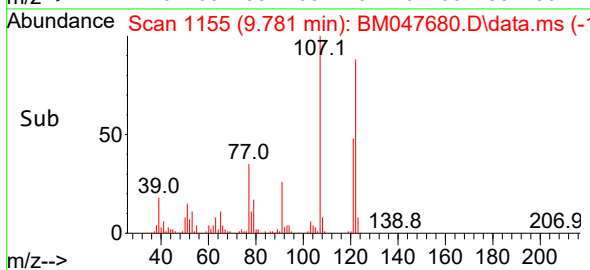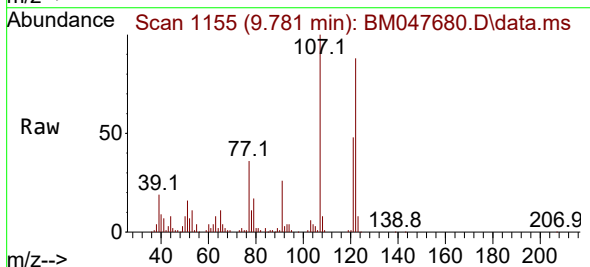



#27

Bis(2-Chloroethoxy)methane

Concen: 11.126 ng/ul

RT: 10.016 min Scan# 1195

Delta R.T. -0.006 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55

Instrument :

BNA_M

ClientSampleId :

SSTD010021





Tgt Ion: 93 Resp: 134781

Ion Ratio Lower Upper

93 100

95 30.9 27.1 40.7

123 10.0 8.2 12.4

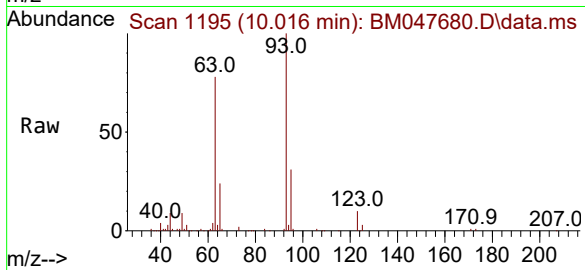

#29

2,4-Dichlorophenol

Concen: 10.622 ng/ul

RT: 10.251 min Scan# 1235

Delta R.T. -0.006 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55




Tgt Ion:162 Resp: 83104


Ion Ratio Lower Upper

162 100

164 61.9 52.2 78.2

98 40.6 30.6 46.0



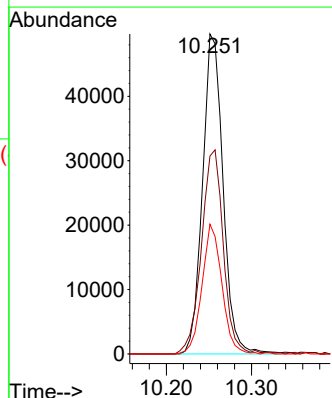
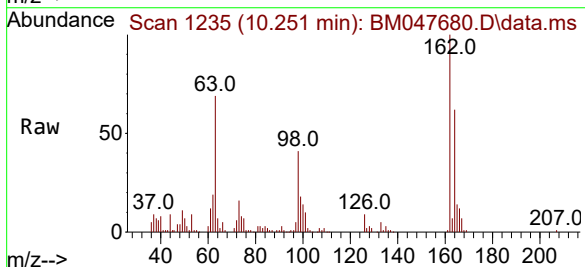




#30
Naphthalene
Concen: 10.997 ng/ul
RT: 10.657 min Scan# 11
Delta R.T. -0.006 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55




Instrument :
BNA_M
ClientSampleId :
SSTD010021


Tgt Ion:128 Resp: 315178
Ion Ratio Lower Upper
128 100
129 11.0 8.6 12.8
127 12.4 10.4 15.6



#32
4-Chloroaniline
Concen: 9.438 ng/ul
RT: 10.763 min Scan# 1322
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55

Tgt Ion:127 Resp: 117279
Ion Ratio Lower Upper
127 100
129 32.4 25.9 38.9

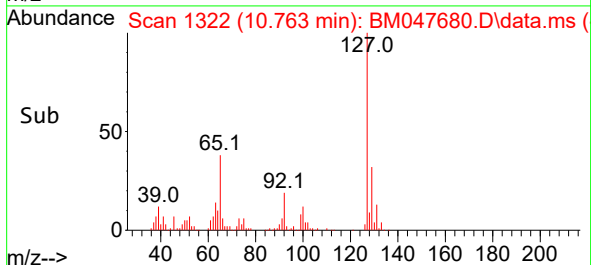



#33

Hexachlorobutadiene

Concen: 12.376 ng/ul

RT: 10.951 min Scan# 11

Delta R.T. -0.000 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55

Instrument :

BNA_M

ClientSampleId :

SSTD010021





Tgt Ion:225 Resp: 57751

Ion Ratio Lower Upper

225 100

223 63.3 50.3 75.5

227 62.2 49.1 73.7



#34

Caprolactam

Concen: 7.370 ng/ul

RT: 11.528 min Scan# 1452

Delta R.T. -0.006 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55




Tgt Ion:113 Resp: 22209


Ion Ratio Lower Upper

113 100

55 218.5 167.9 251.9

56 165.9 131.3 196.9




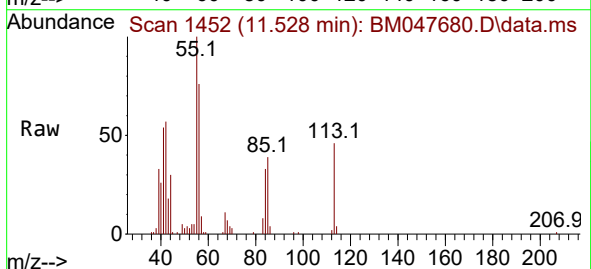




#35
4-Chloro-3-methylphenol
Concen: 9.292 ng/ul
RT: 11.886 min Scan# 1513
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55




Instrument :
BNA_M
ClientSampleId :
SSTD010021


Tgt Ion:107 Resp: 81866
Ion Ratio Lower Upper
107 100
144 25.8 18.7 28.1
142 80.7 62.7 94.1



#36
2-Methylnaphthalene
Concen: 9.864 ng/ul
RT: 12.269 min Scan# 1578
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55

Tgt Ion:142 Resp: 194343
Ion Ratio Lower Upper
142 100
141 88.4 72.5 108.7





#37

1-Methylnaphthalene

Concen: 9.951 ng/ul

RT: 12.492 min Scan# 1

Delta R.T. -0.000 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55

Instrument :

BNA_M

ClientSampleId :

SSTD010021





Tgt Ion:142 Resp: 198075

Ion Ratio Lower Upper

142 100

141 89.6 73.4 110.2

116 4.3 3.0 4.6

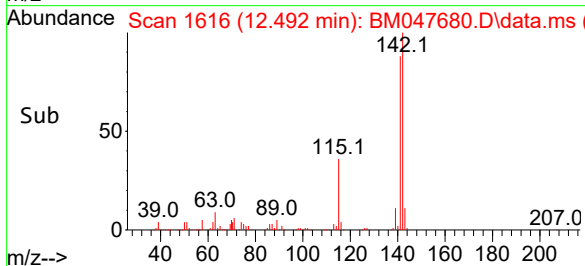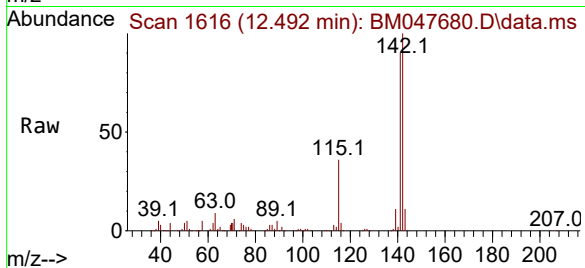

#39

1,2,4,5-Tetrachlorobenzene

Concen: 11.605 ng/ul

RT: 12.639 min Scan# 1641

Delta R.T. -0.000 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55

Tgt Ion:216 Resp: 102731




Ion Ratio Lower Upper


216 100

214 78.8 61.0 91.4

179 19.6 17.7 26.5

108 19.6 17.0 25.4


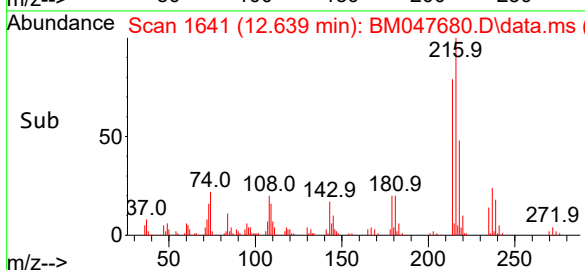

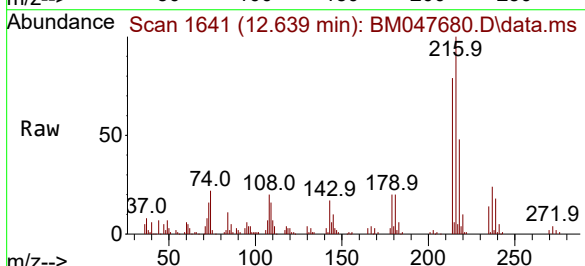




#40
Hexachlorocyclopentadiene
Concen: 9.525 ng/ul
RT: 12.628 min Scan# 1639
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55




Instrument :
BNA_M
ClientSampleId :
SSTD010021


Tgt Ion:237 Resp: 57969
Ion Ratio Lower Upper
237 100
235 64.2 49.8 74.6
272 13.4 9.7 14.5

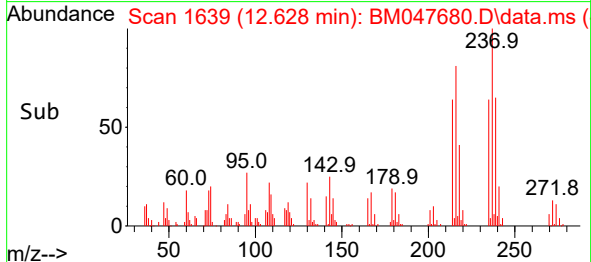

#41
2,4,6-Trichlorophenol
Concen: 10.463 ng/ul
RT: 12.880 min Scan# 1682
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55

Tgt Ion:196 Resp: 56833
Ion Ratio Lower Upper
196 100
198 94.1 77.1 115.7
200 29.6 24.5 36.7





#42

2,4,5-Trichlorophenol

Concen: 10.714 ng/ul

RT: 12.945 min Scan# 1

Delta R.T. -0.000 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55

Instrument :

BNA_M

ClientSampleId :

SSTD010021





Tgt Ion:196 Resp: 63252

Ion Ratio Lower Upper

196 100

198 97.7 79.5 119.3

200 32.1 25.8 38.8



#43

1,1'-Biphenyl

Concen: 10.800 ng/ul

RT: 13.280 min Scan# 1750

Delta R.T. -0.000 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55




Tgt Ion:154 Resp: 253847


Ion Ratio Lower Upper

154 100

153 39.9 31.1 46.7

76 14.7 12.1 18.1

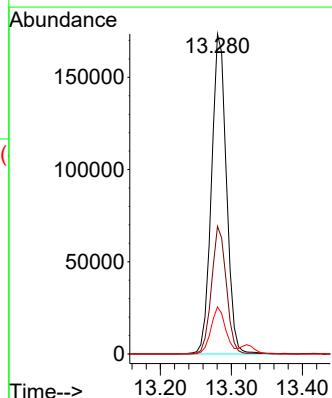



#44

2-Chloronaphthalene

Concen: 10.836 ng/ul

RT: 13.322 min Scan# 1

Delta R.T. -0.000 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55

Instrument :

BNA_M

ClientSampleId :

SSTD010021





Tgt Ion:162 Resp: 195309

Ion Ratio Lower Upper

162 100

164 34.3 25.3 37.9

127 41.2 32.9 49.3

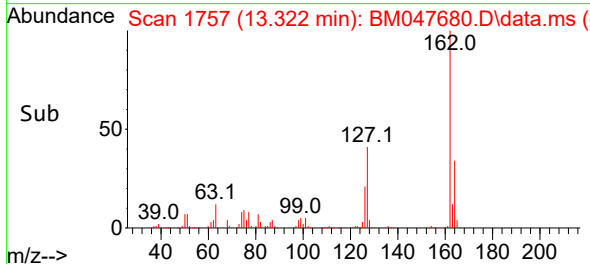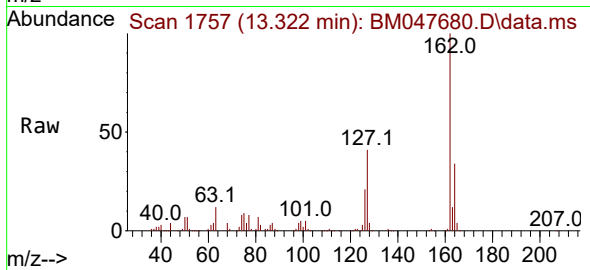

#45

2-Nitroaniline

Concen: 10.472 ng/ul

RT: 13.522 min Scan# 1791

Delta R.T. -0.000 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55




Tgt Ion: 65 Resp: 54914


Ion Ratio Lower Upper

65 100

92 61.7 49.1 73.7

138 83.0 67.6 101.4


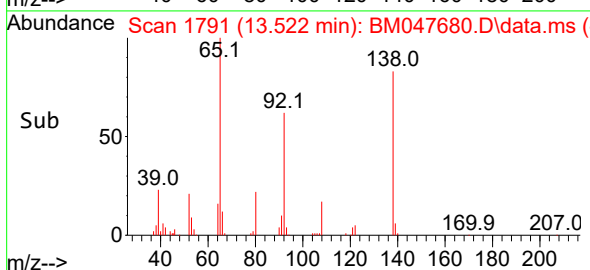

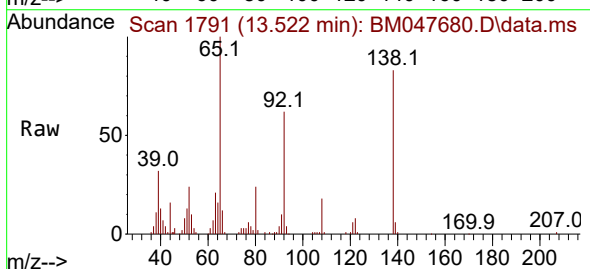




#47
Dimethylphthalate
Concen: 10.238 ng/ul
RT: 13.904 min Scan# 1856
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55




Instrument :
BNA_M
ClientSampleId :
SSTD010021


Tgt Ion:163 Resp: 227910
Ion Ratio Lower Upper
163 100
194 3.8 3.0 4.6
164 10.0 7.8 11.6

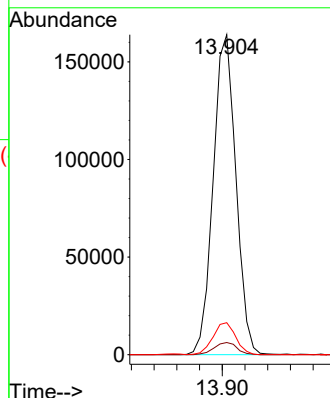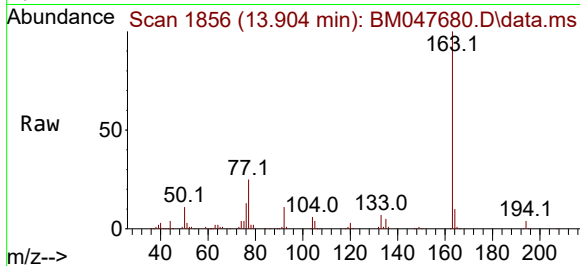

#48
2,6-Dinitrotoluene
Concen: 8.852 ng/ul
RT: 14.016 min Scan# 1875
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55

Tgt Ion:165 Resp: 35961
Ion Ratio Lower Upper
165 100
89 79.8 58.5 87.7
121 28.4 20.2 30.2



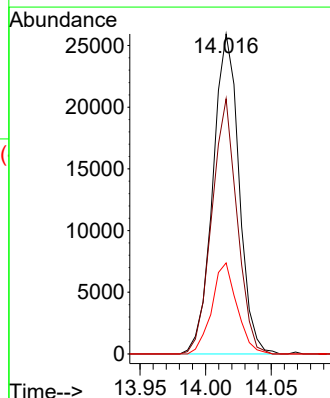
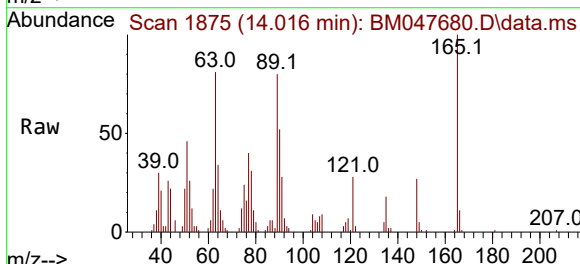




#50
Acenaphthylene
Concen: 10.517 ng/ul
RT: 14.169 min Scan# 1901
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55




Instrument :
BNA_M
ClientSampleId :
SSTD010021


Tgt Ion:152 Resp: 300647
Ion Ratio Lower Upper
152 100
151 19.5 16.2 24.2
153 12.8 10.7 16.1

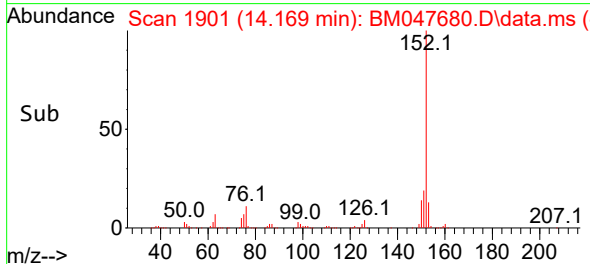

#51
3-Nitroaniline
Concen: 8.327 ng/ul
RT: 14.339 min Scan# 1930
Delta R.T. -0.006 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55

Tgt Ion:138 Resp: 39491
Ion Ratio Lower Upper
138 100
108 13.3 9.0 13.6
92 132.6 101.5 152.3

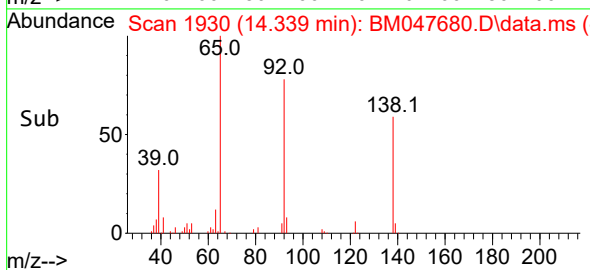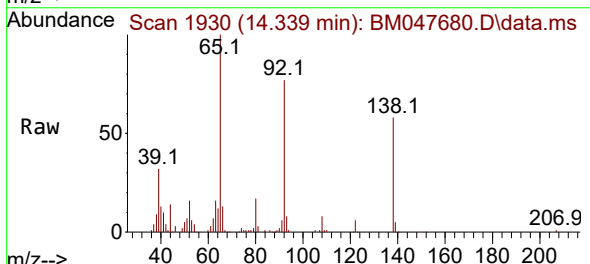



#52

Acenaphthene

Concen: 10.570 ng/ul

RT: 14.510 min Scan# 1959

Delta R.T. -0.000 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55

Instrument :

BNA_M

ClientSampleId :

SSTD010021





Tgt Ion:153 Resp: 214670

Ion Ratio Lower Upper

153 100

152 49.0 39.7 59.5

154 86.2 72.6 108.8

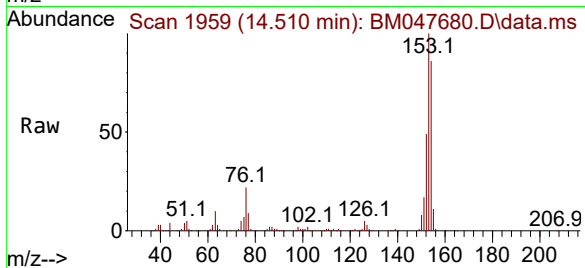

#53

2,4-Dinitrophenol

Concen: 7.218 ng/ul

RT: 14.551 min Scan# 1966

Delta R.T. 0.006 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55




Tgt Ion:184 Resp: 16134


Ion Ratio Lower Upper

184 100

63 82.3 77.5 116.3

154 66.9 55.8 83.6




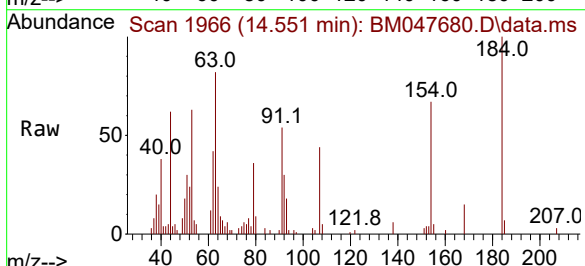




#55
4-Nitrophenol
Concen: 8.762 ng/ul
RT: 14.645 min Scan# 1983
Delta R.T. -0.006 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55




Instrument :
BNA_M
ClientSampleId :
SSTD010021


Tgt Ion:109 Resp: 32033
Ion Ratio Lower Upper
109 100
139 130.4 105.7 158.5
65 160.3 123.1 184.7

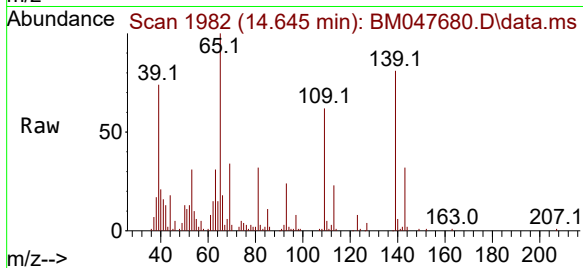

#56
Dibenzofuran
Concen: 10.943 ng/ul
RT: 14.845 min Scan# 2016
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55

Tgt Ion:168 Resp: 288883
Ion Ratio Lower Upper
168 100
139 39.2 31.0 46.6

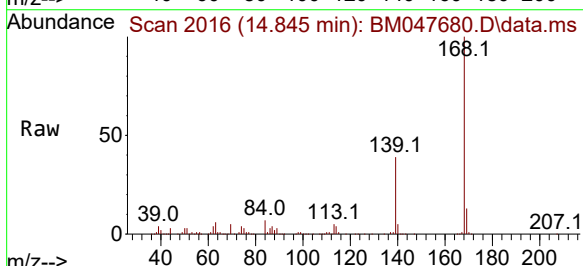



#57

2,4-Dinitrotoluene

Concen: 9.487 ng/ul

RT: 14.798 min Scan# 2008

Delta R.T. -0.006 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55

Instrument :

BNA_M

ClientSampleId :

SSTD010021





Tgt Ion:165 Resp: 55498

Ion Ratio Lower Upper

165 100

63 61.6 45.8 68.6

182 2.1 1.7 2.5

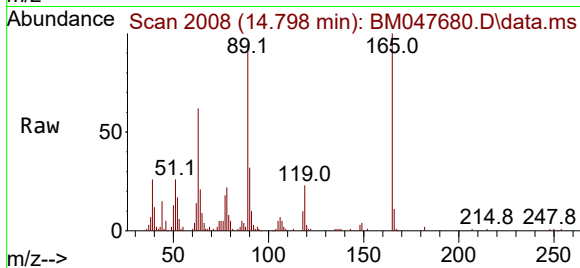

#58

2,3,4,6-Tetrachlorophenol

Concen: 10.463 ng/ul

RT: 15.069 min Scan# 2054

Delta R.T. -0.000 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55

Tgt Ion:232 Resp: 47534




Ion Ratio Lower Upper


232 100

131 53.2 40.2 60.4

130 2.5 2.6 4.0#

166 32.3 25.3 37.9

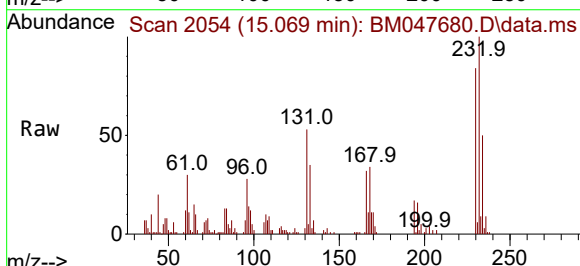



#59

Diethylphthalate

Concen: 9.629 ng/ul

RT: 15.269 min Scan# 2088

Delta R.T. -0.000 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55

Instrument :

BNA_M

ClientSampleId :

SSTD010021





Tgt Ion:149 Resp: 226794

Ion Ratio Lower Upper

149 100

177 21.1 16.9 25.3

150 11.9 9.2 13.8



#61

Fluorene

Concen: 10.349 ng/ul

RT: 15.492 min Scan# 2126

Delta R.T. -0.000 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55




Tgt Ion:166 Resp: 238429


Ion Ratio Lower Upper

166 100

165 99.2 77.8 116.6

167 13.5 10.8 16.2


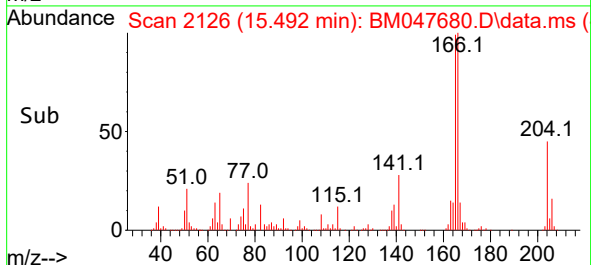
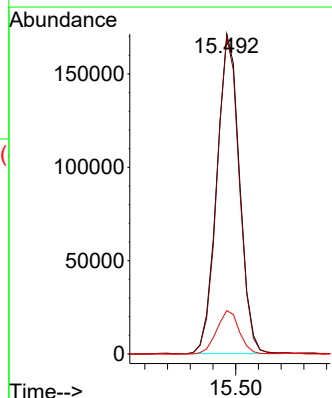





#62
4-Chlorophenyl-phenylether
Concen: 10.532 ng/ul
RT: 15.486 min Scan# 2125
Delta R.T. -0.006 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55




Instrument :
BNA_M
ClientSampleId :
SSTD010021


Tgt Ion:204 Resp: 112360
Ion Ratio Lower Upper
204 100
206 33.3 27.0 40.4
141 62.0 49.2 73.8

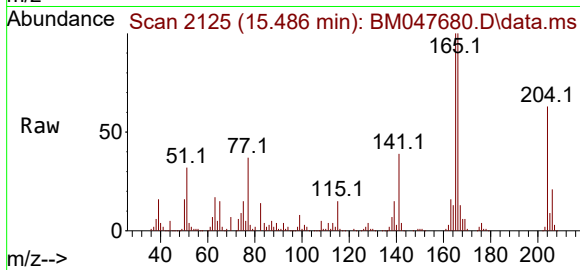

#63
4-Nitroaniline
Concen: 8.530 ng/ul
RT: 15.498 min Scan# 2127
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55

Tgt Ion:138 Resp: 40031
Ion Ratio Lower Upper
138 100
92 52.1 44.9 67.3
108 78.0 62.4 93.6



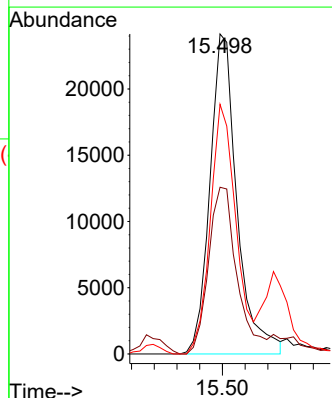
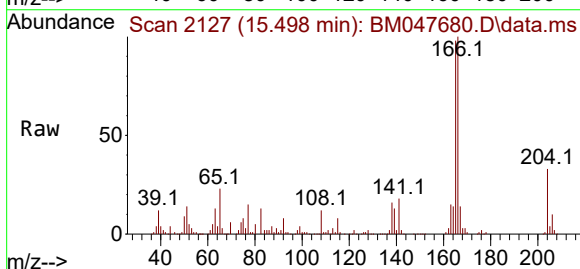




#66
 4,6-Dinitro-2-methylphenol
 Concen: 8.920 ng/ul
 RT: 15.563 min Scan# 2138
 Delta R.T. -0.000 min
 Lab File: BM047680.D
 Acq: 27 Sep 2024 18:55




Instrument :
 BNA_M
 ClientSampleId :
 SST010021


Tgt Ion:198 Resp: 30489
 Ion Ratio Lower Upper
 198 100
 182 7.0 5.1 7.7
 77 35.7 26.2 39.2

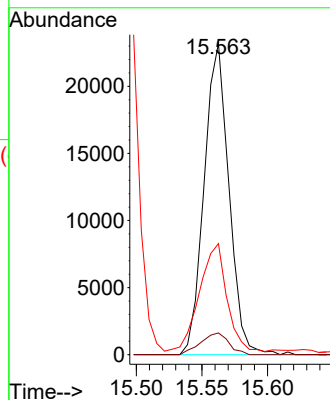

#67
 N-Nitrosodiphenylamine
 Concen: 10.390 ng/ul
 RT: 15.698 min Scan# 2161
 Delta R.T. -0.000 min
 Lab File: BM047680.D
 Acq: 27 Sep 2024 18:55

Tgt Ion:169 Resp: 184753
 Ion Ratio Lower Upper
 169 100
 168 67.6 53.5 80.3
 167 36.9 30.0 45.0



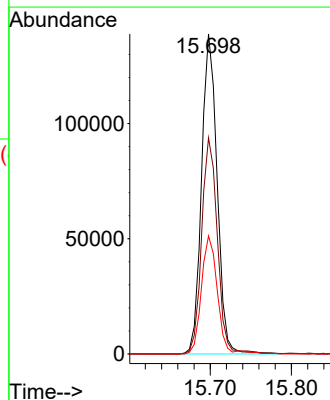





#68
4-Bromophenyl-phenylether
Concen: 10.325 ng/ul
RT: 16.380 min Scan# 211
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55




Instrument :
BNA_M
ClientSampleId :
SSTD010021


Tgt Ion:248 Resp: 61106
Ion Ratio Lower Upper
248 100
250 88.2 76.5 114.7
141 69.9 60.8 91.2

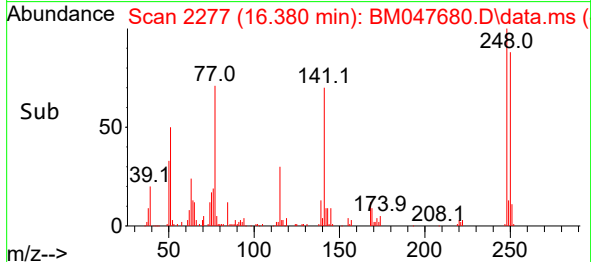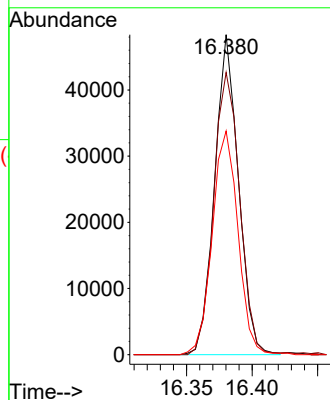

#69
Hexachlorobenzene
Concen: 10.504 ng/ul
RT: 16.498 min Scan# 2297
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55

Tgt Ion:284 Resp: 71033
Ion Ratio Lower Upper
284 100
142 40.5 32.4 48.6
249 30.7 26.3 39.5

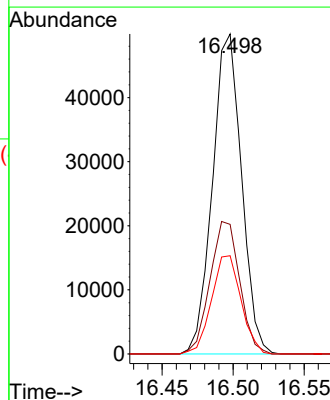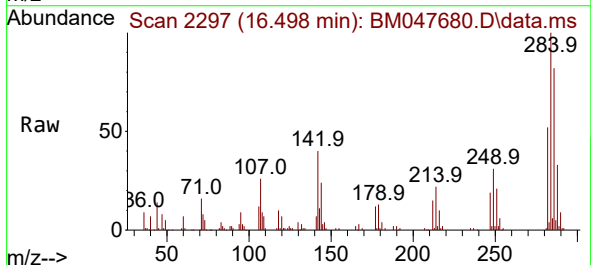



#70

Atrazine

Concen: 9.490 ng/ul

RT: 16.645 min Scan# 21

Delta R.T. -0.006 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55

Instrument :

BNA_M

ClientSampleId :

SSTD010021





Tgt Ion:200 Resp: 59285

Ion Ratio Lower Upper

200 100

173 27.6 20.2 30.2

215 48.3 39.4 59.2

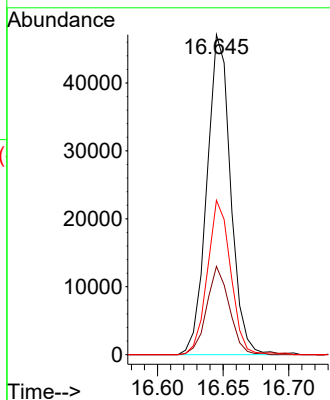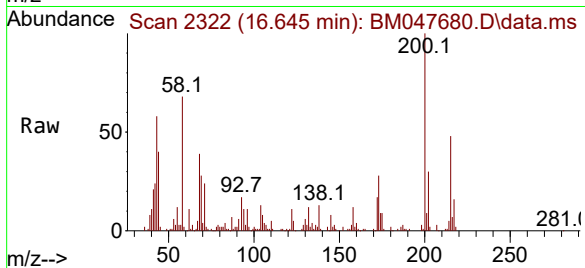

#71

Pentachlorophenol

Concen: 8.727 ng/ul

RT: 16.839 min Scan# 2355

Delta R.T. -0.000 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55




Tgt Ion:266 Resp: 37139


Ion Ratio Lower Upper

266 100

264 61.3 50.2 75.2

268 68.2 50.9 76.3



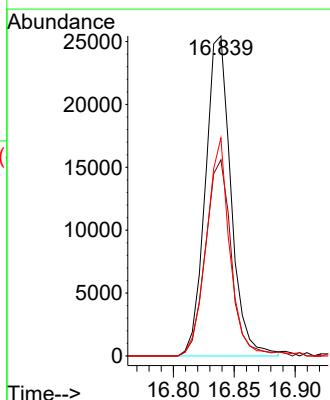
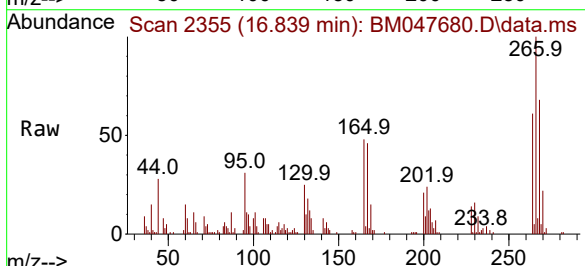




#72
Phenanthrene
Concen: 10.675 ng/ul
RT: 17.227 min Scan# 2421
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55




Instrument :
BNA_M
ClientSampleId :
SSTD010021


Tgt Ion:178 Resp: 348365
Ion Ratio Lower Upper
178 100
179 15.6 12.0 18.0
176 19.3 15.4 23.0

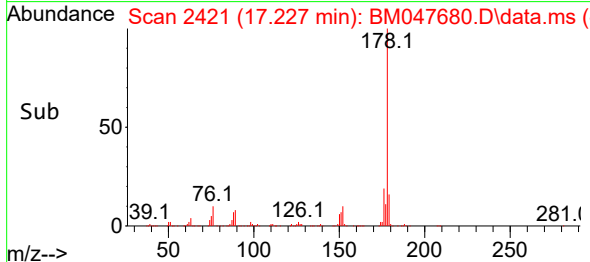

#74
Anthracene
Concen: 10.705 ng/ul
RT: 17.315 min Scan# 2436
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55

Tgt Ion:178 Resp: 353719
Ion Ratio Lower Upper
178 100
179 15.3 12.4 18.6
176 19.0 14.7 22.1


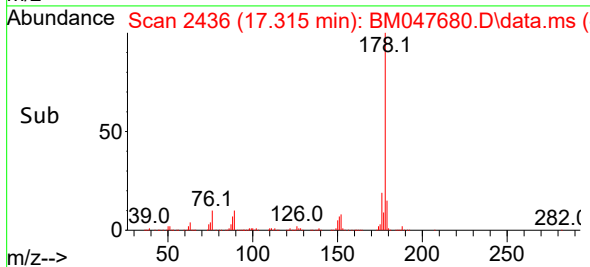

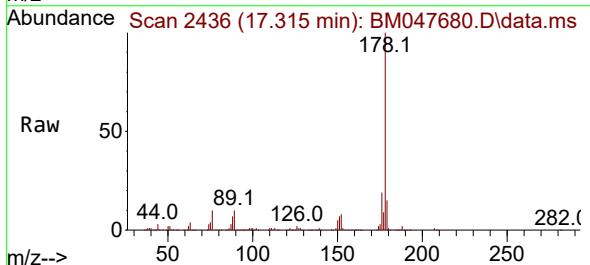




#75
1,2,3,4-Tetrachlorobenzene
Concen: 12.208 ng/uL
RT: 13.245 min Scan# 11
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55




Instrument :
BNA_M
ClientSampleId :
SSTD010021


Tgt Ion:216 Resp: 101551
Ion Ratio Lower Upper
216 100
214 81.1 63.0 94.4
218 47.3 37.6 56.4

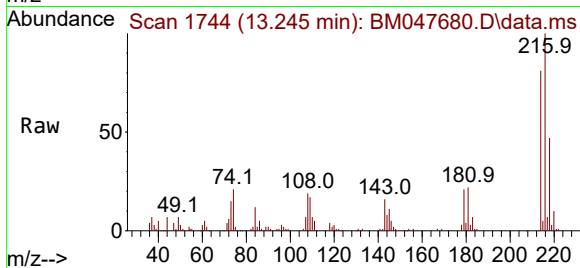

#76
Pentachlorobenzene
Concen: 11.797 ng/uL
RT: 14.769 min Scan# 2003
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55

Tgt Ion:250 Resp: 96922
Ion Ratio Lower Upper
250 100
248 63.1 50.2 75.2
252 64.3 49.4 74.0


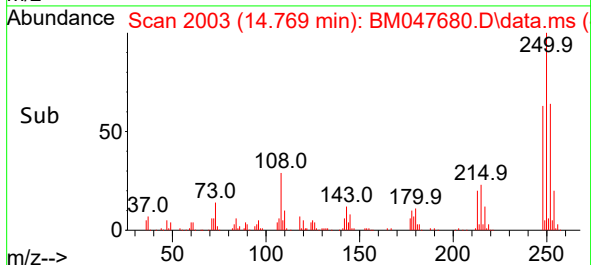

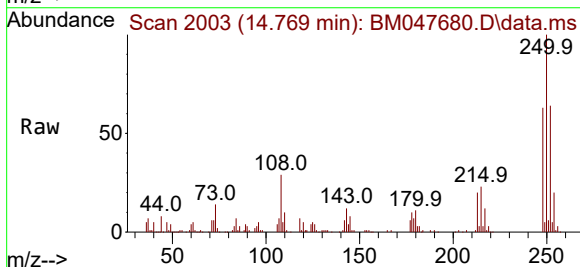




#77
 Carbazole
 Concen: 10.215 ng/ul
 RT: 17.580 min Scan# 2481
 Delta R.T. -0.000 min
 Lab File: BM047680.D
 Acq: 27 Sep 2024 18:55




Instrument :
 BNA_M
 ClientSampleId :
 SSTD010021


Tgt Ion:167 Resp: 308595
 Ion Ratio Lower Upper
 167 100
 166 21.8 17.4 26.0
 139 13.0 10.9 16.3

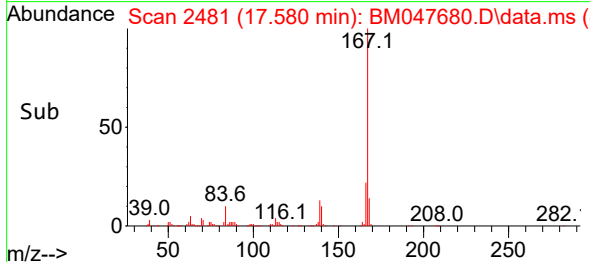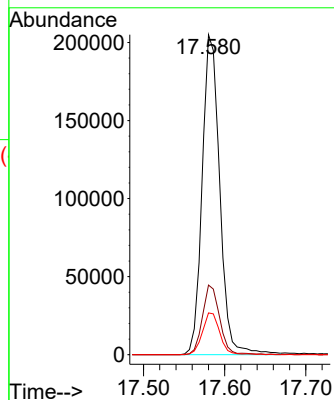

#78
 Di-n-butylphthalate
 Concen: 8.664 ng/ul
 RT: 18.151 min Scan# 2578
 Delta R.T. -0.000 min
 Lab File: BM047680.D
 Acq: 27 Sep 2024 18:55

Tgt Ion:149 Resp: 337453
 Ion Ratio Lower Upper
 149 100
 150 9.3 7.4 11.2
 104 5.7 4.6 7.0


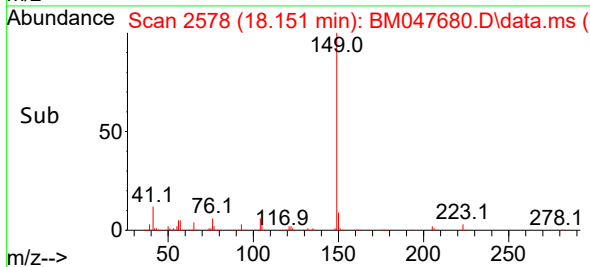
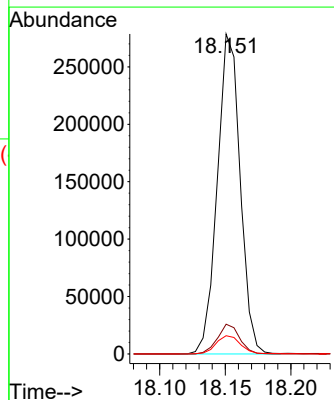
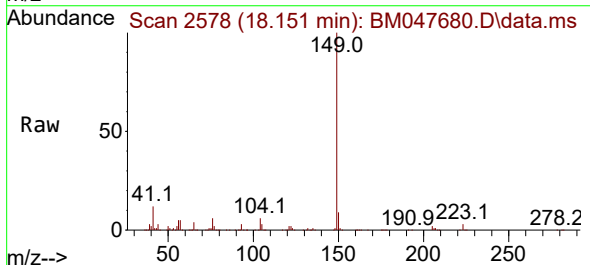




#80
Fluoranthene
Concen: 10.004 ng/ul
RT: 19.239 min Scan# 2763
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55




Instrument :
BNA_M
ClientSampleId :
SSTD010021


Tgt Ion:202 Resp: 366070
Ion Ratio Lower Upper
202 100
101 10.7 9.0 13.4
100 9.2 6.8 10.2

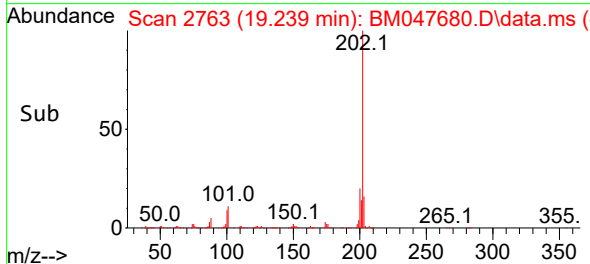

#82
Pyrene
Concen: 10.570 ng/ul
RT: 19.598 min Scan# 2824
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55

Tgt Ion:202 Resp: 412264
Ion Ratio Lower Upper
202 100
101 13.3 10.9 16.3
100 11.1 9.4 14.2

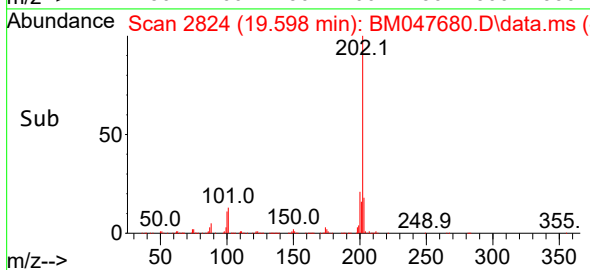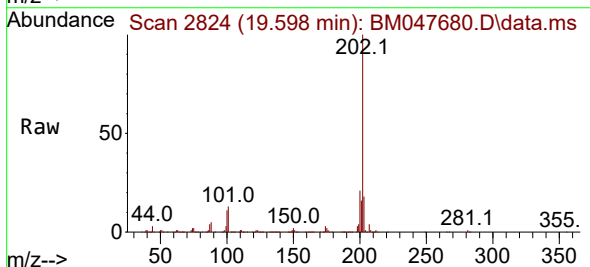



#83

Butylbenzylphthalate

Concen: 7.421 ng/ul

RT: 20.498 min Scan# 2976

Delta R.T. 0.006 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55

Instrument :

BNA_M

ClientSampleId :

SSTD010021





Tgt Ion:149 Resp: 132134

Ion Ratio Lower Upper

149 100

91 77.3 66.9 100.3

206 18.4 14.4 21.6



#84

3,3'-Dichlorobenzidine

Concen: 8.259 ng/ul

RT: 21.315 min Scan# 3116

Delta R.T. -0.000 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55




Tgt Ion:252 Resp: 104025


Ion Ratio Lower Upper

252 100

254 62.6 51.5 77.3

126 12.3 9.4 14.0





#85

Benzo(a)anthracene

Concen: 10.172 ng/ul

RT: 21.392 min Scan# 3129

Delta R.T. -0.000 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55

Instrument :

BNA_M

ClientSampleId :

SSTD010021





Tgt Ion:228 Resp: 387095

Ion Ratio Lower Upper

228 100

229 20.0 15.6 23.4

226 26.7 21.9 32.9

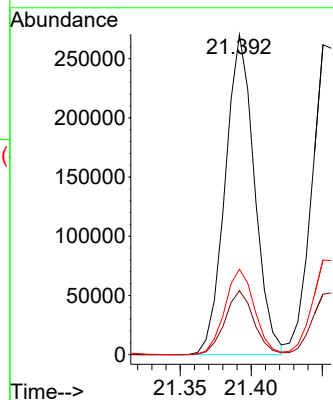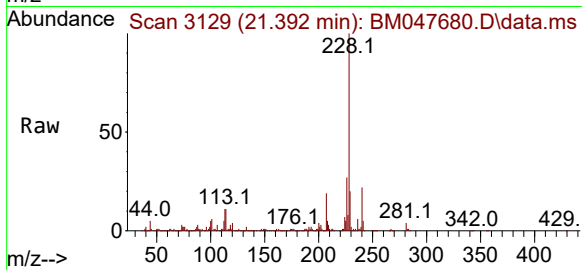

#86

Bis(2-ethylhexyl)phthalate

Concen: 7.364 ng/ul

RT: 21.321 min Scan# 3117

Delta R.T. -0.000 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55




Tgt Ion:149 Resp: 198810


Ion Ratio Lower Upper

149 100

167 25.5 21.3 31.9

279 3.3 2.7 4.1

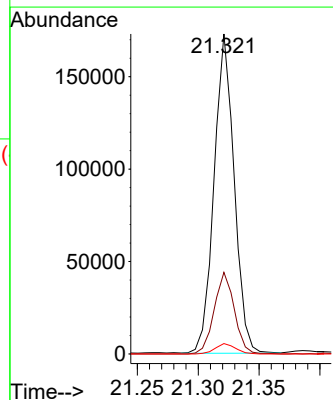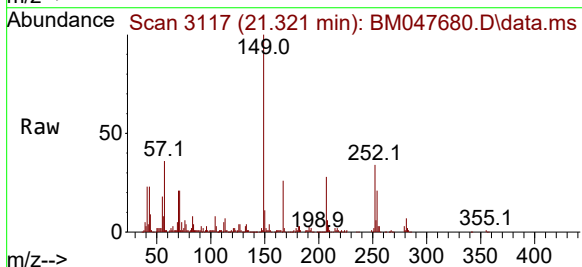



#87

Chrysene

Concen: 10.847 ng/ul

RT: 21.450 min Scan# 3139

Delta R.T. -0.000 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55

Instrument :

BNA_M

ClientSampleId :

SSTD010021





Tgt Ion:228 Resp: 380840

Ion Ratio Lower Upper

228 100

226 30.5 23.6 35.4

229 19.5 15.3 22.9

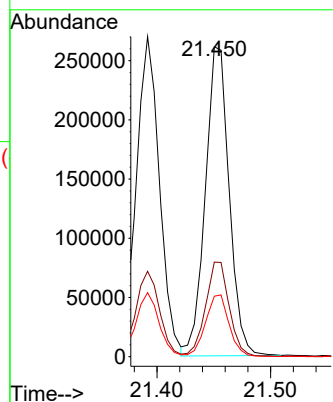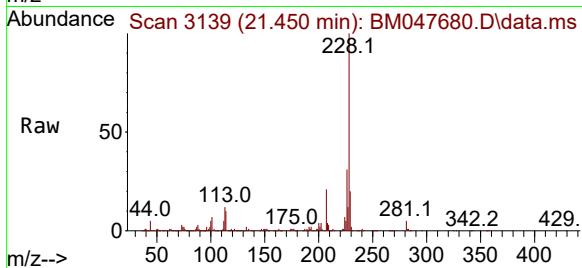

#89

Di-n-octyl phthalate

Concen: 6.516 ng/ul




RT: 22.456 min Scan# 3310


Delta R.T. -0.000 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55

Tgt Ion:149 Resp: 301643



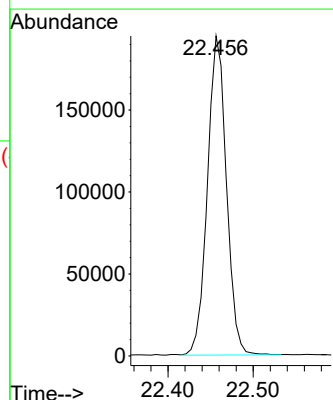
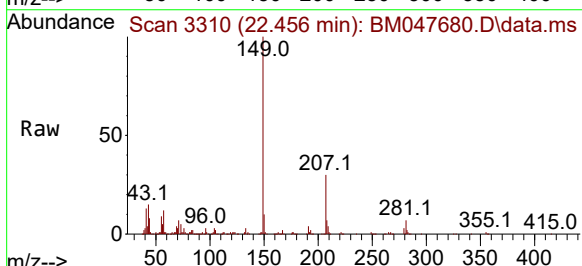




#90
Benzo(b)fluoranthene
Concen: 10.076 ng/ul
RT: 23.462 min Scan# 3481
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55




Instrument :
BNA_M
ClientSampleId :
SSTD010021


Tgt Ion:252 Resp: 374805
Ion Ratio Lower Upper
252 100
253 20.8 17.4 26.2
125 11.0 9.0 13.4

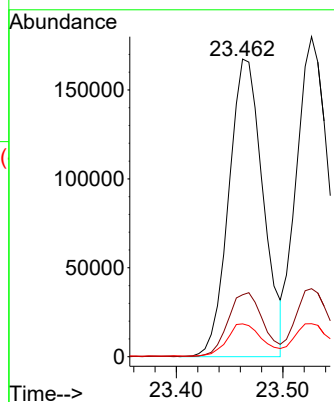

#91
Benzo(k)fluoranthene
Concen: 10.505 ng/ul
RT: 23.527 min Scan# 3492
Delta R.T. -0.000 min
Lab File: BM047680.D
Acq: 27 Sep 2024 18:55

Tgt Ion:252 Resp: 383812
Ion Ratio Lower Upper
252 100
253 21.3 17.5 26.3
125 10.3 8.9 13.3

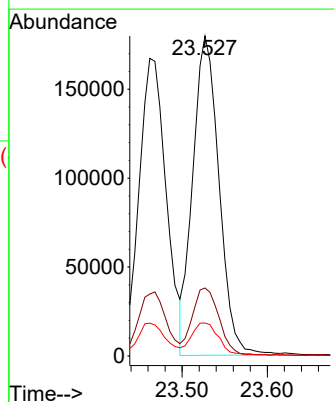



#93

Benzo(a)pyrene

Concen: 10.353 ng/ul

RT: 24.274 min Scan# 3

Delta R.T. -0.000 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55

Instrument :

BNA_M

ClientSampleId :

SSTD010021





Tgt Ion:252 Resp: 353798

Ion Ratio Lower Upper

252 100

253 21.3 17.2 25.8

125 11.7 10.1 15.1

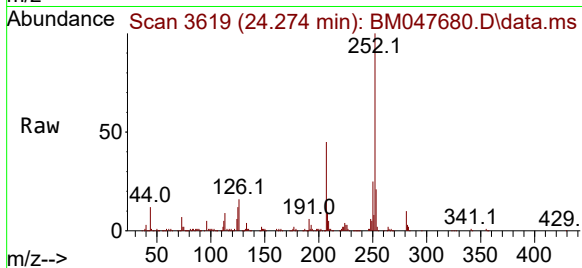

#94

Indeno(1,2,3-cd)pyrene

Concen: 10.920 ng/ul

RT: 27.803 min Scan# 4219

Delta R.T. -0.006 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55




Tgt Ion:276 Resp: 457650


Ion Ratio Lower Upper

276 100

138 21.8 16.9 25.3

277 22.9 18.9 28.3

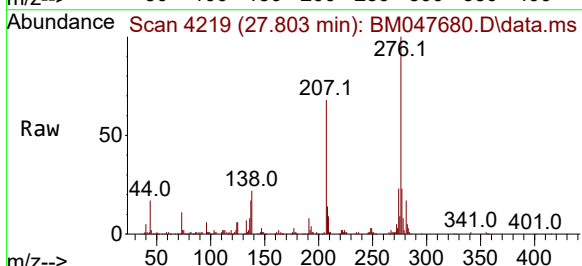



#95

Dibenzo(a,h)anthracene

Concen: 10.856 ng/ul

RT: 27.868 min Scan# 41

Delta R.T. 0.006 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55

Instrument :

BNA_M

ClientSampleId :

SSTD010021





Tgt Ion:278 Resp: 370445

Ion Ratio Lower Upper

278 100

139 16.0 13.4 20.2

279 24.0 18.4 27.6

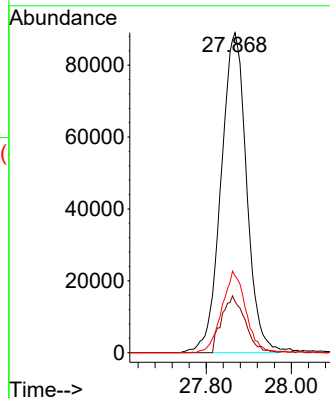

#96

Benzo(g,h,i)perylene

Concen: 11.191 ng/ul

RT: 28.856 min Scan# 4398

Delta R.T. -0.006 min

Lab File: BM047680.D

Acq: 27 Sep 2024 18:55

Tgt Ion:276 Resp: 358270

Ion Ratio Lower Upper

276 100

138 23.8 18.7 28.1

277 22.8 18.3 27.5

