

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092823\
 Data File : BM042119.D
 Acq On : 28 Sep 2023 17:49
 Operator : MA/JU
 Sample : PB155821BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK821

Quant Time: Sep 29 04:40:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 29 04:39:33 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.941	152	3890	0.400	ng/ul	0.00
4) Naphthalene-d8	10.752	136	10341	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.583	164	5096	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.337	188	11613	0.400	ng/ul	0.00
17) Chrysene-d12	21.512	240	6917	0.400	ng/ul	# 0.00
23) Perylene-d12	23.915	264	7725	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.360	96	32049	6.046	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.335	152	4585	0.354	ng/ul	0.00
18) Fluoranthene-d10	19.361	212	8501	0.298	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.577	166	2094	0.071	ng/ul#	14
20) Pyrene	19.729	202	2046	0.027	ng/ul#	1
26) Benzo(a)pyrene	23.763	252	4200	0.086	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092823\
Data File : BM042119.D
Acq On : 28 Sep 2023 17:49
Operator : MA/JU
Sample : PB155821BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK821

Quant Time: Sep 29 04:40:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 29 04:39:33 2023
Response via : Initial Calibration




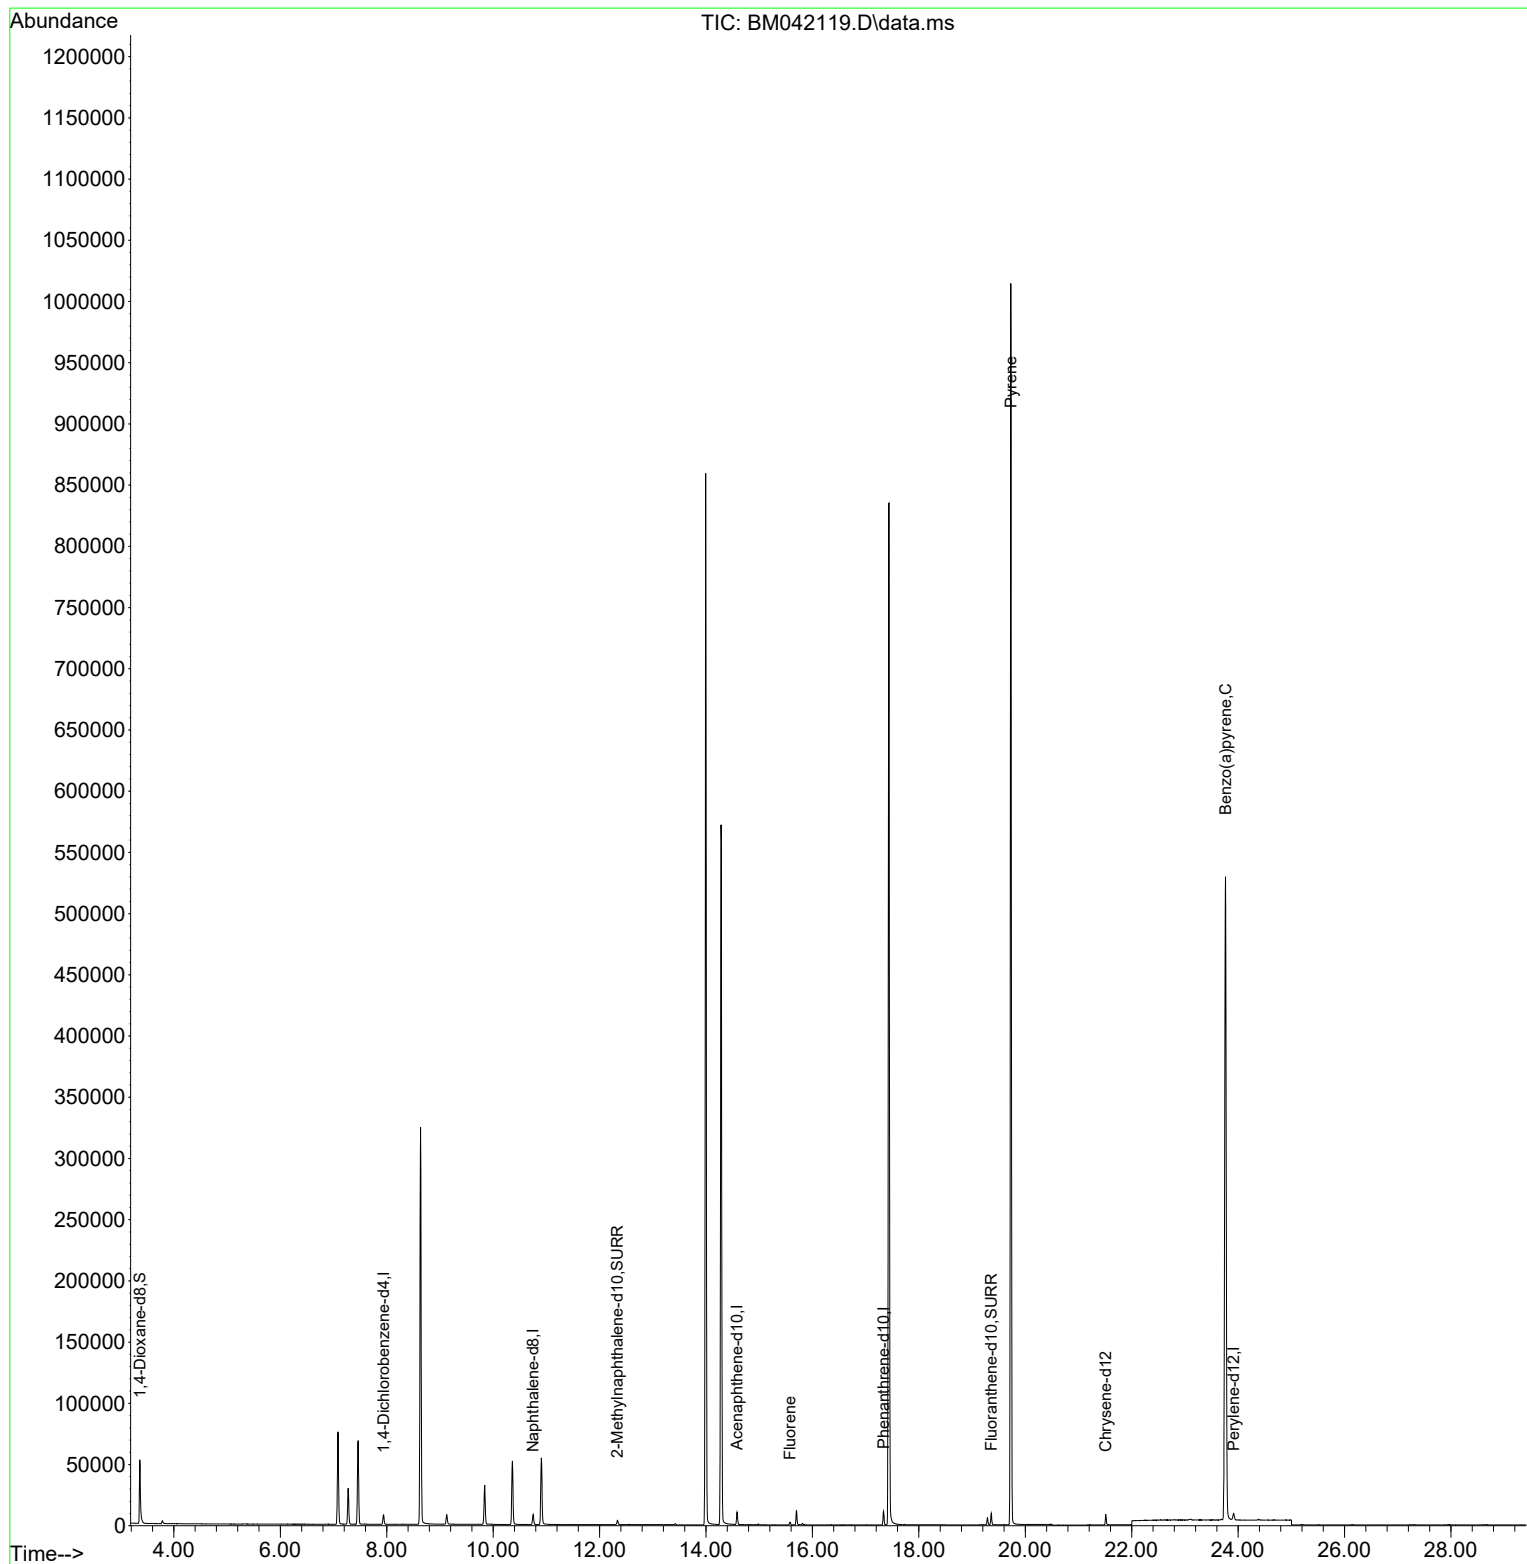


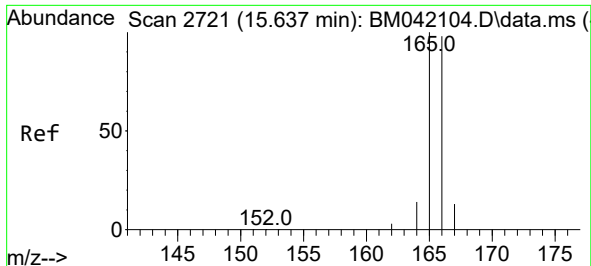

#12
Fluorene
Concen: 0.071 ng/ul
RT: 15.577 min Scan# 21
Delta R.T. -0.060 min
Lab File: BM042119.D
Acq: 28 Sep 2023 17:49




Instrument :
BNA_M
ClientSampleId :
SBLK821


Tgt Ion:166 Resp: 2094
Ion Ratio Lower Upper
166 100
165 8.6 79.8 119.8#
167 32.1 11.1 16.7#

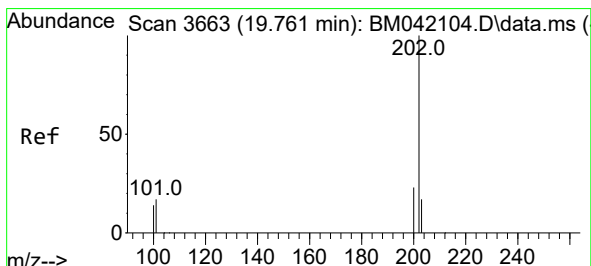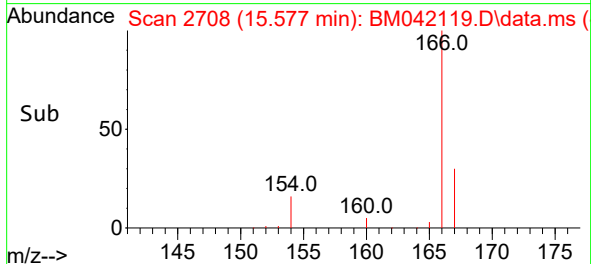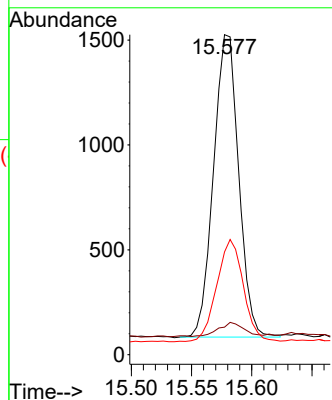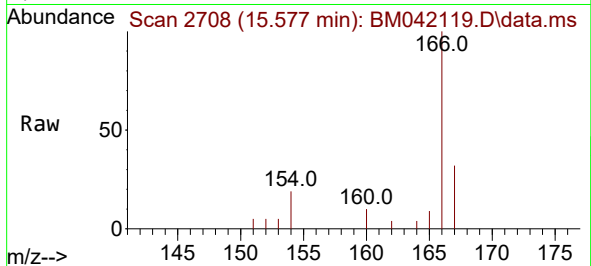

#20
Pyrene
Concen: 0.027 ng/ul
RT: 19.729 min Scan# 3656
Delta R.T. -0.028 min
Lab File: BM042119.D
Acq: 28 Sep 2023 17:49


Tgt Ion:202 Resp: 2046
Ion Ratio Lower Upper
202 100
101 170.0 14.1 21.1#
100 1271.3 11.4 17.0#

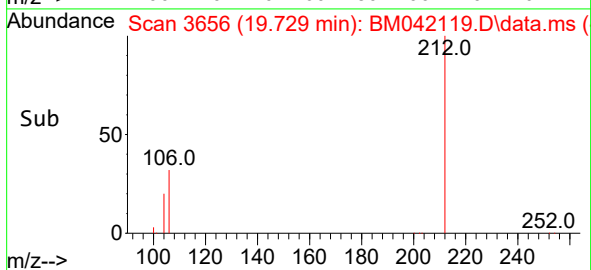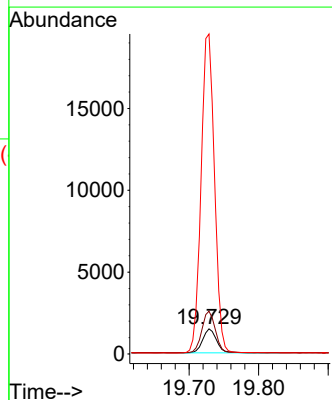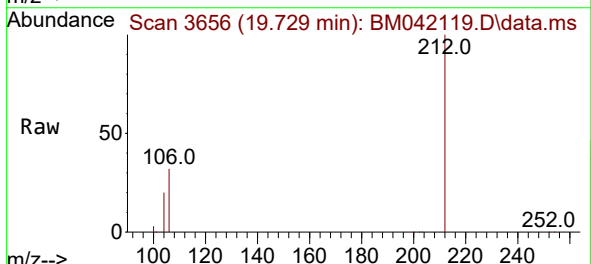

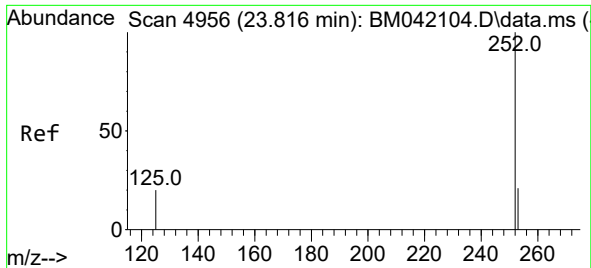

#26
 Benzo(a)pyrene
 Concen: 0.086 ng/ul
 RT: 23.763 min Scan# 4938
 Delta R.T. -0.044 min
 Lab File: BM042119.D
 Acq: 28 Sep 2023 17:49

Instrument :
 BNA_M
 ClientSampleId :
 SBLK821

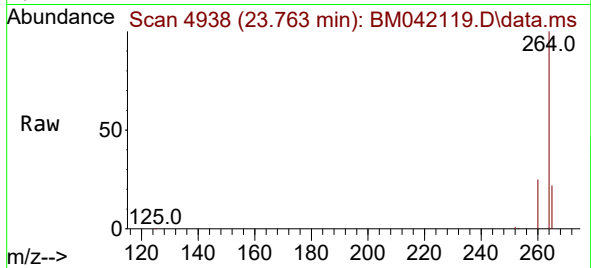

Tgt Ion:252 Resp: 4200
 Ion Ratio Lower Upper
 252 100
 253 50.0 23.2 34.8#
 125 44.6 22.5 33.7#

