

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092823\
 Data File : BM042120.D
 Acq On : 28 Sep 2023 18:26
 Operator : MA/JU
 Sample : PB155824BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK824

Quant Time: Sep 29 04:41:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 29 04:39:33 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.941	152	3010	0.400	ng/ul	0.00
4) Naphthalene-d8	10.752	136	7826	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.583	164	3789	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.337	188	8509	0.400	ng/ul	0.00
17) Chrysene-d12	21.512	240	5303	0.400	ng/ul	0.00
23) Perylene-d12	23.912	264	6467	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.360	96	27218	6.636	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.335	152	3862	0.394	ng/ul	0.00
18) Fluoranthene-d10	19.362	212	7027	0.322	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.577	166	1777	0.081	ng/ul#	15
20) Pyrene	19.729	202	1835	0.031	ng/ul#	1
26) Benzo(a)pyrene	23.760	252	4066	0.099	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092823\
Data File : BM042120.D
Acq On : 28 Sep 2023 18:26
Operator : MA/JU
Sample : PB155824BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK824

Quant Time: Sep 29 04:41:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 29 04:39:33 2023
Response via : Initial Calibration




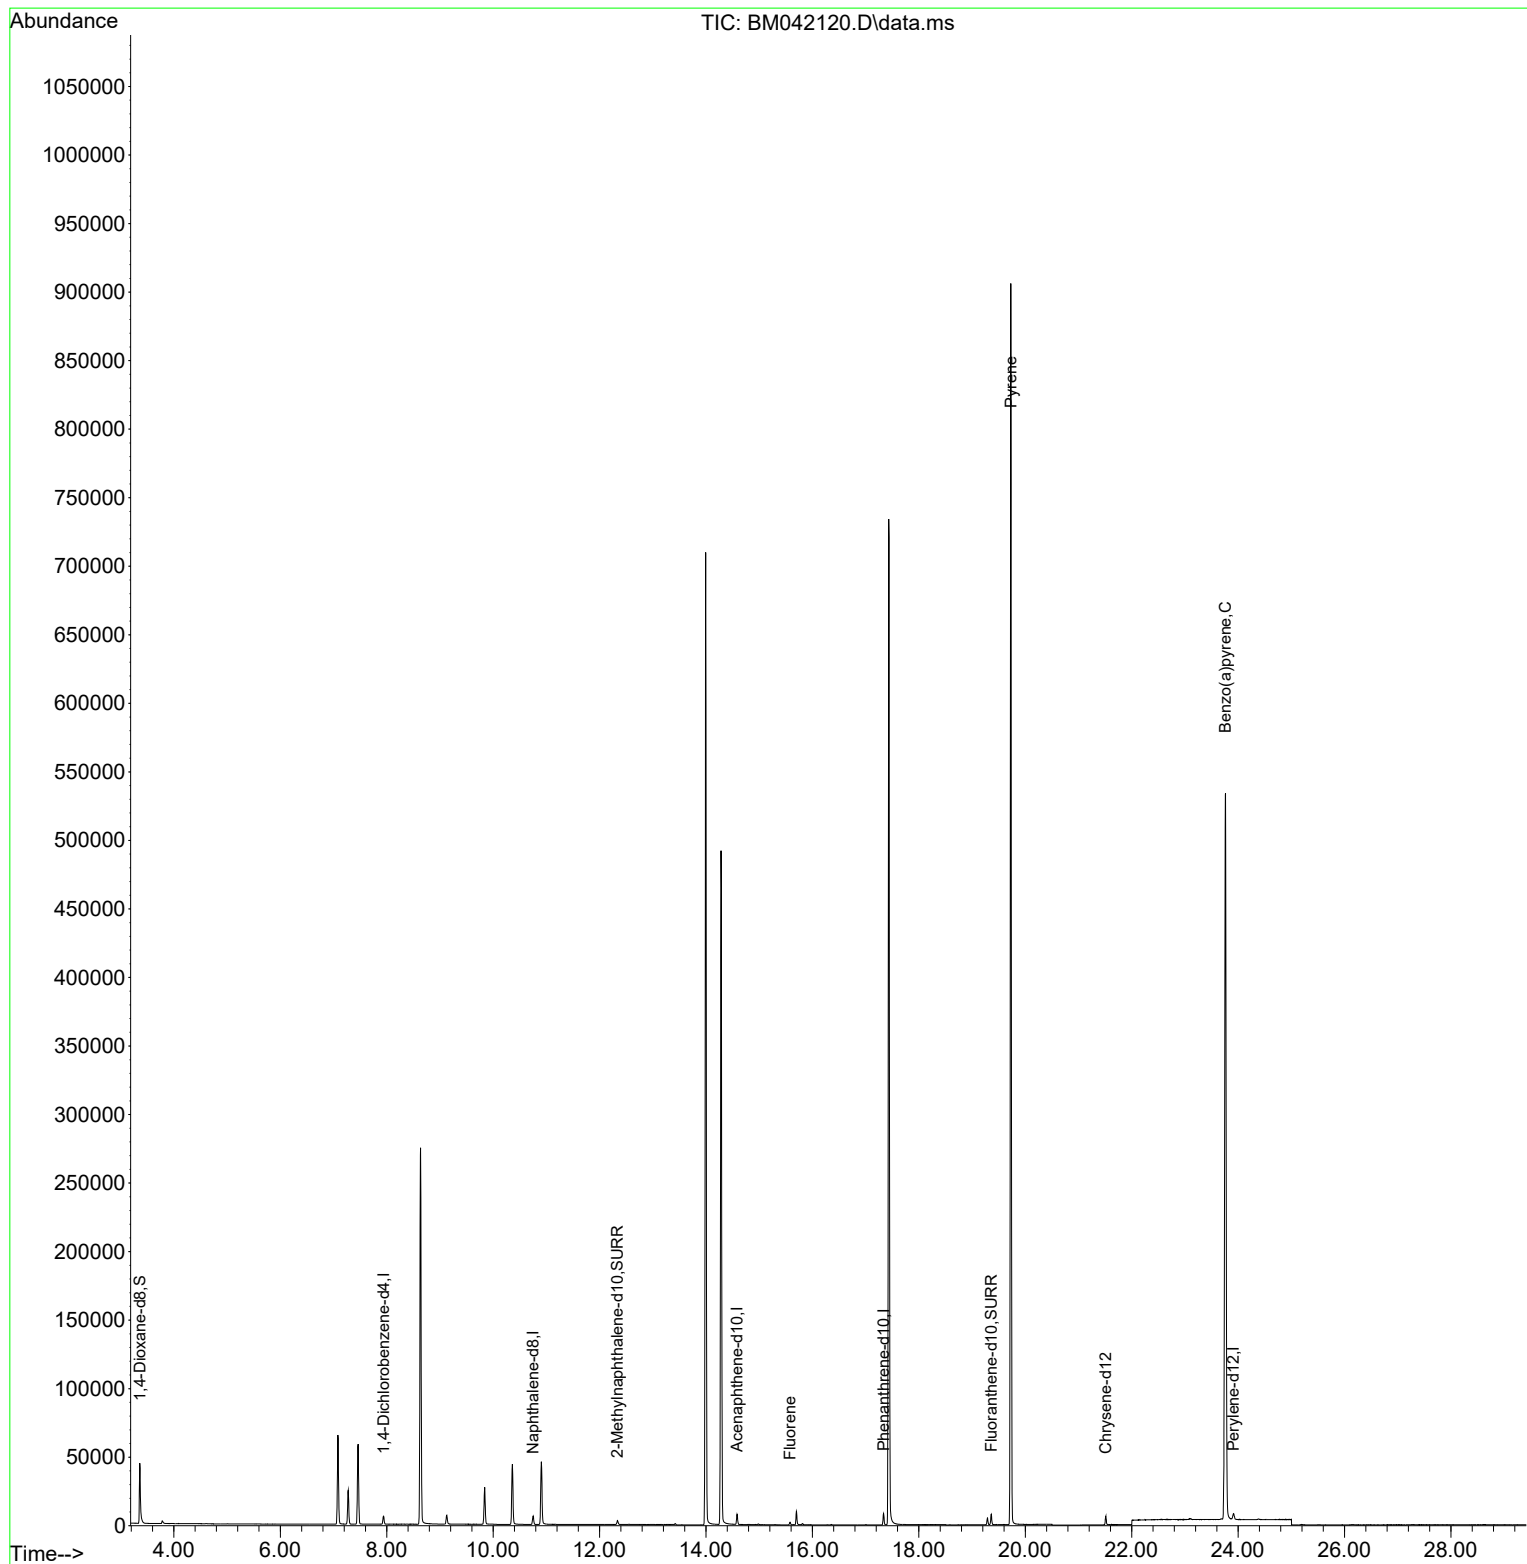


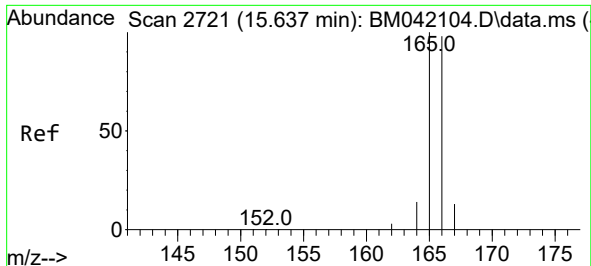

#12
Fluorene
Concen: 0.081 ng/ul
RT: 15.577 min Scan# 21
Delta R.T. -0.060 min
Lab File: BM042120.D
Acq: 28 Sep 2023 18:26




Instrument :
BNA_M
ClientSampleId :
SBLK824


Tgt Ion:166 Resp: 1777
Ion Ratio Lower Upper
166 100
165 9.4 79.8 119.8#
167 32.6 11.1 16.7#

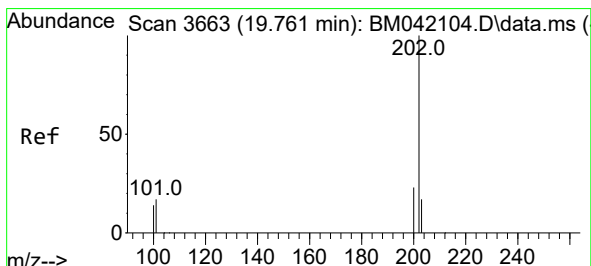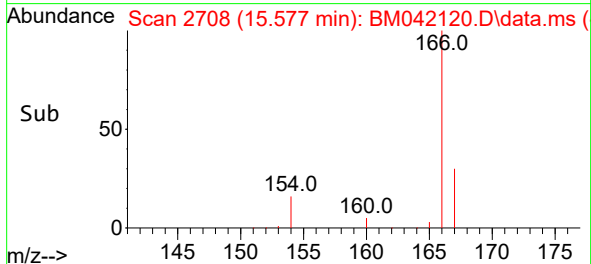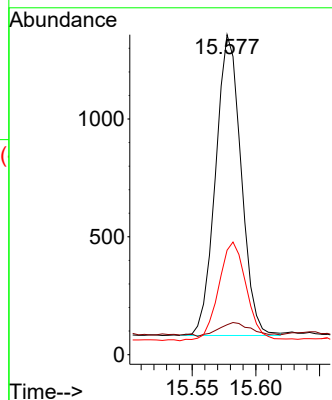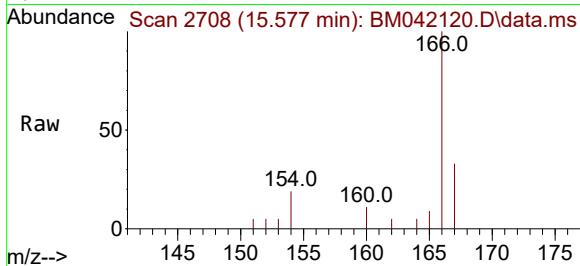

#20
Pyrene
Concen: 0.031 ng/ul
RT: 19.729 min Scan# 3656
Delta R.T. -0.028 min
Lab File: BM042120.D
Acq: 28 Sep 2023 18:26


Tgt Ion:202 Resp: 1835
Ion Ratio Lower Upper
202 100
101 169.6 14.1 21.1#
100 1257.0 11.4 17.0#

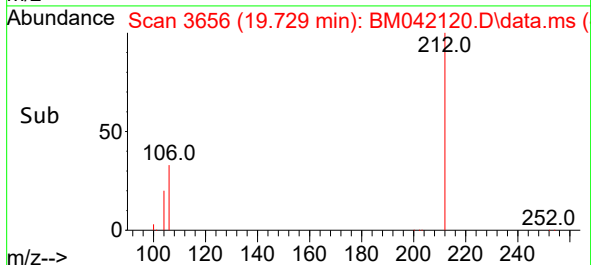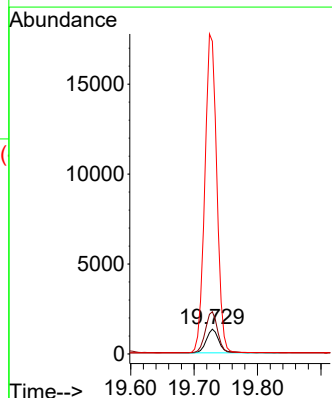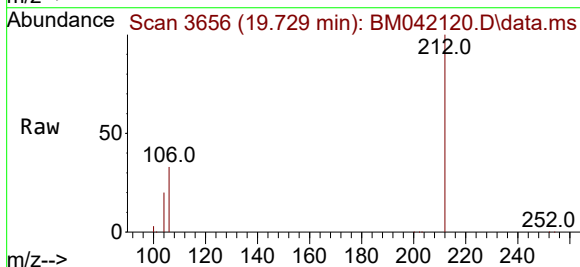

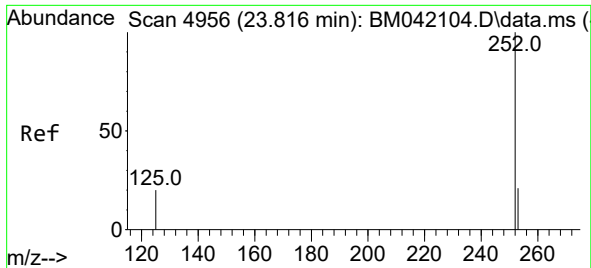

#26
Benzo(a)pyrene
Concen: 0.099 ng/ul
RT: 23.760 min Scan# 49
Delta R.T. -0.047 min
Lab File: BM042120.D
Acq: 28 Sep 2023 18:26

Instrument :
BNA_M
ClientSampleId :
SBLK824

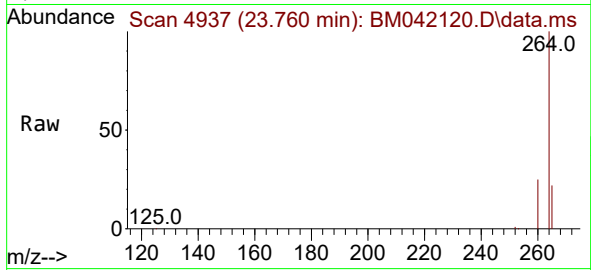

Tgt Ion:252 Resp: 4066
Ion Ratio Lower Upper
252 100
253 48.6 23.2 34.8#
125 44.3 22.5 33.7#

