

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092823\
 Data File : BM042125.D
 Acq On : 28 Sep 2023 21:27
 Operator : MA/JU
 Sample : 04480-14
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBBN4

Quant Time: Sep 29 04:41:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 29 04:39:33 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.937	152	3942	0.400	ng/ul	0.00
4) Naphthalene-d8	10.752	136	10635	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.583	164	5471	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.337	188	13435	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.512	240	8659	0.400	ng/ul	0.00
23) Perylene-d12	23.915	264	9730	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.360	96	19635	3.655	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.335	152	5364	0.403	ng/ul	0.00
18) Fluoranthene-d10	19.362	212	12649	0.355	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.398	88	1188	0.210	ng/ul#	74
5) Naphthalene	10.801	128	773	0.022	ng/ul#	54

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Sep 29 04:41:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 29 04:39:33 2023
Response via : Initial Calibration







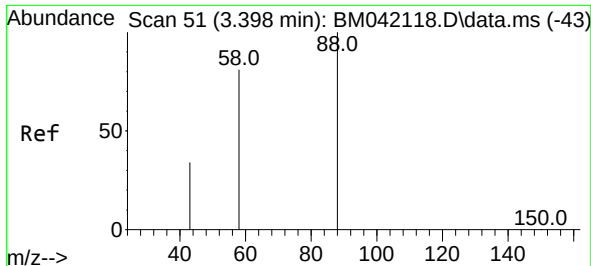

#2
 1,4-Dioxane
 Concen: 0.210 ng/ul
 RT: 3.398 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: BM042125.D
 Acq: 28 Sep 2023 21:27

Instrument :
 BNA_M
 ClientSampleId :
 BBBN4

Tgt Ion: 88 Resp: 1188
 Ion Ratio Lower Upper
 88 100
 43 95.1 42.9 64.3#
 58 71.4 56.4 84.6

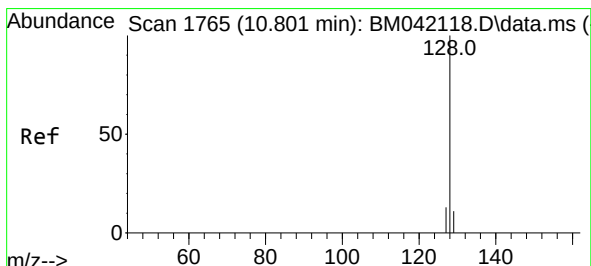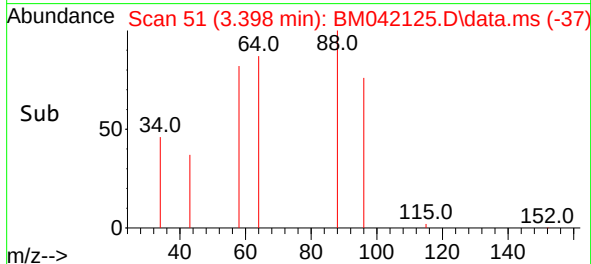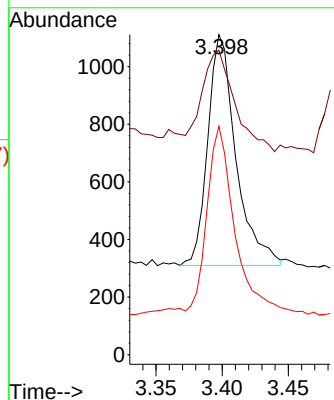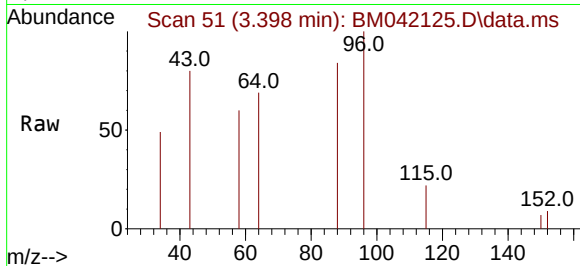

#5
 Naphthalene
 Concen: 0.022 ng/ul
 RT: 10.801 min Scan# 1765
 Delta R.T. -0.000 min
 Lab File: BM042125.D
 Acq: 28 Sep 2023 21:27

Tgt Ion: 128 Resp: 773
 Ion Ratio Lower Upper
 128 100
 129 33.3 9.2 13.8#
 127 28.0 10.8 16.2#

