

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
 Data File : BM047703.D
 Acq On : 28 Sep 2024 22:36
 Operator : RC/JU
 Sample : P3927-02DL 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDC80DL

Quant Time: Sep 29 03:48:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 28 02:30:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	188131	20.000	ng/u1	0.00
20) Naphthalene-d8	10.610	136	738015	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.445	164	447827	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.186	188	946804	20.000	ng/u1	0.00
79) Chrysene-d12	21.409	240	867295	20.000	ng/u1	0.00
88) Perylene-d12	24.409	264	998860	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.257	96	1851	0.318	ng/uL	0.00
4) Pyridine-d5	3.687	84	25216	1.479	ng/u1	0.01
7) Phenol-d5	6.975	99	25043	1.408	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.145	67	19222	1.523	ng/u1	0.00
11) 2-Chlorophenol-d4	7.345	132	20004	1.546	ng/u1	0.00
15) 4-Methylphenol-d8	8.516	113	17847	1.349	ng/u1	0.00
21) Nitrobenzene-d5	8.963	128	8281	1.409	ng/u1	0.00
24) 2-Nitrophenol-d4	9.686	143	7156	1.271	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.227	165	15511	1.379	ng/u1	0.00
31) 4-Chloroaniline-d4	10.739	131	24779	1.425	ng/u1	0.00
46) Dimethylphthalate-d6	13.857	166	65446	2.016	ng/u1	0.00
49) Acenaphthylene-d8	14.139	160	66415	1.725	ng/u1	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/u1	0.00
60) Fluorene-d10	15.433	176	55345	1.968	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/u1	0.00
73) Anthracene-d10	17.280	188	85283	1.832	ng/u1	0.00
81) Pyrene-d10	19.568	212	97907	1.989	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.203	264	91465	1.765	ng/u1	0.00
Target Compounds						
					Qvalue	
58) 2,3,4,6-Tetrachlorophenol	15.074	232	10036	1.380	ng/u1#	93
71) Pentachlorophenol	16.833	266	397617	55.057	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
Data File : BM047703.D
Acq On : 28 Sep 2024 22:36
Operator : RC/JU
Sample : P3927-02DL 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDC80DL

Quant Time: Sep 29 03:48:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 28 02:30:36 2024
Response via : Initial Calibration




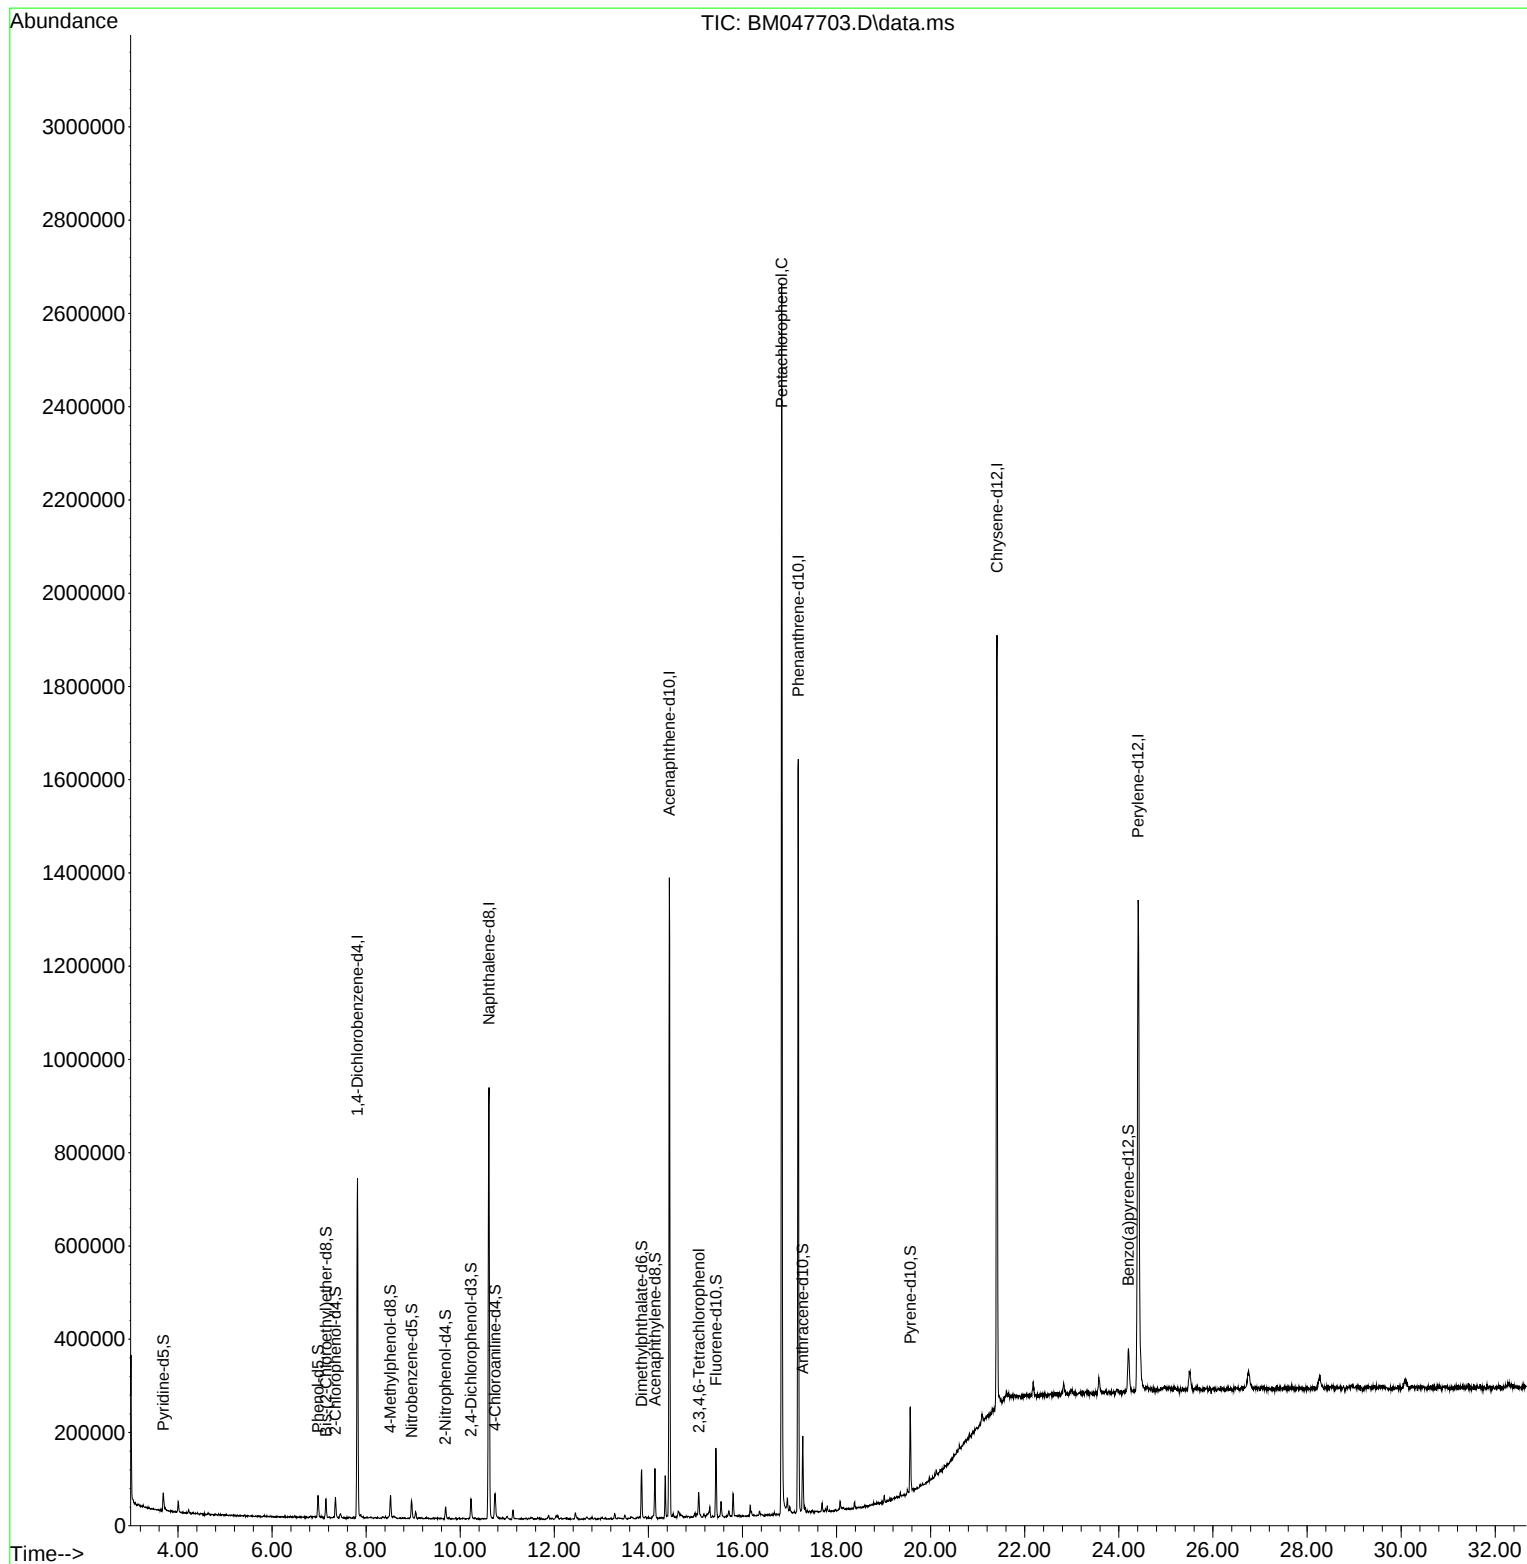


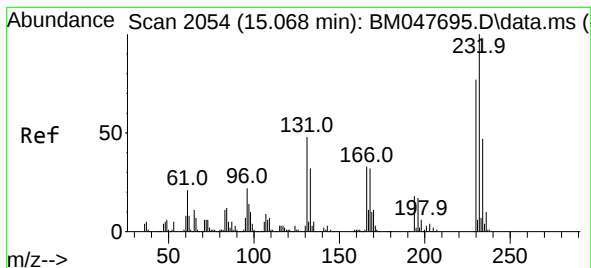

#58
2,3,4,6-Tetrachlorophenol
Concen: 1.380 ng/ul
RT: 15.074 min Scan# 2055
Delta R.T. 0.006 min
Lab File: BM047703.D
Acq: 28 Sep 2024 22:36

Instrument :
BNA_M
ClientSampleId :
DDC80DL

Tgt Ion:	232	Resp:	10036
Ion Ratio	Lower	Upper	
232	100		
131	48.7	40.2	60.4
130	3.2	2.6	4.0
166	23.5	25.3	37.9

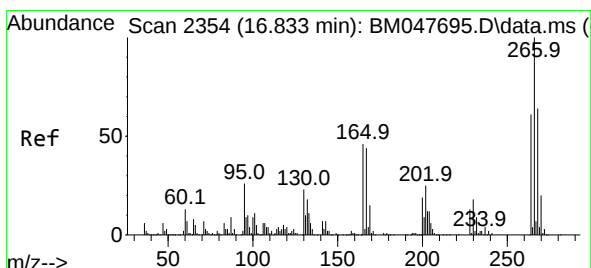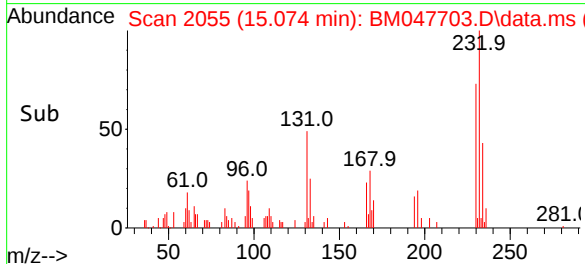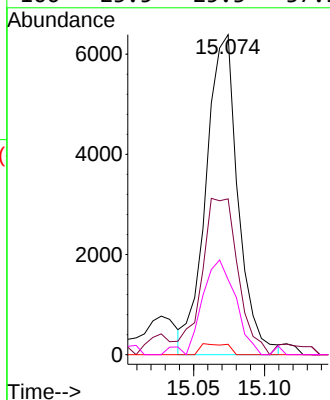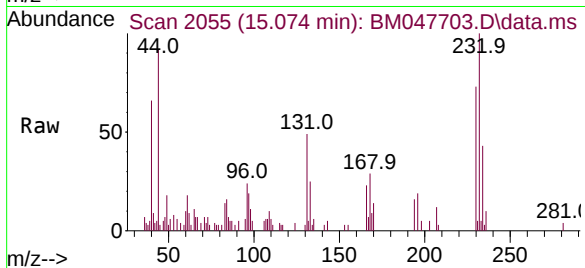

#71
Pentachlorophenol
Concen: 55.057 ng/ul
RT: 16.833 min Scan# 2354
Delta R.T. -0.006 min
Lab File: BM047703.D
Acq: 28 Sep 2024 22:36

Tgt Ion:	266	Resp:	397617
Ion Ratio	Lower	Upper	
266	100		
264	63.0	50.2	75.2
268	62.6	50.9	76.3

