

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
 Data File : BM047705.D
 Acq On : 28 Sep 2024 23:56
 Operator : RC/JU
 Sample : P3927-16DL 2X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCA4DL

Quant Time: Sep 29 03:17:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 28 02:30:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	193397	20.000	ng/u1	0.00
20) Naphthalene-d8	10.610	136	780929	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.445	164	461242	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.186	188	945976	20.000	ng/u1	0.00
79) Chrysene-d12	21.409	240	845114	20.000	ng/u1	0.00
88) Perylene-d12	24.415	264	970875	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	8782	1.467	ng/uL	0.00
4) Pyridine-d5	3.675	84	124561	7.109	ng/u1	0.00
7) Phenol-d5	6.975	99	138719	7.585	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	100902	7.775	ng/u1	0.00
11) 2-Chlorophenol-d4	7.346	132	108025	8.119	ng/u1	0.00
15) 4-Methylphenol-d8	8.516	113	104087	7.655	ng/u1	0.00
21) Nitrobenzene-d5	8.969	128	48186	7.750	ng/u1	0.00
24) 2-Nitrophenol-d4	9.687	143	43133	7.239	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	93979	7.895	ng/u1	0.00
31) 4-Chloroaniline-d4	10.739	131	141839	7.708	ng/u1	0.00
46) Dimethylphthalate-d6	13.857	166	328156	9.813	ng/u1	0.00
49) Acenaphthylene-d8	14.139	160	357449	9.015	ng/u1	0.00
54) 4-Nitrophenol-d4	14.633	143	36315	5.454	ng/u1	0.00
60) Fluorene-d10	15.439	176	277181	9.569	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.545	200	25923	4.683	ng/u1	0.00
73) Anthracene-d10	17.280	188	428761	9.218	ng/u1	0.00
81) Pyrene-d10	19.568	212	499430	10.413	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.203	264	487147	9.671	ng/u1	0.00
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.833	266	579580	80.323	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
Data File : BM047705.D
Acq On : 28 Sep 2024 23:56
Operator : RC/JU
Sample : P3927-16DL 2X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCA4DL

Quant Time: Sep 29 03:17:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 28 02:30:36 2024
Response via : Initial Calibration

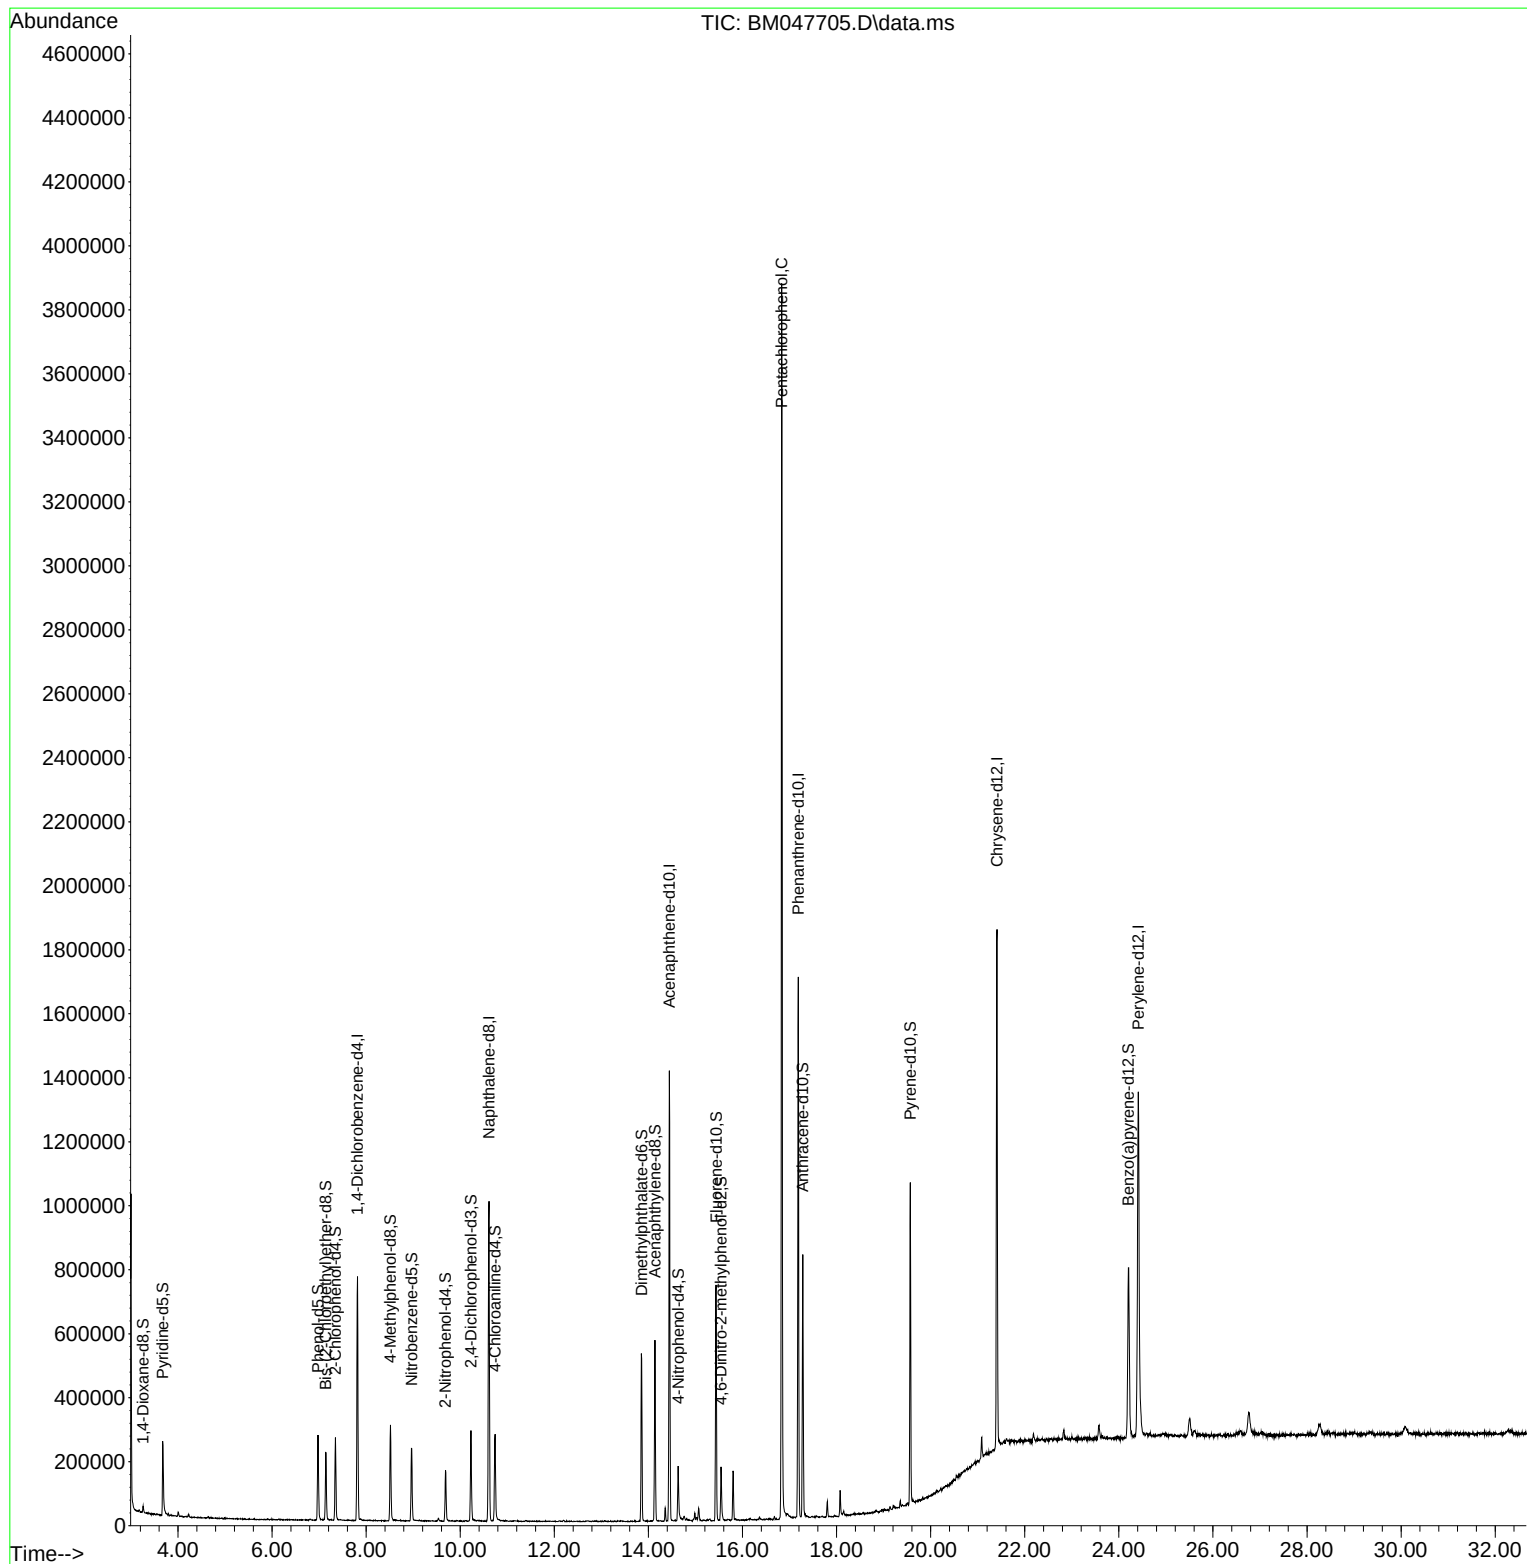

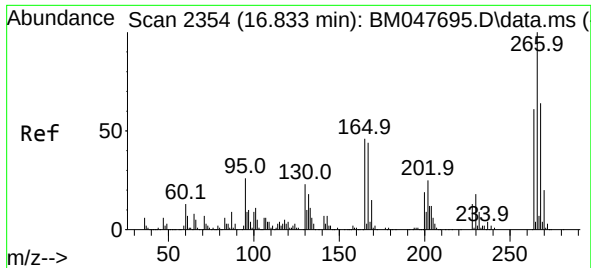

#71
 Pentachlorophenol
 Concen: 80.323 ng/ul
 RT: 16.833 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BM047705.D
 Acq: 28 Sep 2024 23:56

Instrument :
 BNA_M
 ClientSampleId :
 DDCA4DL

Tgt Ion:266 Resp: 579580
 Ion Ratio Lower Upper
 266 100
 264 63.2 50.2 75.2
 268 63.0 50.9 76.3

