

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
 Data File : BM047706.D
 Acq On : 29 Sep 2024 00:36
 Operator : RC/JU
 Sample : P3927-03DL 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDC81DL

Quant Time: Sep 29 03:51:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 28 02:30:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	216159	20.000	ng/u1	0.00
20) Naphthalene-d8	10.610	136	915754	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.451	164	542565	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.186	188	1142802	20.000	ng/u1	0.00
79) Chrysene-d12	21.409	240	1054679	20.000	ng/u1	0.00
88) Perylene-d12	24.415	264	1202292	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.263	96	2035	0.304	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	6.981	99	31083	1.521	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	24916	1.718	ng/u1	0.00
11) 2-Chlorophenol-d4	7.351	132	24501	1.648	ng/u1	0.00
15) 4-Methylphenol-d8	8.516	113	24024	1.581	ng/u1	0.00
21) Nitrobenzene-d5	8.963	128	9536	1.308	ng/u1	0.00
24) 2-Nitrophenol-d4	9.692	143	8972	1.284	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	20596	1.476	ng/u1	0.00
31) 4-Chloroaniline-d4	10.739	131	25872	1.199	ng/u1	0.00
46) Dimethylphthalate-d6	13.851	166	79073	2.010	ng/u1	0.00
49) Acenaphthylene-d8	14.139	160	83529	1.791	ng/u1	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/u1	
60) Fluorene-d10	15.433	176	68832	2.020	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.545	200	5400	0.807	ng/u1	0.00
73) Anthracene-d10	17.280	188	100869	1.795	ng/u1	0.00
81) Pyrene-d10	19.568	212	120718	2.017	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.203	264	106644	1.710	ng/u1	0.00
Target Compounds						
					Qvalue	
58) 2,3,4,6-Tetrachlorophenol	15.069	232	164087	18.628	ng/u1	100
71) Pentachlorophenol	16.839	266	1604408	184.057	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
Data File : BM047706.D
Acq On : 29 Sep 2024 00:36
Operator : RC/JU
Sample : P3927-03DL 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDC81DL

Quant Time: Sep 29 03:51:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 28 02:30:36 2024
Response via : Initial Calibration

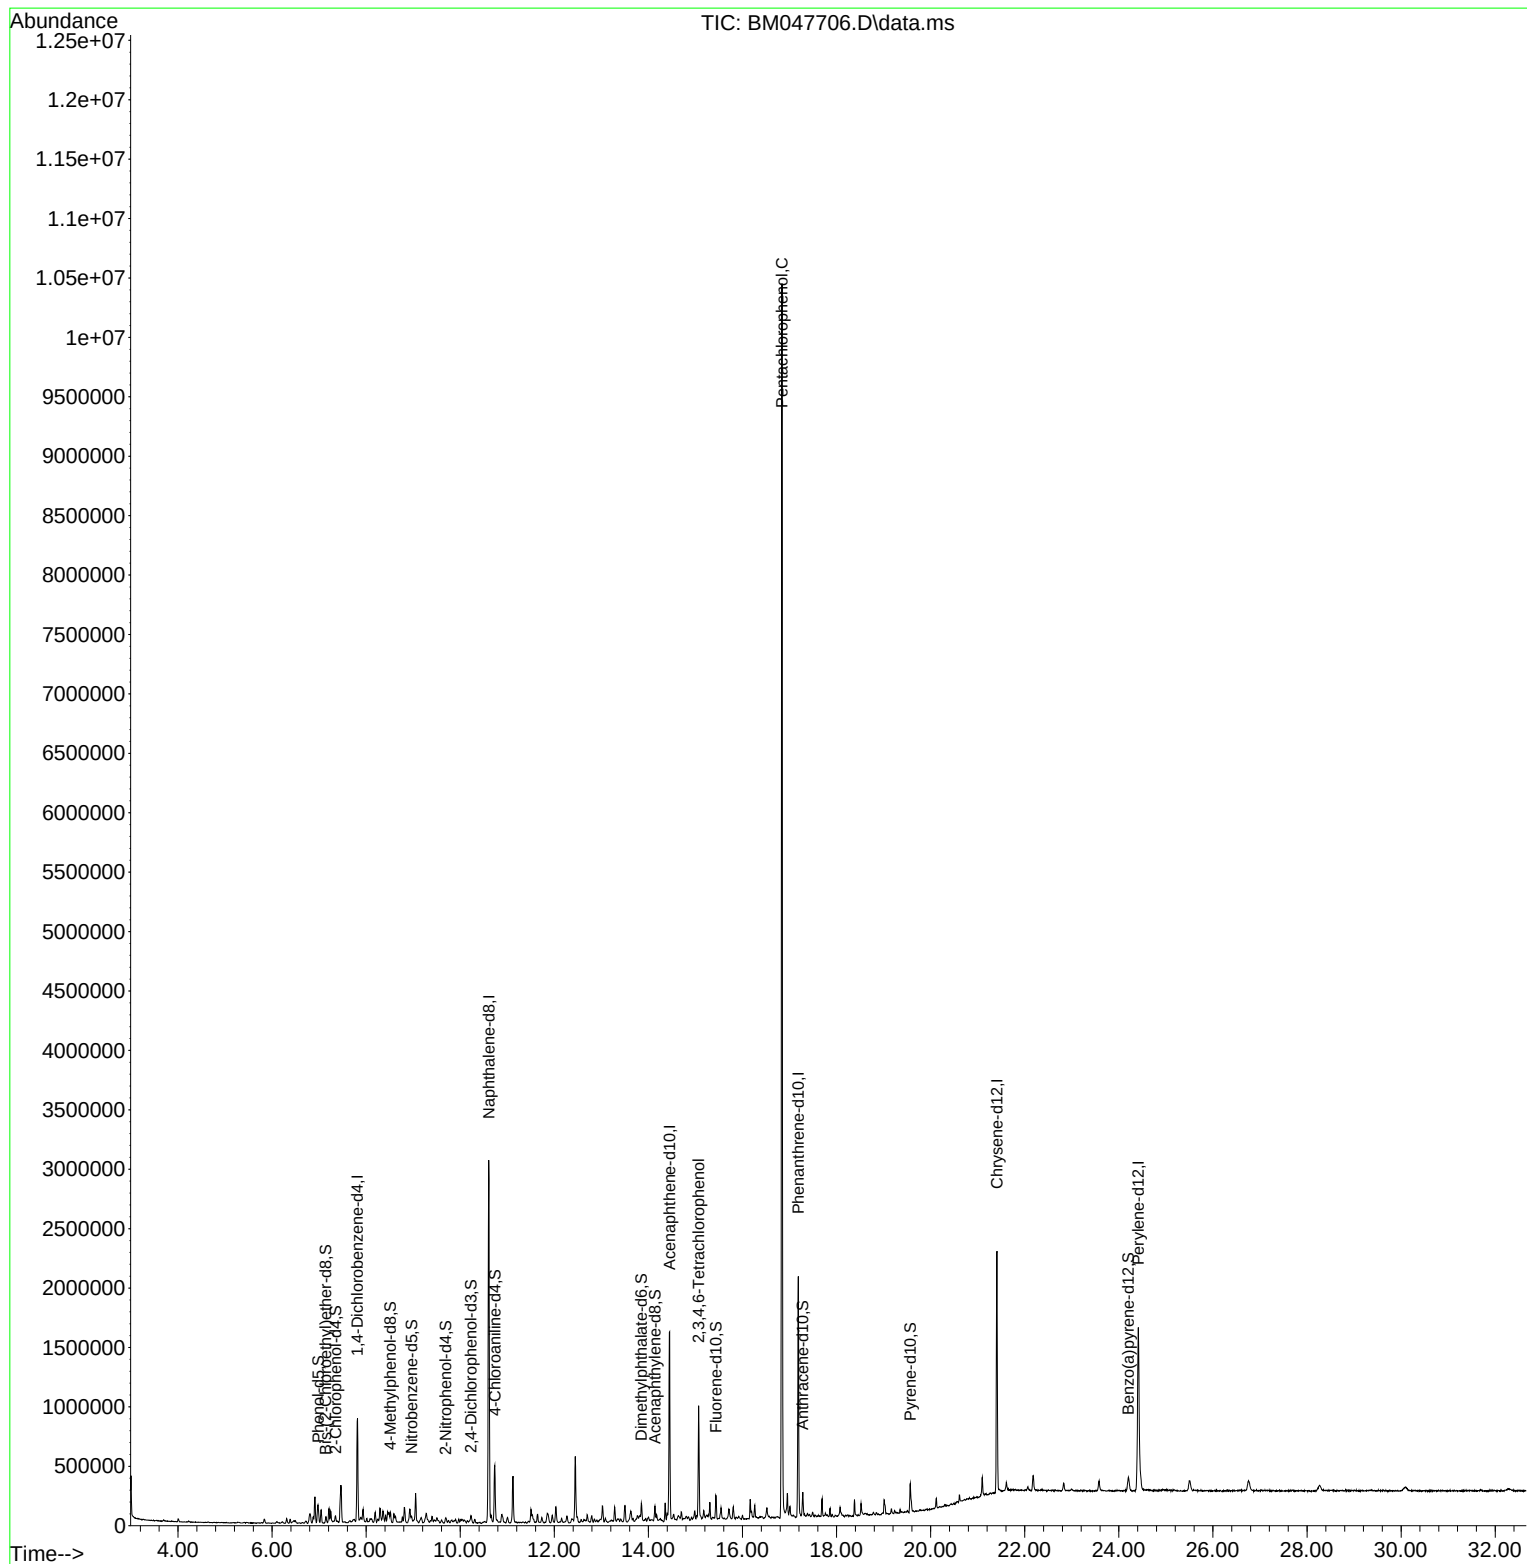




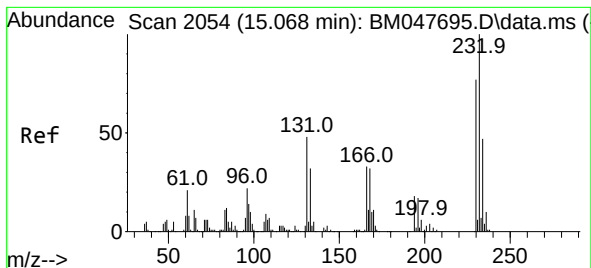


#58
2,3,4,6-Tetrachlorophenol
Concen: 18.628 ng/ul
RT: 15.069 min Scan# 2054
Delta R.T. -0.000 min
Lab File: BM047706.D
Acq: 29 Sep 2024 00:36

Instrument :
BNA_M
ClientSampleId :
DDC81DL

Tgt Ion:232 Resp: 164087

Ion	Ratio	Lower	Upper
232	100		
131	50.4	40.2	60.4
130	2.8	2.6	4.0
166	31.6	25.3	37.9

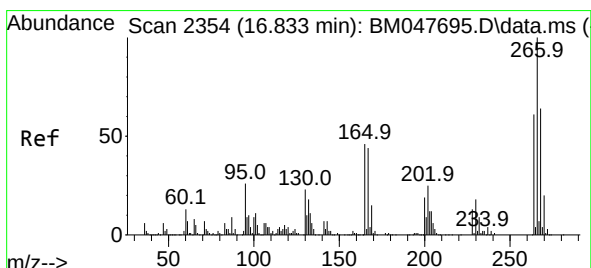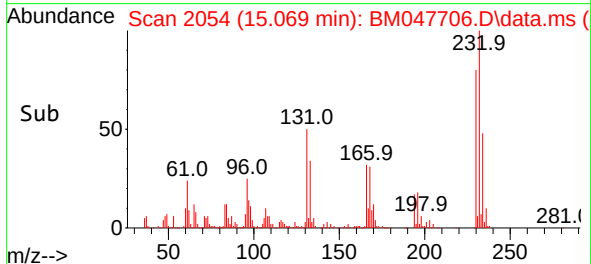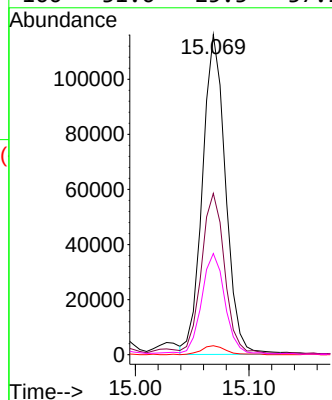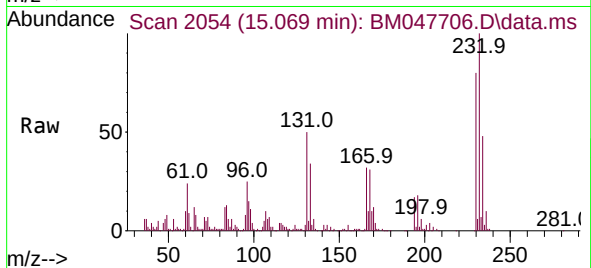

#71
Pentachlorophenol
Concen: 184.057 ng/ul
RT: 16.839 min Scan# 2355
Delta R.T. -0.000 min
Lab File: BM047706.D
Acq: 29 Sep 2024 00:36

Tgt Ion:266 Resp: 1604408

Ion	Ratio	Lower	Upper
266	100		
264	62.5	50.2	75.2
268	64.4	50.9	76.3

