

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
 Data File : BM047707.D
 Acq On : 29 Sep 2024 01:16
 Operator : RC/JU
 Sample : P3927-17DL 30X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDCA5DL

Quant Time: Sep 29 03:53:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 28 02:30:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	187195	20.000	ng/u1	0.00
20) Naphthalene-d8	10.610	136	722453	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.445	164	433884	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.186	188	911777	20.000	ng/u1	0.00
79) Chrysene-d12	21.409	240	818742	20.000	ng/u1	0.00
88) Perylene-d12	24.415	264	935009	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	6.981	99	11171	0.631	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	9602	0.764	ng/u1	0.00
11) 2-Chlorophenol-d4	7.345	132	8425	0.654	ng/u1	0.00
15) 4-Methylphenol-d8	8.516	113	7596	0.577	ng/u1	0.00
21) Nitrobenzene-d5	8.963	128	3666	0.637	ng/u1	0.00
24) 2-Nitrophenol-d4	9.692	143	3122	0.566	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	6579	0.597	ng/u1	0.00
31) 4-Chloroaniline-d4	10.745	131	10210	0.600	ng/u1	0.00
46) Dimethylphthalate-d6	13.857	166	29762	0.946	ng/u1	0.00
49) Acenaphthylene-d8	14.139	160	32666	0.876	ng/u1	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/u1	
60) Fluorene-d10	15.433	176	24999	0.917	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/u1	
73) Anthracene-d10	17.280	188	38863	0.867	ng/u1	0.00
81) Pyrene-d10	19.562	212	44341	0.954	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.209	264	40907	0.843	ng/u1	0.00


Target Compounds					Qvalue
71) Pentachlorophenol	16.833	266	528396	75.976 ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
Data File : BM047707.D
Acq On : 29 Sep 2024 01:16
Operator : RC/JU
Sample : P3927-17DL 30X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDCA5DL

Quant Time: Sep 29 03:53:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 28 02:30:36 2024
Response via : Initial Calibration

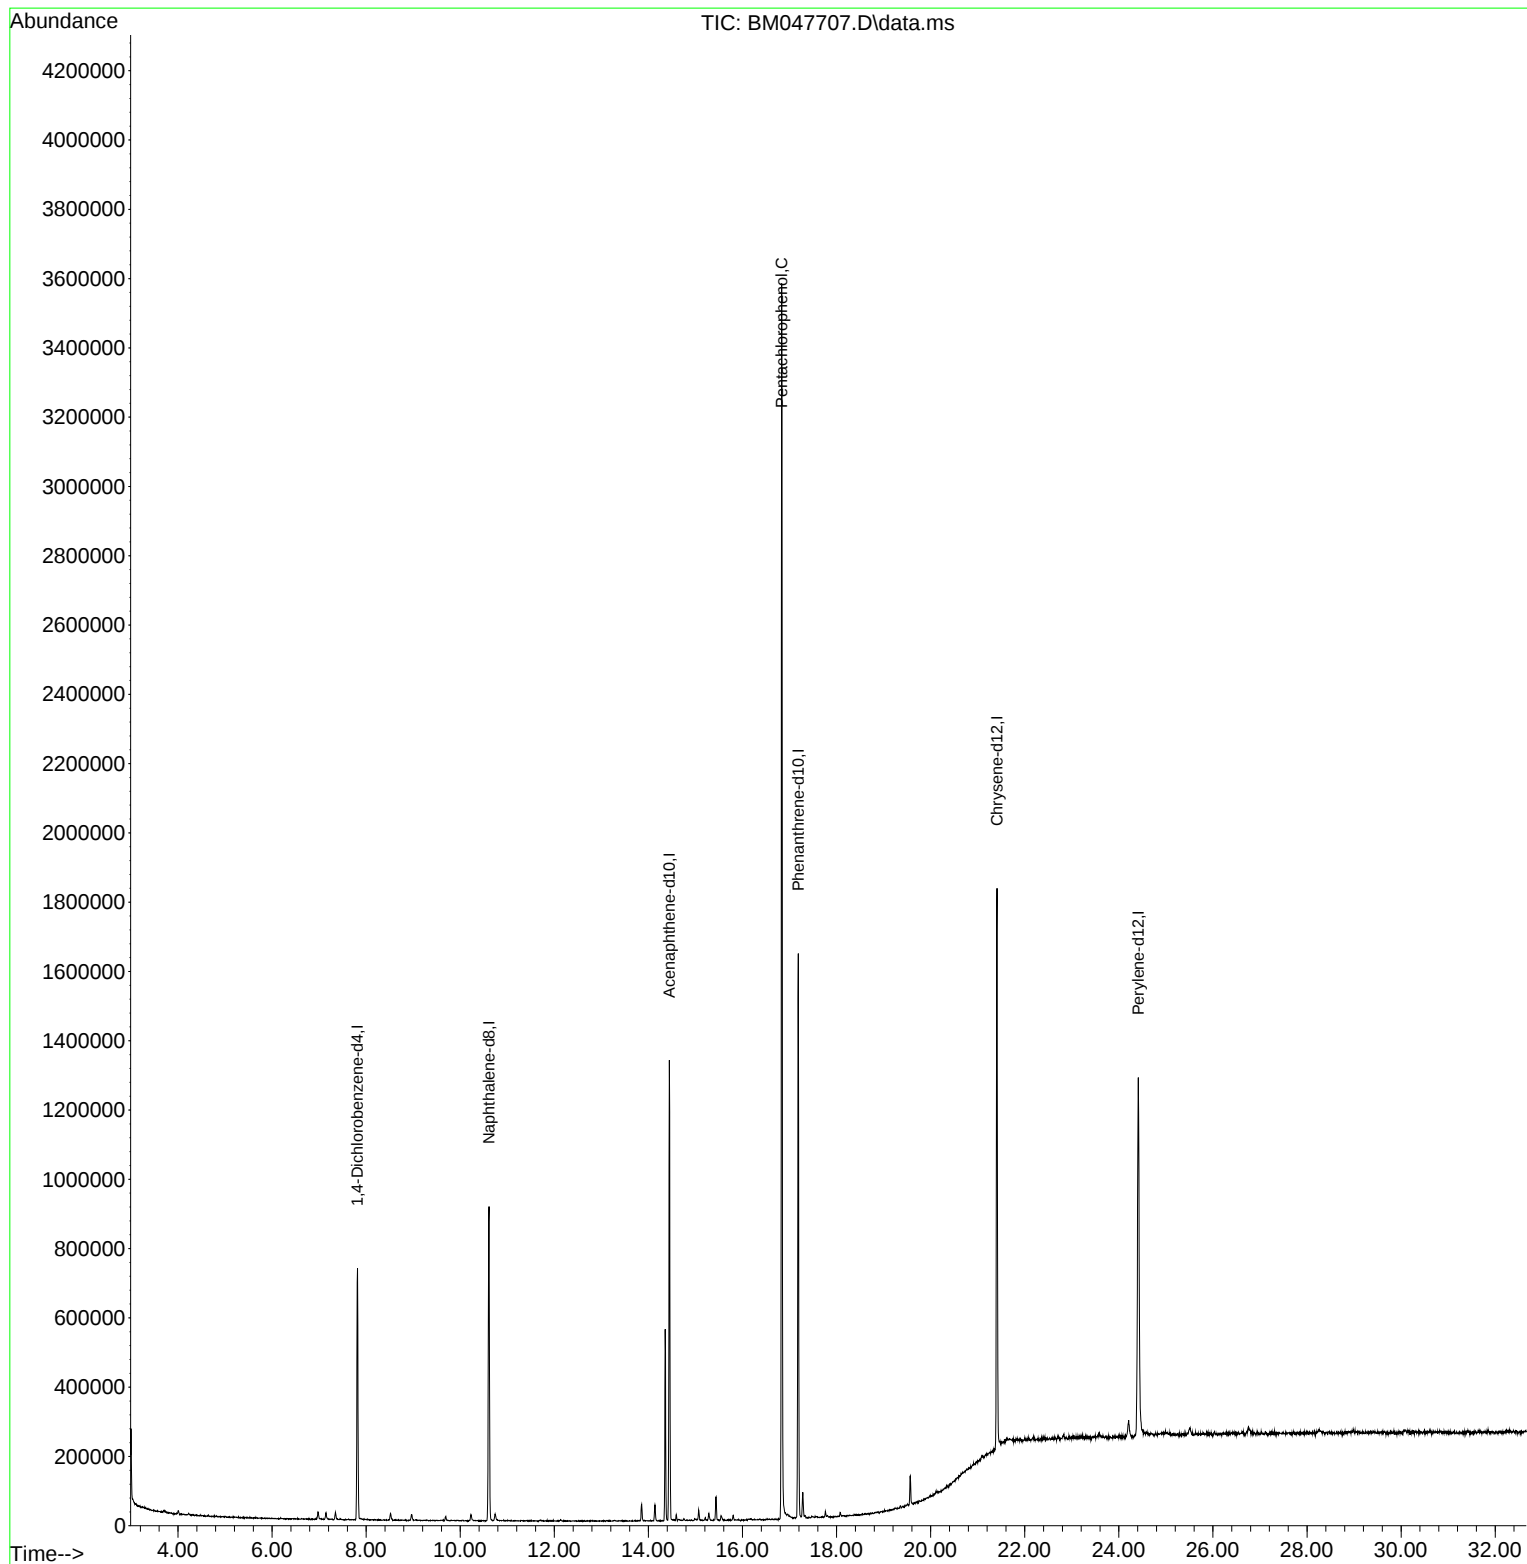

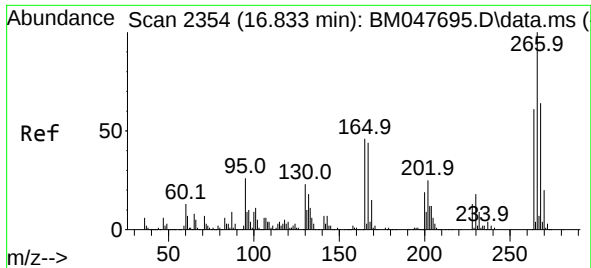

#71
 Pentachlorophenol
 Concen: 75.976 ng/ul
 RT: 16.833 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BM047707.D
 Acq: 29 Sep 2024 01:16

Instrument :
 BNA_M
 ClientSampleId :
 DDCA5DL

Tgt Ion:266 Resp: 528396
 Ion Ratio Lower Upper
 266 100
 264 63.1 50.2 75.2
 268 64.7 50.9 76.3

