

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
 Data File : BM047688.D
 Acq On : 28 Sep 2024 12:44
 Operator : RC/JU
 Sample : PB163765BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK765

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047688.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.257	42	46	54	rVB	86517	111368	2.74%	0.228%
2	3.669	112	116	134	rBV	995359	1501778	36.96%	3.081%
3	4.010	168	174	182	rBV3	21916	34362	0.85%	0.070%
4	4.228	209	211	216	rVB4	8338	12118	0.30%	0.025%
5	4.640	278	281	288	rVB7	5972	9575	0.24%	0.020%
6	5.175	367	372	375	rBV5	2748	5112	0.13%	0.010%
7	6.798	646	648	657	rVB8	3712	7069	0.17%	0.015%
8	6.975	671	678	687	rBV	1032391	1592232	39.19%	3.266%
9	7.145	699	707	716	rVV	842895	1295573	31.88%	2.658%
10	7.345	734	741	752	rBV	995800	1542962	37.97%	3.165%
11	7.816	814	821	829	rBV	789231	1240775	30.54%	2.545%
12	8.516	932	940	956	rBV	1129893	1808066	44.50%	3.709%
13	8.969	1009	1017	1030	rBV	895704	1509509	37.15%	3.097%
14	9.069	1030	1034	1042	rVV5	4502	9797	0.24%	0.020%
15	9.139	1042	1046	1051	rVB4	3118	4880	0.12%	0.010%
16	9.686	1131	1139	1149	rBV	664558	1126574	27.73%	2.311%
17	10.228	1224	1231	1243	rBV	1021211	1695239	41.72%	3.478%
18	10.610	1289	1296	1308	rBV	983873	1656368	40.76%	3.398%
19	10.739	1310	1318	1332	rBV	1089060	1853001	45.60%	3.801%
20	12.198	1561	1566	1571	rBV3	13743	24486	0.60%	0.050%
21	13.433	1770	1776	1778	rBV3	4997	6864	0.17%	0.014%
22	13.857	1841	1848	1858	rBV	1741922	2376595	58.49%	4.876%
23	14.139	1889	1896	1908	rBV	1935195	2803212	68.99%	5.751%
24	14.445	1940	1948	1957	rBV	1349219	1983394	48.81%	4.069%
25	14.633	1973	1980	1994	rBV	794934	1239394	30.50%	2.543%
26	14.851	2014	2017	2022	rVB6	5008	6426	0.16%	0.013%
27	15.268	2083	2088	2093	rBV5	5083	7100	0.17%	0.015%
28	15.439	2109	2117	2124	rBV	2471511	3387654	83.37%	6.950%
29	15.486	2124	2125	2129	rVV4	6402	6693	0.16%	0.014%
30	15.545	2129	2135	2147	rVV	769744	1032210	25.40%	2.118%
31	15.680	2154	2158	2167	rVB5	8646	16173	0.40%	0.033%
32	16.221	2247	2250	2255	rVB5	6457	6803	0.17%	0.014%
33	16.833	2350	2354	2357	rBV6	6893	10563	0.26%	0.022%
34	17.186	2407	2414	2424	rBV	1539741	2174090	53.51%	4.460%
35	17.280	2424	2430	2447	rVV	2537916	3556485	87.53%	7.296%
36	18.080	2561	2566	2569	rBV6	8033	14535	0.36%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
Data File : BM047688.D
Acq On : 28 Sep 2024 12:44
Operator : RC/JU
Sample : PB163765BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK765

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Title : SVOA CALIBRATION

37	19.133	2742	2745	2751	rVB4	23313	33757	0.83%	0.069%
38	19.209	2754	2758	2761	rVB	19001	24783	0.61%	0.051%
39	19.268	2766	2768	2772	rVB5	7097	8856	0.22%	0.018%
40	19.509	2805	2809	2812	rBV5	30405	38319	0.94%	0.079%
41	19.568	2813	2819	2832	rVV	3217302	4063295	100.00%	8.336%
42	20.550	2983	2986	2989	rBV3	29862	34425	0.85%	0.071%
43	21.409	3126	3132	3141	rBV	1467396	2239040	55.10%	4.593%
44	24.209	3600	3608	3625	rVB2	1665850	3957575	97.40%	8.119%
45	24.415	3635	3643	3661	rVB	947560	2675510	65.85%	5.489%




Sum of corrected areas: 48744595

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
Data File : BM047688.D
Acq On : 28 Sep 2024 12:44
Operator : RC/JU
Sample : PB163765BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK765

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

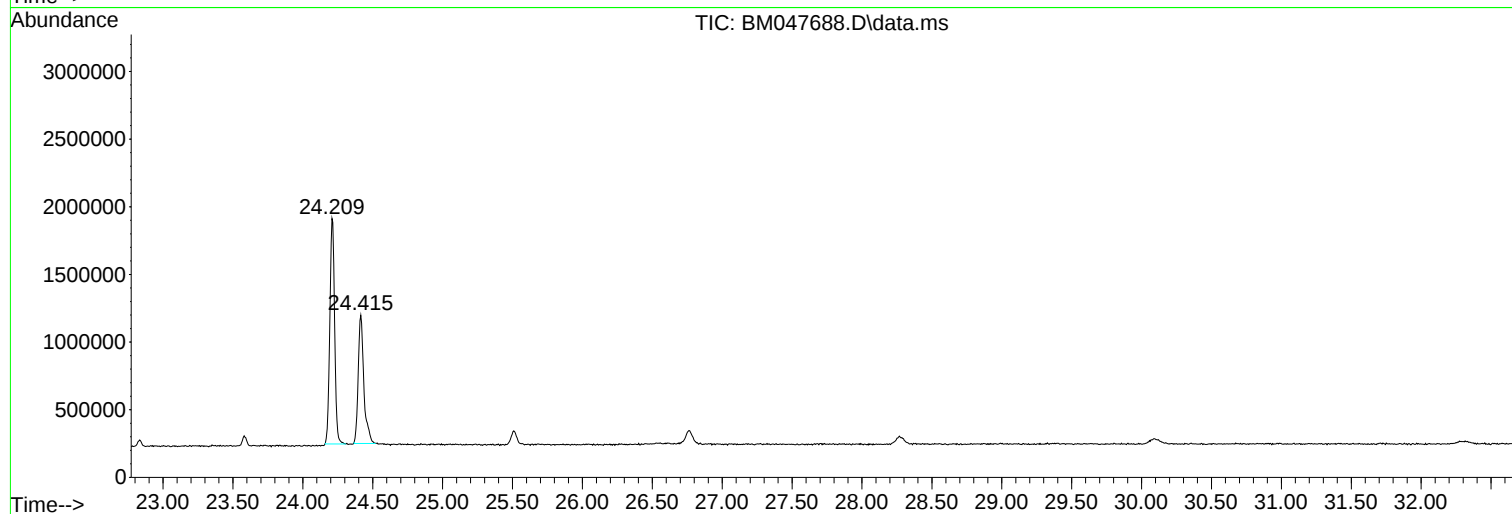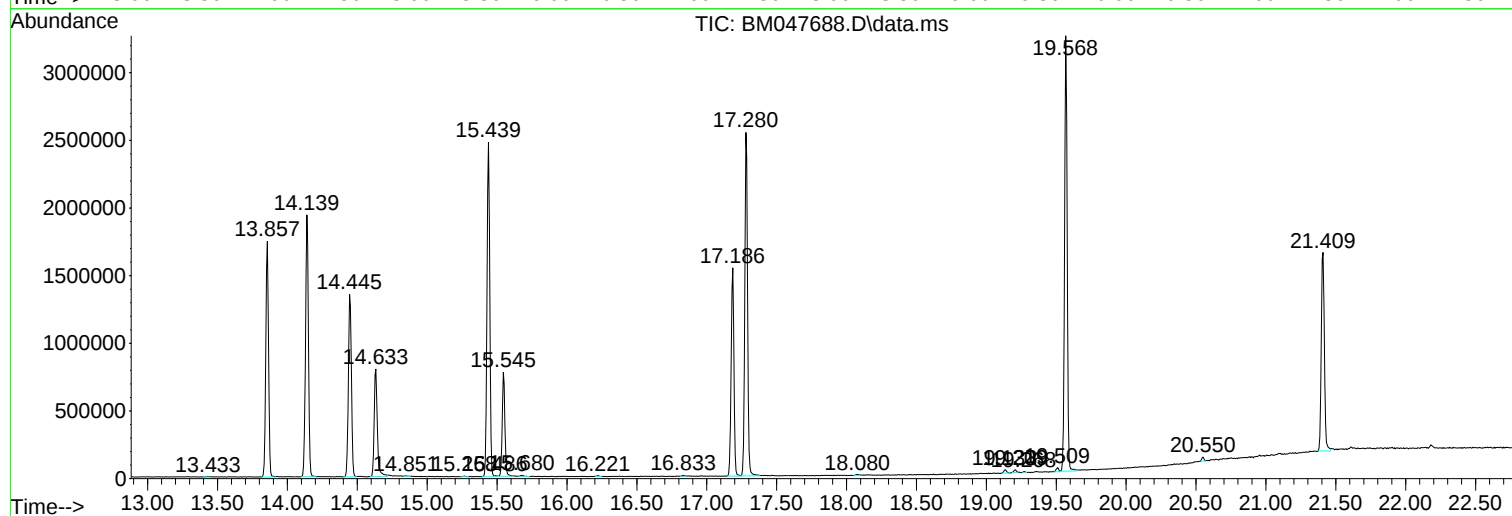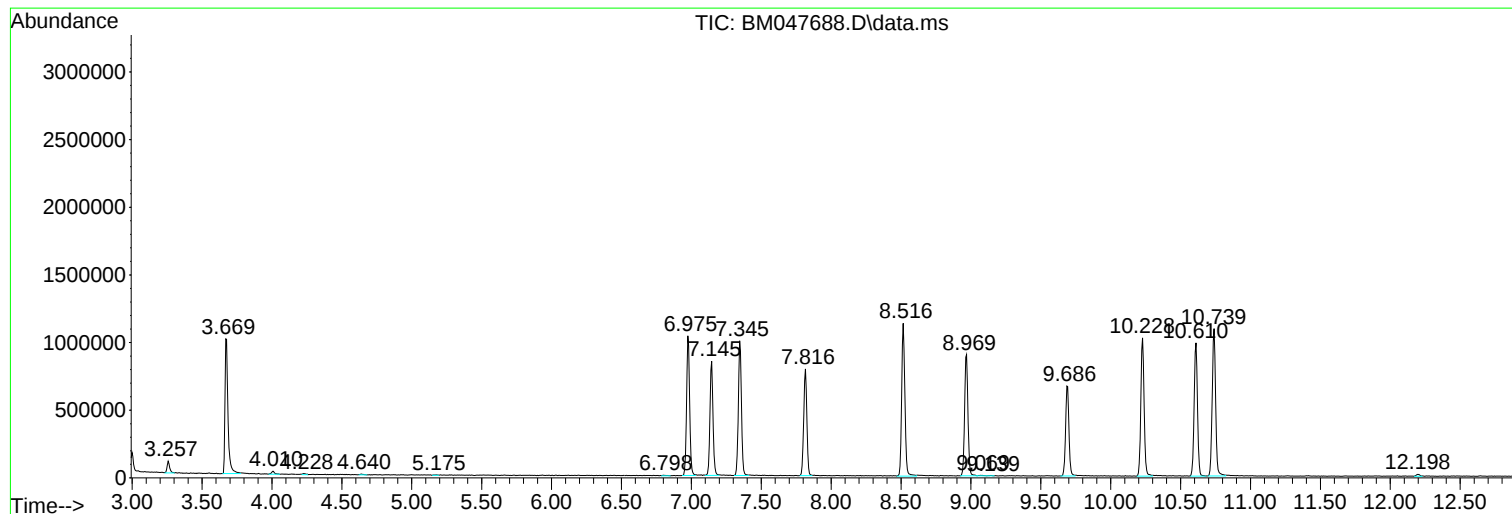

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
Data File : BM047688.D
Acq On : 28 Sep 2024 12:44
Operator : RC/JU
Sample : PB163765BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK765

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092824\
Data File : BM047688.D
Acq On : 28 Sep 2024 12:44
Operator : RC/JU
Sample : PB163765BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK765

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------